

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059548.D
 Acq On : 27 Jun 2024 09:23
 Operator : MD/SY
 Sample : VU0627WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	109	rBV	69214	85048	14.30%	1.790%
2	1.756	138	145	149	rBV3	4123	5425	0.91%	0.114%
3	1.907	183	192	212	rVB	59169	81910	13.77%	1.724%
4	1.994	217	219	223	rBV2	655	358	0.06%	0.008%
5	2.560	383	395	410	rBV	116759	189267	31.82%	3.983%
6	2.788	458	466	477	rVB	1384	2452	0.41%	0.052%
7	3.039	533	544	555	rBV3	5326	10166	1.71%	0.214%
8	3.177	580	587	593	rBV3	444	741	0.12%	0.016%
9	3.351	634	641	651	rVB2	1256	2035	0.34%	0.043%
10	3.563	702	707	713	rBV	239	222	0.04%	0.005%
11	3.634	724	729	735	rVB2	138	180	0.03%	0.004%
12	3.779	769	774	778	rBV2	151	182	0.03%	0.004%
13	3.914	811	816	818	rBV2	192	172	0.03%	0.004%
14	4.007	838	845	848	rBV2	266	277	0.05%	0.006%
15	4.033	848	853	856	rBV	197	164	0.03%	0.003%
16	4.229	911	914	923	rVB	284	269	0.05%	0.006%
17	4.274	924	928	933	rVB2	322	320	0.05%	0.007%
18	4.312	935	940	944	rBV2	325	459	0.08%	0.010%
19	4.467	985	988	992	rBV2	261	177	0.03%	0.004%
20	4.611	1024	1033	1065	rBV	55600	142297	23.92%	2.995%
21	4.975	1143	1146	1149	rVB2	308	190	0.03%	0.004%
22	5.055	1155	1171	1193	rBV	110193	244667	41.14%	5.149%
23	5.177	1206	1209	1212	rBV2	316	155	0.03%	0.003%
24	5.213	1217	1220	1223	rVB2	376	237	0.04%	0.005%
25	5.235	1223	1227	1234	rBV3	336	420	0.07%	0.009%
26	5.287	1239	1243	1247	rBV2	230	171	0.03%	0.004%
27	5.377	1267	1271	1273	rBV	358	286	0.05%	0.006%
28	5.717	1357	1377	1403	rBV3	217669	594774	100.00%	12.518%
29	5.840	1412	1415	1418	rVB2	544	346	0.06%	0.007%
30	6.013	1465	1469	1473	rBV2	324	299	0.05%	0.006%
31	6.242	1527	1540	1561	rBV	209825	407363	68.49%	8.574%
32	6.457	1603	1607	1609	rBV	247	223	0.04%	0.005%
33	6.531	1621	1630	1645	rVB7	2759	5798	0.97%	0.122%
34	6.682	1664	1677	1698	rBV	136142	269658	45.34%	5.675%
35	6.991	1767	1773	1777	rBV2	214	235	0.04%	0.005%
36	7.107	1805	1809	1812	rBV2	690	534	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059548.D
 Acq On : 27 Jun 2024 09:23
 Operator : MD/SY
 Sample : VU0627WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.171	1825	1829	1833	rVB2	202	156	0.03%	0.003%
38	7.200	1833	1838	1841	rBV2	337	393	0.07%	0.008%
39	7.232	1845	1848	1851	rVB	232	153	0.03%	0.003%
40	7.277	1858	1862	1868	rBV2	184	207	0.03%	0.004%
41	7.563	1939	1951	1974	rBV2	64578	120474	20.26%	2.536%
42	7.672	1983	1985	1990	rVB2	337	220	0.04%	0.005%
43	7.698	1990	1993	1996	rVB2	222	181	0.03%	0.004%
44	7.795	2020	2023	2026	rBV	294	219	0.04%	0.005%
45	7.894	2041	2054	2073	rBV	245603	434327	73.02%	9.141%
46	8.177	2131	2142	2163	rBV	46618	82870	13.93%	1.744%
47	8.402	2206	2212	2219	rVV3	495	626	0.11%	0.013%
48	8.434	2219	2222	2229	rVB	181	213	0.04%	0.004%
49	8.476	2230	2235	2236	rBV	206	166	0.03%	0.003%
50	8.550	2252	2258	2265	rBV4	1385	1780	0.30%	0.037%
51	8.627	2270	2282	2313	rBV	142167	285031	47.92%	5.999%
52	8.788	2330	2332	2336	rVB3	373	311	0.05%	0.007%
53	8.843	2346	2349	2353	rVB2	242	154	0.03%	0.003%
54	8.917	2369	2372	2377	rVB2	559	441	0.07%	0.009%
55	9.087	2420	2425	2428	rBV2	223	210	0.04%	0.004%
56	9.412	2514	2526	2568	rBV	314556	544047	91.47%	11.450%
57	9.566	2568	2574	2575	rBV2	1451	1055	0.18%	0.022%
58	9.627	2590	2593	2597	rVB2	246	158	0.03%	0.003%
59	9.695	2609	2614	2615	rBV3	871	750	0.13%	0.016%
60	9.904	2675	2679	2686	rVB2	193	231	0.04%	0.005%
61	9.942	2687	2691	2694	rBV2	166	171	0.03%	0.004%
62	9.981	2699	2703	2707	rBV2	187	161	0.03%	0.003%
63	10.110	2737	2743	2744	rBV3	568	540	0.09%	0.011%
64	10.174	2760	2763	2769	rVB2	208	210	0.04%	0.004%
65	10.238	2779	2783	2786	rBV	268	188	0.03%	0.004%
66	10.290	2795	2799	2803	rVB2	365	323	0.05%	0.007%
67	10.489	2853	2861	2864	rBV2	859	1140	0.19%	0.024%
68	10.576	2881	2888	2890	rBV2	258	292	0.05%	0.006%
69	10.653	2909	2912	2915	rVB2	239	153	0.03%	0.003%
70	10.749	2930	2942	2961	rBV	209521	344466	57.92%	7.250%
71	10.891	2983	2986	2990	rBV	325	181	0.03%	0.004%
72	10.936	2995	3000	3001	rBV	292	194	0.03%	0.004%
73	11.090	3043	3048	3053	rBV3	611	566	0.10%	0.012%
74	11.347	3125	3128	3134	rVB2	418	388	0.07%	0.008%
75	11.376	3134	3137	3139	rBV2	366	303	0.05%	0.006%
76	11.473	3160	3167	3179	rVB2	981	1518	0.26%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059548.D
 Acq On : 27 Jun 2024 09:23
 Operator : MD/SY
 Sample : VU0627WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.688	3232	3234	3240	rVB	356	298	0.05%	0.006%
78	11.740	3245	3250	3260	rBV6	1665	2612	0.44%	0.055%
79	11.807	3260	3271	3295	rVV	275874	456516	76.75%	9.608%
80	12.068	3349	3352	3361	rVB2	252	380	0.06%	0.008%
81	12.190	3378	3390	3410	rBV2	239818	400004	67.25%	8.419%
82	12.843	3591	3593	3596	rVB	328	172	0.03%	0.004%
83	12.984	3633	3637	3642	rBV2	358	453	0.08%	0.010%
84	13.010	3642	3645	3653	rVB3	496	546	0.09%	0.011%
85	13.103	3669	3674	3676	rBV	375	278	0.05%	0.006%
86	13.232	3708	3714	3721	rBV5	1312	1850	0.31%	0.039%
87	13.373	3755	3758	3761	rBV	241	157	0.03%	0.003%
88	13.852	3899	3907	3916	rBV5	1954	3148	0.53%	0.066%
89	13.945	3933	3936	3938	rBV	251	174	0.03%	0.004%
90	14.068	3971	3974	3975	rBV	271	159	0.03%	0.003%
91	14.100	3978	3984	4000	rVV5	2955	5378	0.90%	0.113%
92	14.264	4033	4035	4039	rVB2	275	154	0.03%	0.003%
93	14.338	4049	4058	4068	rVB5	2217	3752	0.63%	0.079%
94	14.585	4132	4135	4138	rBV	302	249	0.04%	0.005%
95	14.798	4199	4201	4205	rVB2	486	204	0.03%	0.004%
96	15.318	4360	4363	4366	rBV	389	285	0.05%	0.006%
97	15.791	4507	4510	4514	rBV3	483	301	0.05%	0.006%
98	16.051	4587	4591	4594	rBV2	797	663	0.11%	0.014%
99	16.460	4715	4718	4719	rBV3	670	421	0.07%	0.009%
100	16.904	4854	4856	4860	rBV3	892	574	0.10%	0.012%




Sum of corrected areas: 4751372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059548.D
Acq On : 27 Jun 2024 09:23
Operator : MD/SY
Sample : VU0627WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

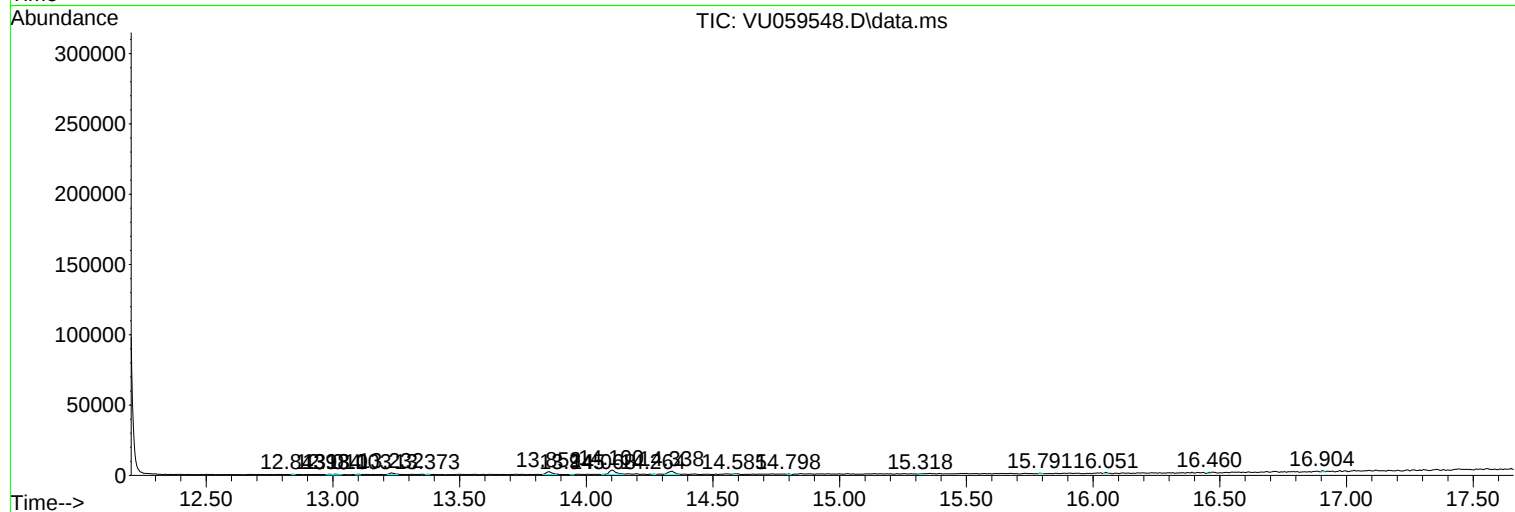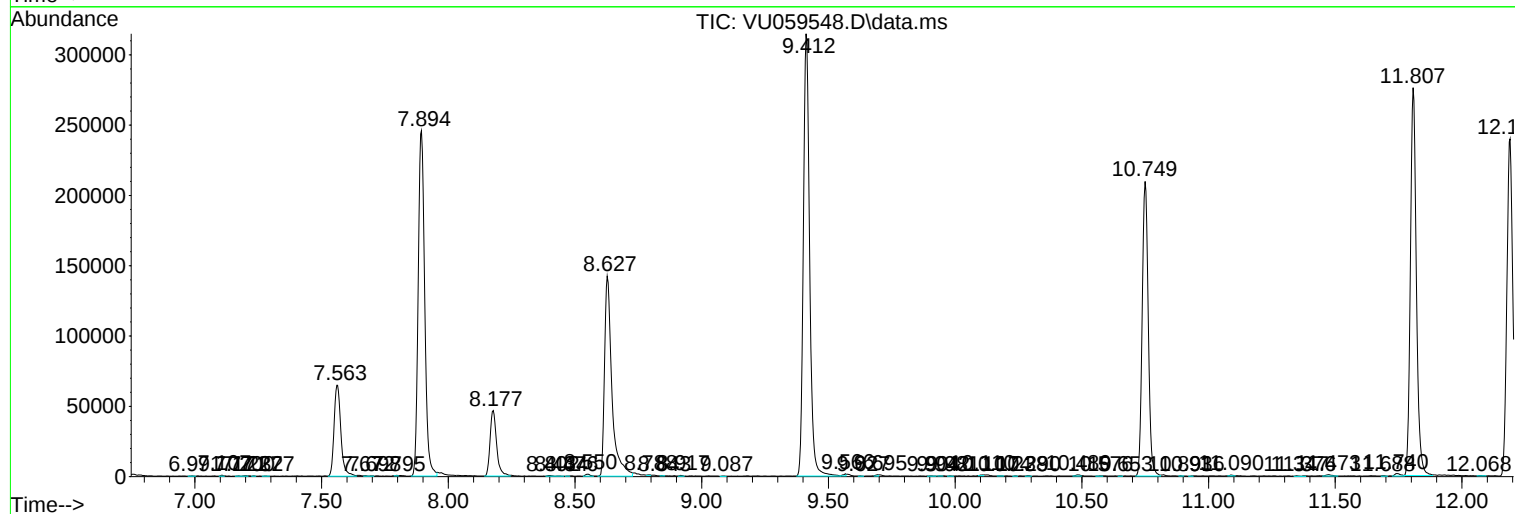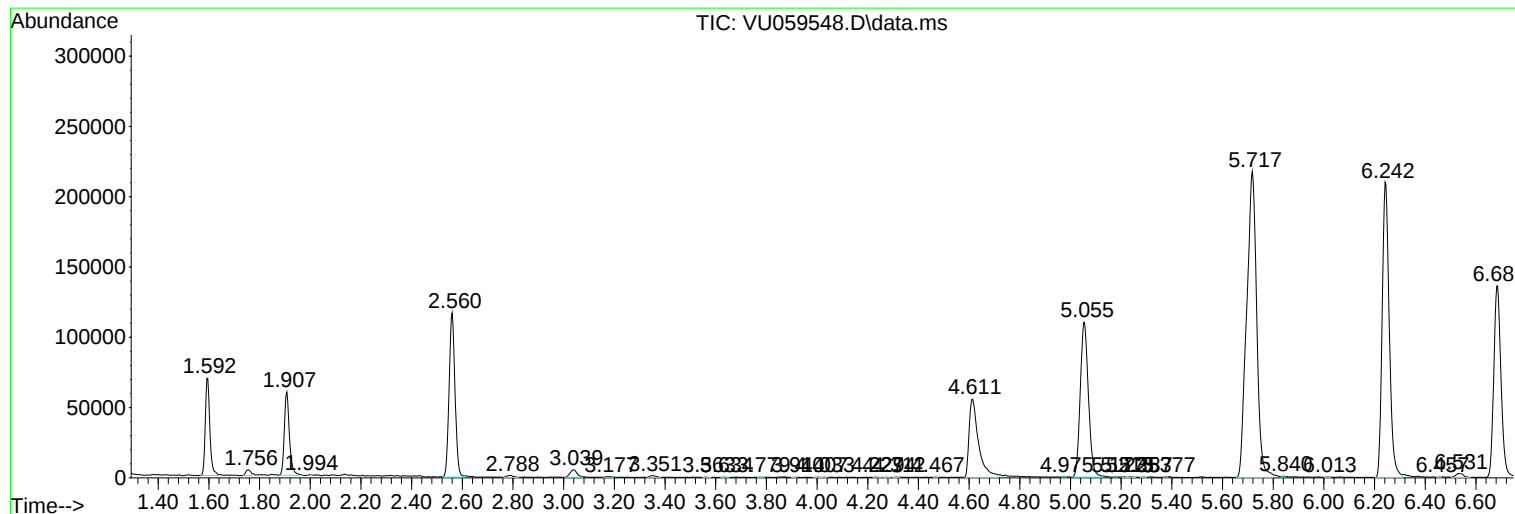

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059548.D
Acq On : 27 Jun 2024 09:23
Operator : MD/SY
Sample : VU0627WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059548.D
Acq On : 27 Jun 2024 09:23
Operator : MD/SY
Sample : VU0627WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------