

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059549.D
 Acq On : 27 Jun 2024 09:46
 Operator : MD/SY
 Sample : P3037-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rBV	70593	86395	14.49%	1.803%
2	1.763	138	147	153	rBV3	4209	6368	1.07%	0.133%
3	1.908	184	192	212	rBV	57291	81429	13.66%	1.699%
4	2.210	284	286	287	rBV2	477	187	0.03%	0.004%
5	2.258	299	301	306	rBV3	662	441	0.07%	0.009%
6	2.374	334	337	339	rBV3	629	391	0.07%	0.008%
7	2.412	346	349	352	rBV2	619	414	0.07%	0.009%
8	2.560	382	395	412	rBV	112170	187282	31.41%	3.907%
9	2.785	458	465	474	rVB3	999	1817	0.30%	0.038%
10	2.956	514	518	522	rVB3	250	210	0.04%	0.004%
11	2.978	522	525	528	rBV	213	147	0.02%	0.003%
12	3.039	535	544	555	rBV4	2519	4846	0.81%	0.101%
13	3.171	579	585	602	rVB4	887	2131	0.36%	0.044%
14	3.242	602	607	608	rBV	233	196	0.03%	0.004%
15	3.280	616	619	621	rBV	211	138	0.02%	0.003%
16	3.348	634	640	641	rBV4	899	746	0.13%	0.016%
17	3.509	687	690	693	rBV2	207	146	0.02%	0.003%
18	3.570	703	709	711	rBV	164	189	0.03%	0.004%
19	3.833	787	791	795	rBV2	148	140	0.02%	0.003%
20	3.866	798	801	802	rBV	184	134	0.02%	0.003%
21	3.933	820	822	828	rVB2	193	174	0.03%	0.004%
22	4.091	868	871	875	rVB2	216	156	0.03%	0.003%
23	4.232	912	915	921	rVB2	415	476	0.08%	0.010%
24	4.261	921	924	926	rBV2	418	256	0.04%	0.005%
25	4.451	979	983	987	rVB2	195	159	0.03%	0.003%
26	4.477	987	991	994	rBV	177	188	0.03%	0.004%
27	4.612	1024	1033	1062	rBV	59989	152770	25.62%	3.187%
28	5.055	1156	1171	1191	rBV	110183	244132	40.95%	5.093%
29	5.296	1243	1246	1250	rVV2	383	374	0.06%	0.008%
30	5.380	1266	1272	1273	rBV	464	384	0.06%	0.008%
31	5.435	1286	1289	1294	rVV2	196	194	0.03%	0.004%
32	5.518	1312	1315	1318	rVB3	273	161	0.03%	0.003%
33	5.615	1340	1345	1347	rBV2	162	152	0.03%	0.003%
34	5.718	1357	1377	1404	rBV2	212849	596242	100.00%	12.440%
35	5.920	1434	1440	1442	rBV	325	314	0.05%	0.007%
36	6.129	1501	1505	1509	rBV2	280	264	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059549.D
 Acq On : 27 Jun 2024 09:46
 Operator : MD/SY
 Sample : P3037-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.161	1513	1515	1521	rVB2	260	217	0.04%	0.005%
38	6.242	1527	1540	1567	rBV	210105	410514	68.85%	8.565%
39	6.454	1604	1606	1609	rBV	238	160	0.03%	0.003%
40	6.531	1618	1630	1639	rBV8	2574	5323	0.89%	0.111%
41	6.685	1664	1678	1696	rBV	137477	272455	45.70%	5.684%
42	6.904	1743	1746	1749	rBV	201	138	0.02%	0.003%
43	7.017	1777	1781	1783	rBV	381	208	0.03%	0.004%
44	7.103	1802	1808	1812	rBV3	411	397	0.07%	0.008%
45	7.145	1816	1821	1822	rBV	209	155	0.03%	0.003%
46	7.300	1865	1869	1872	rBV	213	241	0.04%	0.005%
47	7.370	1887	1891	1894	rBV	161	151	0.03%	0.003%
48	7.560	1939	1950	1978	rBV	67210	123272	20.67%	2.572%
49	7.763	2009	2013	2019	rBV2	239	263	0.04%	0.005%
50	7.792	2019	2022	2033	rVB3	771	1195	0.20%	0.025%
51	7.894	2041	2054	2074	rBV	243688	433668	72.73%	9.048%
52	8.068	2105	2108	2115	rBV2	141	197	0.03%	0.004%
53	8.119	2121	2124	2127	rBV3	211	139	0.02%	0.003%
54	8.177	2131	2142	2161	rVV2	47546	85239	14.30%	1.778%
55	8.402	2206	2212	2216	rVB4	443	511	0.09%	0.011%
56	8.550	2253	2258	2264	rVB5	1088	1327	0.22%	0.028%
57	8.628	2272	2282	2324	rBV	155321	313600	52.60%	6.543%
58	8.914	2367	2371	2375	rBV4	536	621	0.10%	0.013%
59	9.004	2393	2399	2402	rBV2	153	175	0.03%	0.004%
60	9.026	2402	2406	2412	rBV2	153	194	0.03%	0.004%
61	9.216	2462	2465	2469	rVB2	190	153	0.03%	0.003%
62	9.412	2513	2526	2558	rBV	317572	541422	90.81%	11.296%
63	9.573	2569	2576	2578	rBV2	979	952	0.16%	0.020%
64	9.695	2607	2614	2616	rBV2	881	869	0.15%	0.018%
65	10.107	2733	2742	2744	rBV4	781	884	0.15%	0.018%
66	10.483	2853	2859	2869	rVB3	1000	1582	0.27%	0.033%
67	10.528	2869	2873	2880	rBV2	212	247	0.04%	0.005%
68	10.750	2929	2942	2959	rBV	218649	356434	59.78%	7.437%
69	10.891	2983	2986	2988	rBV	210	138	0.02%	0.003%
70	10.994	3015	3018	3020	rBV	292	220	0.04%	0.005%
71	11.248	3093	3097	3103	rBV2	247	291	0.05%	0.006%
72	11.412	3145	3148	3152	rBV2	178	191	0.03%	0.004%
73	11.470	3163	3166	3170	rBV3	456	395	0.07%	0.008%
74	11.746	3247	3252	3260	rVB	1598	1749	0.29%	0.036%
75	11.807	3260	3271	3297	rBV	274037	455695	76.43%	9.507%
76	12.020	3335	3337	3342	rVB3	458	284	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059549.D
 Acq On : 27 Jun 2024 09:46
 Operator : MD/SY
 Sample : P3037-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.187	3377	3389	3408	rBV	235402	399809	67.05%	8.341%
78	12.332	3433	3434	3437	rVB	443	143	0.02%	0.003%
79	12.357	3437	3442	3447	rBV2	328	297	0.05%	0.006%
80	12.380	3447	3449	3450	rBV2	310	134	0.02%	0.003%
81	12.573	3506	3509	3513	rBV2	316	308	0.05%	0.006%
82	12.920	3614	3617	3621	rBV2	246	209	0.04%	0.004%
83	13.004	3641	3643	3647	rVB	269	138	0.02%	0.003%
84	13.354	3748	3752	3756	rVB2	346	327	0.05%	0.007%
85	13.463	3784	3786	3789	rBV	224	131	0.02%	0.003%
86	13.846	3900	3905	3920	rVB4	1040	1790	0.30%	0.037%
87	14.026	3958	3961	3968	rBV2	304	387	0.06%	0.008%
88	14.106	3979	3986	3998	rBV4	1546	2980	0.50%	0.062%
89	14.325	4050	4054	4056	rBV2	600	542	0.09%	0.011%
90	14.563	4125	4128	4134	rVB2	515	512	0.09%	0.011%
91	14.592	4134	4137	4139	rBV2	257	164	0.03%	0.003%
92	14.659	4155	4158	4162	rVB2	394	265	0.04%	0.006%
93	14.685	4163	4166	4171	rBV3	480	380	0.06%	0.008%
94	14.759	4187	4189	4193	rVB3	317	226	0.04%	0.005%
95	14.901	4230	4233	4241	rBV4	612	848	0.14%	0.018%
96	14.971	4253	4255	4257	rBV	314	169	0.03%	0.004%
97	15.045	4275	4278	4280	rBV2	423	269	0.05%	0.006%
98	15.608	4451	4453	4456	rVB3	404	211	0.04%	0.004%
99	16.190	4630	4634	4636	rBV3	629	518	0.09%	0.011%
100	16.331	4676	4678	4681	rBV	580	257	0.04%	0.005%




Sum of corrected areas: 4793023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059549.D
Acq On : 27 Jun 2024 09:46
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

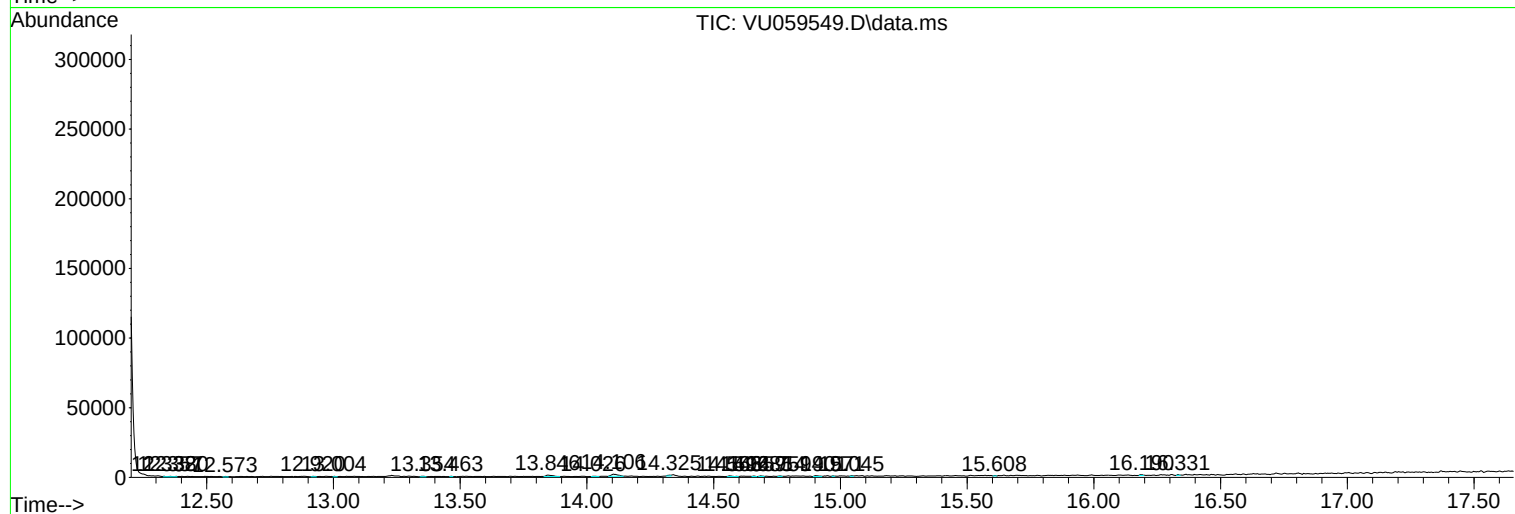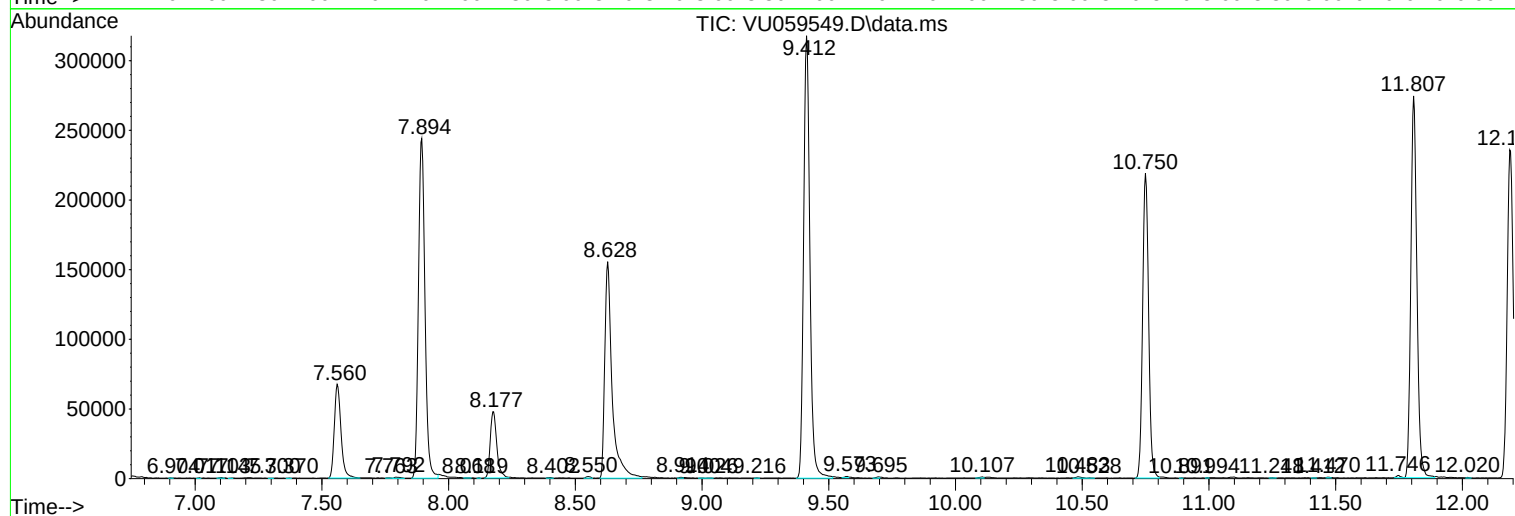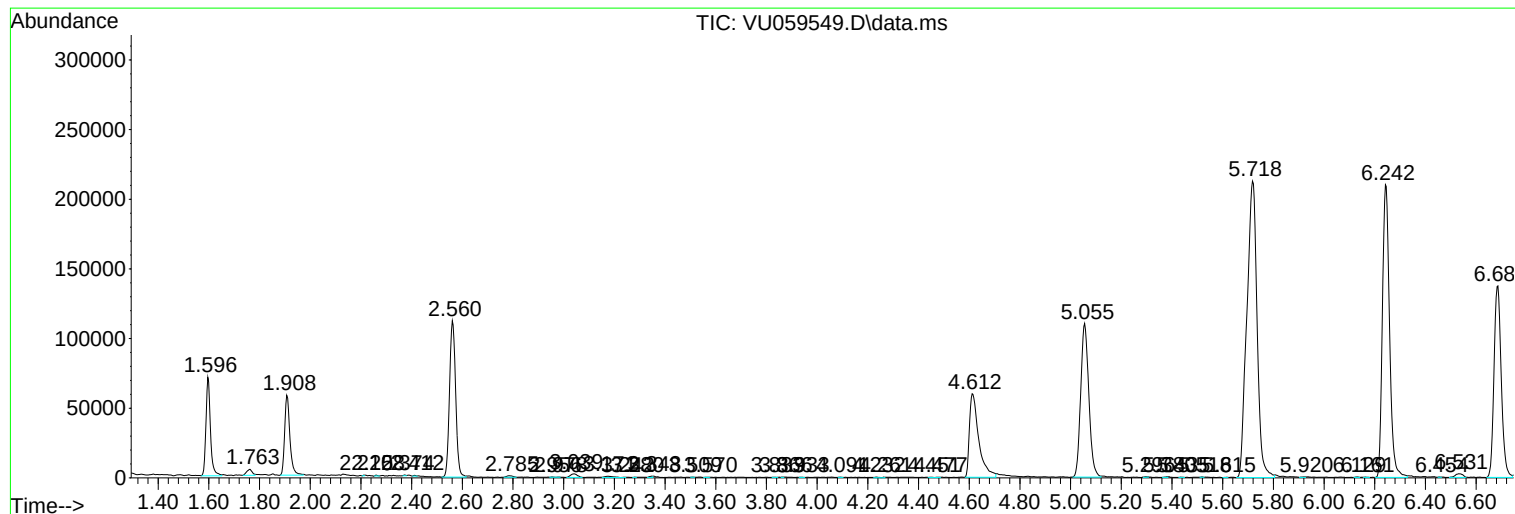

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059549.D
Acq On : 27 Jun 2024 09:46
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059549.D
Acq On : 27 Jun 2024 09:46
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------