

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059550.D
 Acq On : 27 Jun 2024 10:09
 Operator : MD/SY
 Sample : P3081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.354	16	20	31	rBV3	3423	4669	0.73%	0.094%
2	1.596	88	95	112	rVB	79668	96273	15.08%	1.930%
3	1.907	184	192	208	rBV	62364	88104	13.80%	1.766%
4	2.496	373	375	381	rBV2	295	208	0.03%	0.004%
5	2.560	383	395	409	rBV	125315	205483	32.19%	4.119%
6	2.705	437	440	444	rBV2	183	139	0.02%	0.003%
7	2.753	444	455	460	rBV4	1456	2758	0.43%	0.055%
8	2.862	486	489	492	rBV	160	125	0.02%	0.003%
9	3.039	536	544	556	rBV3	1948	3581	0.56%	0.072%
10	3.132	570	573	575	rBV2	201	136	0.02%	0.003%
11	3.177	575	587	598	rVV2	3103	6340	0.99%	0.127%
12	3.293	620	623	628	rBV	150	127	0.02%	0.003%
13	3.322	629	632	634	rVV2	173	119	0.02%	0.002%
14	3.335	634	636	640	rVB	276	137	0.02%	0.003%
15	3.454	669	673	677	rVB2	166	117	0.02%	0.002%
16	3.525	691	695	700	rBV	362	311	0.05%	0.006%
17	3.753	761	766	769	rBV	130	156	0.02%	0.003%
18	3.804	779	782	786	rBV	198	117	0.02%	0.002%
19	3.827	786	789	791	rBV	161	116	0.02%	0.002%
20	3.894	803	810	813	rBV2	180	248	0.04%	0.005%
21	3.959	821	830	833	rBV2	259	335	0.05%	0.007%
22	3.994	839	841	843	rVB2	184	72	0.01%	0.001%
23	4.010	843	846	850	rBV2	160	152	0.02%	0.003%
24	4.187	896	901	903	rBV2	155	142	0.02%	0.003%
25	4.226	910	913	917	rBV2	183	136	0.02%	0.003%
26	4.293	930	934	937	rBV	244	177	0.03%	0.004%
27	4.493	993	996	997	rBV2	128	76	0.01%	0.002%
28	4.615	1021	1034	1061	rBV	58704	152792	23.93%	3.063%
29	5.055	1156	1171	1190	rBV2	116836	259259	40.61%	5.197%
30	5.229	1223	1225	1228	rVB2	214	79	0.01%	0.002%
31	5.364	1262	1267	1269	rBV	219	162	0.03%	0.003%
32	5.374	1269	1270	1274	rVB2	205	78	0.01%	0.002%
33	5.393	1274	1276	1277	rBV	168	70	0.01%	0.001%
34	5.425	1283	1286	1289	rVB	244	125	0.02%	0.003%
35	5.489	1305	1306	1308	rVB	257	89	0.01%	0.002%
36	5.521	1312	1316	1318	rBV	150	118	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059550.D
 Acq On : 27 Jun 2024 10:09
 Operator : MD/SY
 Sample : P3081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.554	1323	1326	1330	rBV	116	64	0.01%	0.001%
38	5.586	1330	1336	1339	rBV2	166	167	0.03%	0.003%
39	5.602	1339	1341	1346	rBB2	152	102	0.02%	0.002%
40	5.628	1346	1349	1354	rBV2	135	125	0.02%	0.003%
41	5.718	1357	1377	1405	rBV2	235365	638408	100.00%	12.797%
42	6.042	1474	1478	1479	rBV	230	141	0.02%	0.003%
43	6.136	1505	1507	1515	rBV2	352	277	0.04%	0.006%
44	6.174	1517	1519	1522	rBV2	93	62	0.01%	0.001%
45	6.242	1528	1540	1566	rBV	228802	442381	69.29%	8.868%
46	6.534	1622	1631	1645	rVB8	2239	4468	0.70%	0.090%
47	6.589	1645	1648	1649	rBV	241	154	0.02%	0.003%
48	6.682	1663	1677	1699	rBV	145753	290204	45.46%	5.817%
49	6.865	1730	1734	1736	rBV2	191	155	0.02%	0.003%
50	6.972	1763	1767	1768	rBV	134	92	0.01%	0.002%
51	7.097	1801	1806	1807	rBV3	794	586	0.09%	0.012%
52	7.139	1817	1819	1821	rBV	116	73	0.01%	0.001%
53	7.177	1829	1831	1833	rBV	114	54	0.01%	0.001%
54	7.193	1833	1836	1838	rBV	373	279	0.04%	0.006%
55	7.245	1849	1852	1856	rVB	124	86	0.01%	0.002%
56	7.309	1869	1872	1878	rVB2	201	199	0.03%	0.004%
57	7.341	1879	1882	1885	rVB2	145	84	0.01%	0.002%
58	7.367	1885	1890	1892	rBV	147	123	0.02%	0.002%
59	7.428	1907	1909	1911	rBV	121	53	0.01%	0.001%
60	7.512	1931	1935	1937	rBV	201	128	0.02%	0.003%
61	7.560	1940	1950	1970	rBV2	61716	109799	17.20%	2.201%
62	7.701	1991	1994	1999	rBV3	476	472	0.07%	0.009%
63	7.785	2017	2020	2023	rBV2	216	166	0.03%	0.003%
64	7.808	2023	2027	2031	rVB3	327	262	0.04%	0.005%
65	7.827	2031	2033	2039	rBV	171	148	0.02%	0.003%
66	7.894	2041	2054	2072	rBV	264143	471192	73.81%	9.445%
67	8.087	2111	2114	2117	rBV2	212	155	0.02%	0.003%
68	8.177	2132	2142	2162	rBV2	41203	71095	11.14%	1.425%
69	8.412	2212	2215	2217	rBV2	97	72	0.01%	0.001%
70	8.441	2222	2224	2225	rBV	225	121	0.02%	0.002%
71	8.463	2227	2231	2232	rBV2	1089	784	0.12%	0.016%
72	8.521	2246	2249	2250	rBV	122	66	0.01%	0.001%
73	8.547	2255	2257	2260	rBV2	535	417	0.07%	0.008%
74	8.589	2267	2270	2272	rBV2	155	104	0.02%	0.002%
75	8.627	2272	2282	2319	rBV3	147982	304339	47.67%	6.101%
76	8.978	2388	2391	2393	rBV2	97	73	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059550.D
 Acq On : 27 Jun 2024 10:09
 Operator : MD/SY
 Sample : P3081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	9.010	2398	2401	2404	rBV2	139	100	0.02%	0.002%
78	9.319	2495	2497	2500	rBV2	140	78	0.01%	0.002%
79	9.412	2513	2526	2556	rBV	330724	566243	88.70%	11.351%
80	9.563	2571	2573	2575	rBV	461	245	0.04%	0.005%
81	9.595	2581	2583	2587	rVB	170	93	0.01%	0.002%
82	9.685	2607	2611	2612	rBV2	428	238	0.04%	0.005%
83	9.759	2631	2634	2638	rVB2	246	154	0.02%	0.003%
84	9.830	2652	2656	2659	rBV	287	286	0.04%	0.006%
85	9.904	2674	2679	2682	rBV2	303	338	0.05%	0.007%
86	10.049	2721	2724	2725	rBV	224	124	0.02%	0.002%
87	10.100	2732	2740	2751	rBV2	3556	5078	0.80%	0.102%
88	10.489	2857	2861	2864	rVB3	299	278	0.04%	0.006%
89	10.512	2864	2868	2875	rBV2	267	304	0.05%	0.006%
90	10.692	2923	2924	2927	rBV2	189	97	0.02%	0.002%
91	10.750	2930	2942	2964	rVV	225913	364608	57.11%	7.309%
92	10.888	2980	2985	2996	rVB4	2220	2814	0.44%	0.056%
93	11.094	3046	3049	3051	rBV	188	112	0.02%	0.002%
94	11.267	3101	3103	3104	rBV	243	93	0.01%	0.002%
95	11.807	3259	3271	3292	rBV	283545	470155	73.64%	9.425%
96	12.026	3337	3339	3342	rVB	259	109	0.02%	0.002%
97	12.116	3365	3367	3371	rVB2	344	211	0.03%	0.004%
98	12.187	3377	3389	3414	rBV	249025	415473	65.08%	8.328%
99	12.991	3637	3639	3645	rVB2	307	235	0.04%	0.005%
100	15.521	4423	4426	4427	rBV	490	292	0.05%	0.006%




Sum of corrected areas: 4988614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059550.D
Acq On : 27 Jun 2024 10:09
Operator : MD/SY
Sample : P3081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

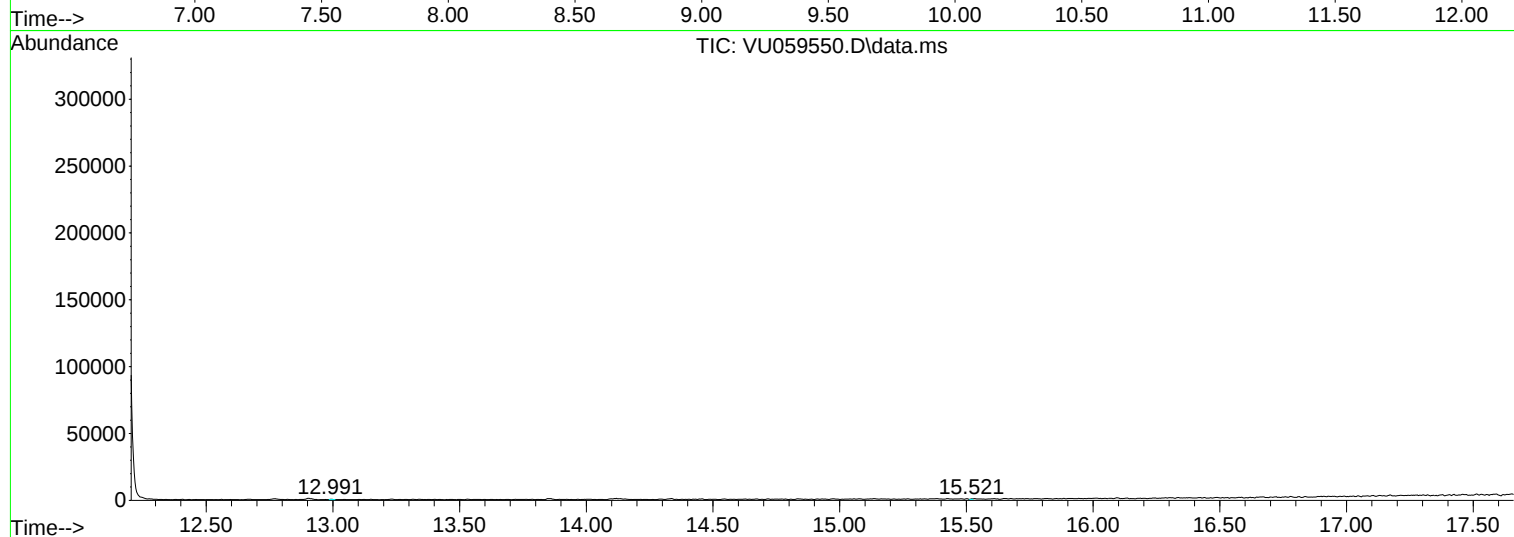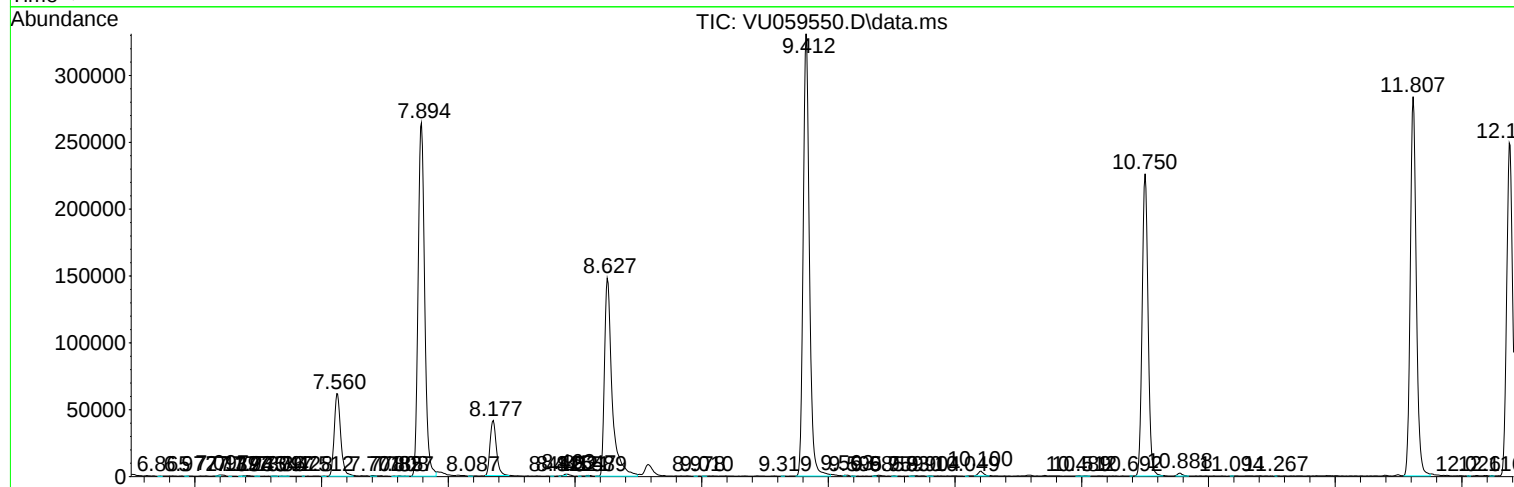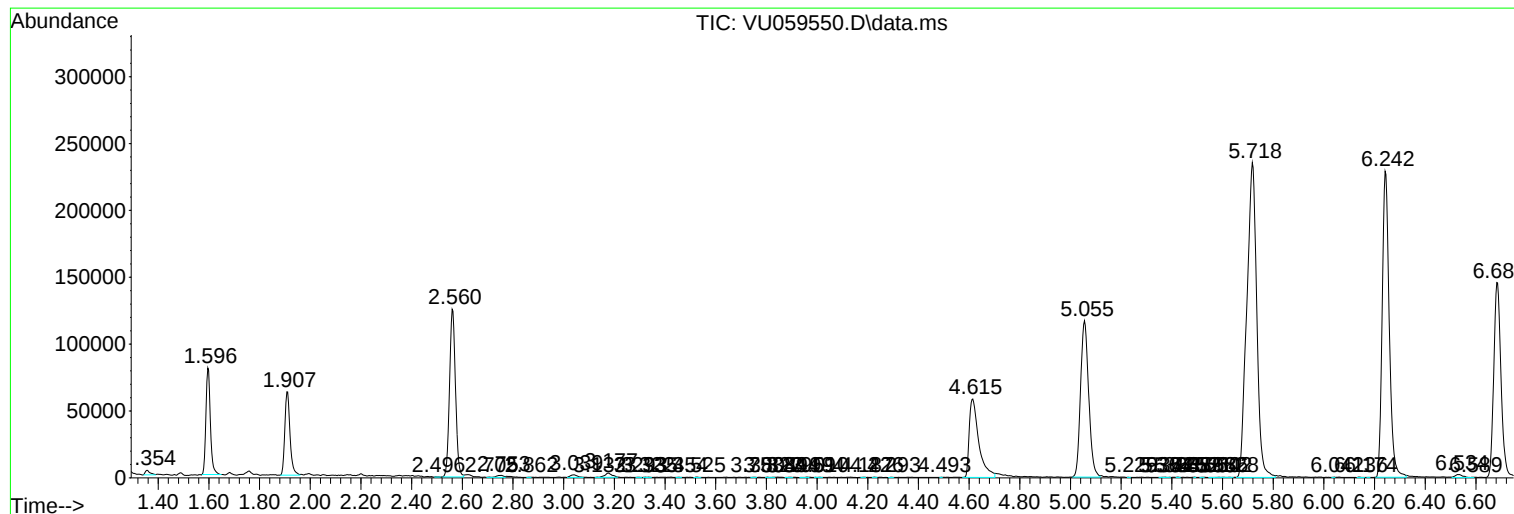

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059550.D
Acq On : 27 Jun 2024 10:09
Operator : MD/SY
Sample : P3081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059550.D
Acq On : 27 Jun 2024 10:09
Operator : MD/SY
Sample : P3081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc