

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059558.D
 Acq On : 27 Jun 2024 13:10
 Operator : MD/SY
 Sample : P3055-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	114	rVV	80505	100297	15.16%	1.869%
2	1.682	117	122	128	rVB3	3084	3347	0.51%	0.062%
3	1.760	138	146	152	rBV3	4133	6684	1.01%	0.125%
4	1.907	183	192	216	rBV	63116	91615	13.85%	1.708%
5	2.258	299	301	304	rBV2	481	329	0.05%	0.006%
6	2.560	383	395	408	rBV	128023	209433	31.66%	3.904%
7	2.618	408	413	425	rVB	4684	7666	1.16%	0.143%
8	2.750	446	454	458	rBV4	751	980	0.15%	0.018%
9	2.821	473	476	479	rVB2	336	218	0.03%	0.004%
10	2.840	479	482	484	rBV	195	143	0.02%	0.003%
11	3.039	535	544	557	rVB3	2535	4951	0.75%	0.092%
12	3.171	573	585	596	rVV4	1692	3986	0.60%	0.074%
13	3.219	596	600	605	rVB2	300	337	0.05%	0.006%
14	3.248	606	609	614	rBV2	160	158	0.02%	0.003%
15	3.348	634	640	649	rVB5	1051	1506	0.23%	0.028%
16	3.682	739	744	746	rVB2	194	159	0.02%	0.003%
17	3.698	746	749	754	rBV2	194	149	0.02%	0.003%
18	3.785	773	776	780	rBV2	164	162	0.02%	0.003%
19	3.859	793	799	807	rBV2	274	418	0.06%	0.008%
20	3.894	807	810	816	rVB2	161	177	0.03%	0.003%
21	3.959	827	830	833	rBV2	222	186	0.03%	0.003%
22	4.052	855	859	862	rBV2	206	168	0.03%	0.003%
23	4.094	867	872	876	rBV2	219	257	0.04%	0.005%
24	4.380	955	961	966	rBV2	221	231	0.03%	0.004%
25	4.422	970	974	976	rBV2	527	490	0.07%	0.009%
26	4.612	1023	1033	1062	rBV	63803	157956	23.88%	2.944%
27	5.055	1153	1171	1198	rBV2	123544	304238	45.99%	5.671%
28	5.184	1208	1211	1215	rVB3	322	222	0.03%	0.004%
29	5.229	1222	1225	1228	rVB2	260	160	0.02%	0.003%
30	5.284	1236	1242	1245	rBV	242	235	0.04%	0.004%
31	5.338	1256	1259	1262	rVB	242	140	0.02%	0.003%
32	5.386	1268	1274	1283	rVB2	306	559	0.08%	0.010%
33	5.425	1283	1286	1290	rBV	231	265	0.04%	0.005%
34	5.447	1290	1293	1298	rBV2	198	190	0.03%	0.004%
35	5.486	1302	1305	1310	rVB	215	161	0.02%	0.003%
36	5.718	1356	1377	1407	rBV3	240084	661538	100.00%	12.330%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059558.D
 Acq On : 27 Jun 2024 13:10
 Operator : MD/SY
 Sample : P3055-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.984	1457	1460	1467	rVB2	198	221	0.03%	0.004%
38	6.039	1475	1477	1481	rBV2	339	249	0.04%	0.005%
39	6.071	1484	1487	1490	rVB2	226	140	0.02%	0.003%
40	6.132	1504	1506	1510	rBV2	316	153	0.02%	0.003%
41	6.242	1526	1540	1567	rBV	233220	459259	69.42%	8.560%
42	6.496	1615	1619	1622	rBV2	279	261	0.04%	0.005%
43	6.531	1622	1630	1641	rVB7	3142	5883	0.89%	0.110%
44	6.682	1663	1677	1698	rBV	152118	295803	44.71%	5.513%
45	6.801	1711	1714	1715	rBV3	313	179	0.03%	0.003%
46	6.891	1735	1742	1748	rBV2	241	431	0.07%	0.008%
47	7.103	1798	1808	1820	rBV5	2925	6380	0.96%	0.119%
48	7.190	1832	1835	1836	rBV	407	223	0.03%	0.004%
49	7.245	1849	1852	1856	rBV2	235	153	0.02%	0.003%
50	7.309	1866	1872	1874	rBV2	240	232	0.04%	0.004%
51	7.560	1938	1950	1973	rBV	75387	137763	20.82%	2.568%
52	7.717	1997	1999	2003	rVV2	349	230	0.03%	0.004%
53	7.737	2003	2005	2008	rVB	267	146	0.02%	0.003%
54	7.891	2040	2053	2071	rBV	283630	493880	74.66%	9.205%
55	8.087	2111	2114	2118	rVB2	289	213	0.03%	0.004%
56	8.174	2130	2141	2159	rBV2	52333	91181	13.78%	1.699%
57	8.332	2188	2190	2197	rVB2	264	220	0.03%	0.004%
58	8.470	2223	2233	2240	rBV2	1330	2207	0.33%	0.041%
59	8.550	2253	2258	2265	rVV4	823	831	0.13%	0.015%
60	8.627	2270	2282	2314	rBV	163931	324897	49.11%	6.056%
61	9.084	2421	2424	2428	rVB	193	151	0.02%	0.003%
62	9.184	2452	2455	2459	rVB2	223	150	0.02%	0.003%
63	9.209	2459	2463	2467	rBV2	185	193	0.03%	0.004%
64	9.322	2496	2498	2503	rVB2	307	183	0.03%	0.003%
65	9.412	2513	2526	2555	rBV	350858	594937	89.93%	11.089%
66	9.566	2571	2574	2585	rVB6	1063	1344	0.20%	0.025%
67	9.692	2606	2613	2625	rBV3	1803	2931	0.44%	0.055%
68	9.798	2641	2646	2651	rBV2	187	224	0.03%	0.004%
69	9.843	2658	2660	2665	rVB2	328	200	0.03%	0.004%
70	9.875	2666	2670	2676	rVB2	310	303	0.05%	0.006%
71	10.103	2733	2741	2743	rBV4	1012	1320	0.20%	0.025%
72	10.196	2767	2770	2776	rVB	287	203	0.03%	0.004%
73	10.261	2787	2790	2794	rBV2	323	292	0.04%	0.005%
74	10.309	2802	2805	2809	rBV2	263	183	0.03%	0.003%
75	10.483	2854	2859	2863	rVV3	294	377	0.06%	0.007%
76	10.573	2885	2887	2891	rVB	395	185	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059558.D
 Acq On : 27 Jun 2024 13:10
 Operator : MD/SY
 Sample : P3055-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.750	2930	2942	2964	rBV	231606	373355	56.44%	6.959%
78	10.827	2964	2966	2974	rVB3	437	480	0.07%	0.009%
79	10.888	2975	2985	2995	rBV2	1869	3231	0.49%	0.060%
80	11.479	3161	3169	3186	rBV6	4103	9009	1.36%	0.168%
81	11.740	3245	3250	3253	rBV2	977	938	0.14%	0.017%
82	11.807	3259	3271	3303	rBV	319680	533036	80.58%	9.935%
83	11.981	3323	3325	3328	rBV	340	172	0.03%	0.003%
84	12.187	3377	3389	3416	rBV	264769	445761	67.38%	8.308%
85	12.460	3471	3474	3479	rBV	478	344	0.05%	0.006%
86	12.769	3562	3570	3577	rVB2	1096	1668	0.25%	0.031%
87	12.878	3601	3604	3607	rBV	256	209	0.03%	0.004%
88	13.232	3707	3714	3720	rBV3	918	1131	0.17%	0.021%
89	13.852	3900	3907	3915	rVB6	1413	2169	0.33%	0.040%
90	13.926	3928	3930	3935	rVB2	284	168	0.03%	0.003%
91	14.100	3976	3984	3995	rBV2	2817	5310	0.80%	0.099%
92	14.273	4036	4038	4041	rBV	293	223	0.03%	0.004%
93	14.328	4050	4055	4064	rBV5	1308	2143	0.32%	0.040%
94	14.582	4132	4134	4137	rBV2	378	256	0.04%	0.005%
95	14.614	4142	4144	4149	rVB3	336	206	0.03%	0.004%
96	14.724	4175	4178	4181	rBV2	485	327	0.05%	0.006%
97	14.794	4197	4200	4202	rBV	367	244	0.04%	0.005%
98	14.839	4211	4214	4216	rBV2	307	211	0.03%	0.004%
99	14.868	4221	4223	4225	rBV	321	190	0.03%	0.004%
100	15.653	4464	4467	4471	rBV4	421	419	0.06%	0.008%




Sum of corrected areas: 5365222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059558.D
Acq On : 27 Jun 2024 13:10
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

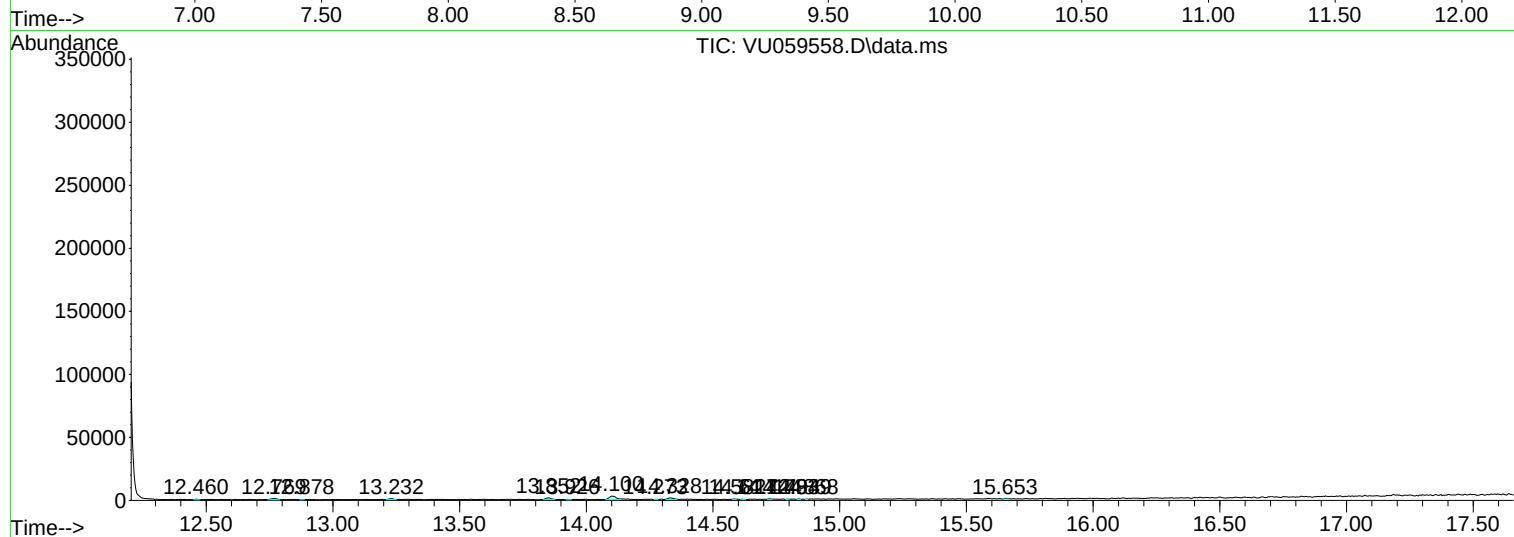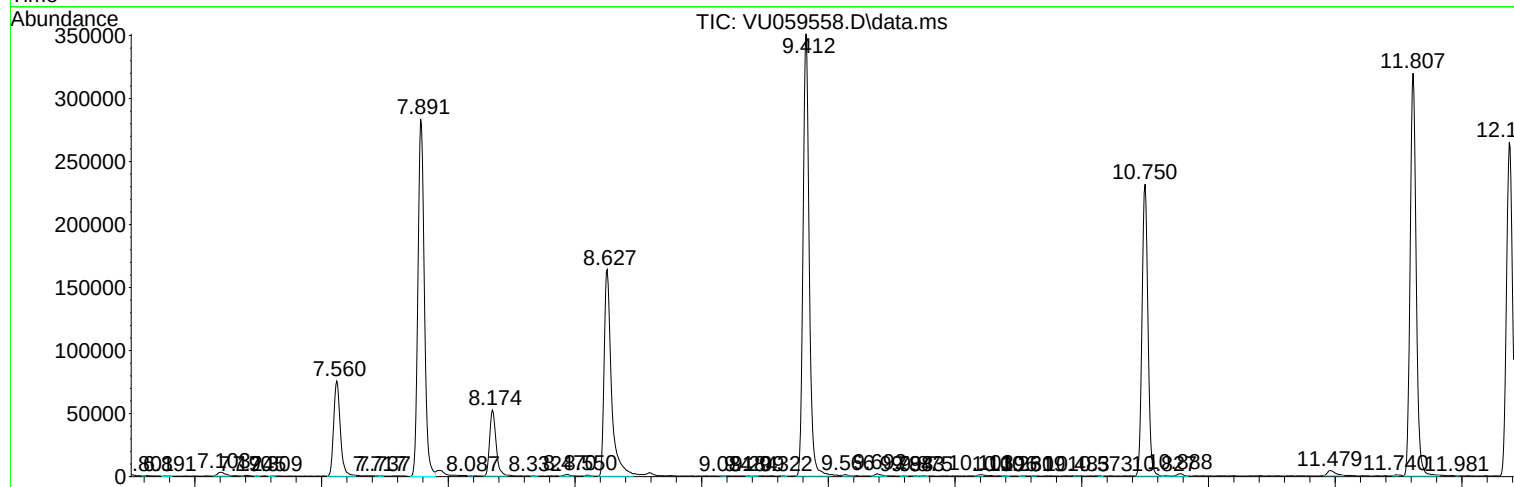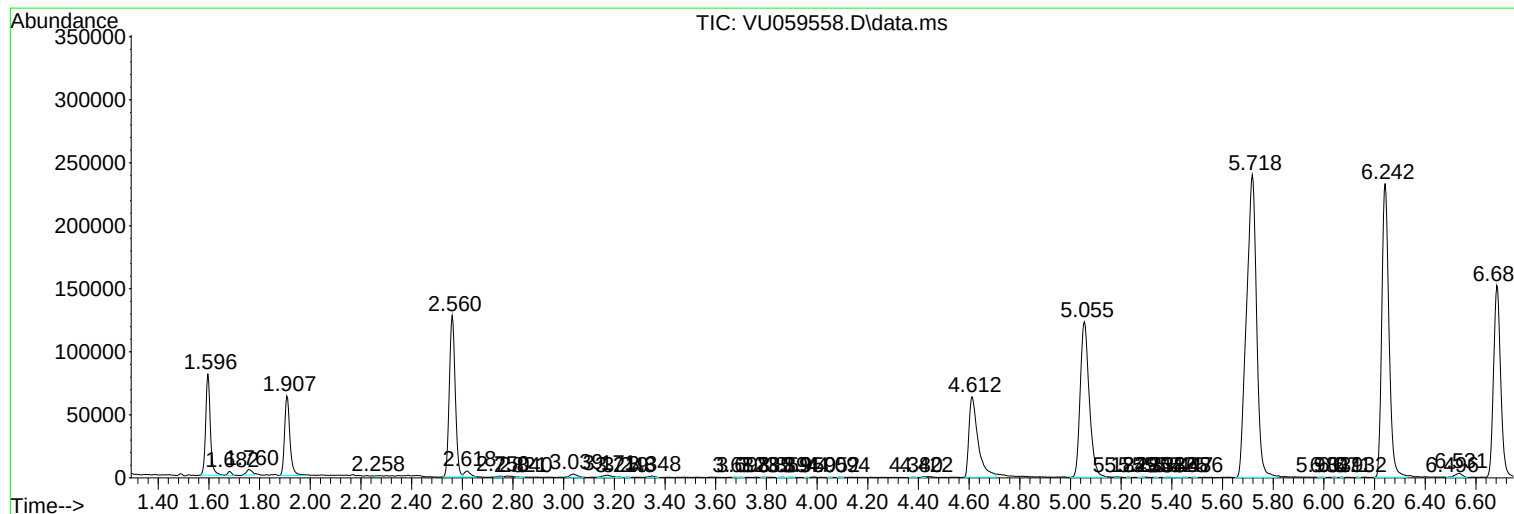

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059558.D
Acq On : 27 Jun 2024 13:10
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059558.D
Acq On : 27 Jun 2024 13:10
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------