

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059560.D
 Acq On : 27 Jun 2024 13:54
 Operator : MD/SY
 Sample : P3062-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	115	rVB	75482	90723	14.56%	1.819%
2	1.907	185	192	211	rVB	60256	84489	13.56%	1.694%
3	2.560	383	395	414	rBV	123194	199256	31.97%	3.996%
4	2.740	448	451	456	rBV2	266	286	0.05%	0.006%
5	2.946	512	515	517	rBV	141	84	0.01%	0.002%
6	3.039	534	544	558	rVB3	6489	11831	1.90%	0.237%
7	3.165	580	583	586	rBV2	257	214	0.03%	0.004%
8	3.309	625	628	630	rBV	219	158	0.03%	0.003%
9	3.438	664	668	672	rBV2	294	284	0.05%	0.006%
10	3.515	690	692	694	rBV	145	94	0.02%	0.002%
11	3.563	703	707	710	rVB	215	146	0.02%	0.003%
12	3.592	710	716	720	rBV2	202	235	0.04%	0.005%
13	3.634	725	729	730	rBV	140	109	0.02%	0.002%
14	3.669	737	740	742	rBV2	229	132	0.02%	0.003%
15	3.753	762	766	769	rBV	209	193	0.03%	0.004%
16	3.788	774	777	780	rBV	190	120	0.02%	0.002%
17	3.927	817	820	823	rBV2	187	157	0.03%	0.003%
18	4.473	984	990	993	rBV2	198	233	0.04%	0.005%
19	4.612	1024	1033	1067	rBV	59935	150314	24.12%	3.014%
20	5.055	1156	1171	1196	rBV	113549	252619	40.53%	5.066%
21	5.203	1214	1217	1220	rVB4	381	272	0.04%	0.005%
22	5.296	1244	1246	1251	rBV2	154	108	0.02%	0.002%
23	5.332	1255	1257	1260	rVB2	170	96	0.02%	0.002%
24	5.460	1293	1297	1302	rBV	196	248	0.04%	0.005%
25	5.512	1308	1313	1316	rBV2	172	170	0.03%	0.003%
26	5.554	1323	1326	1332	rVB2	223	197	0.03%	0.004%
27	5.586	1332	1336	1339	rBV	190	205	0.03%	0.004%
28	5.718	1358	1377	1417	rBV2	225479	623271	100.00%	12.498%
29	5.972	1453	1456	1457	rBV2	187	131	0.02%	0.003%
30	6.052	1478	1481	1486	rBV	279	186	0.03%	0.004%
31	6.081	1487	1490	1494	rBV2	235	189	0.03%	0.004%
32	6.116	1498	1501	1505	rBV	245	218	0.03%	0.004%
33	6.152	1509	1512	1517	rBV	197	174	0.03%	0.003%
34	6.193	1521	1525	1527	rBV	171	146	0.02%	0.003%
35	6.242	1528	1540	1563	rBV	228237	436505	70.03%	8.753%
36	6.528	1622	1629	1638	rVB7	2483	4767	0.76%	0.096%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
 Data File : VU059560.D
 Acq On : 27 Jun 2024 13:54
 Operator : MD/SY
 Sample : P3062-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.566	1638	1641	1642	rBV2	173	101	0.02%	0.002%
38	6.682	1664	1677	1704	rBV	143972	282077	45.26%	5.656%
39	6.862	1729	1733	1736	rBV	234	168	0.03%	0.003%
40	6.885	1736	1740	1742	rBV2	208	158	0.03%	0.003%
41	6.943	1754	1758	1761	rBV2	173	137	0.02%	0.003%
42	7.017	1778	1781	1783	rBV2	140	84	0.01%	0.002%
43	7.129	1813	1816	1818	rBV	143	76	0.01%	0.002%
44	7.197	1833	1837	1838	rBV	398	278	0.04%	0.006%
45	7.283	1862	1864	1866	rVB2	263	80	0.01%	0.002%
46	7.293	1866	1867	1870	rVB2	171	41	0.01%	0.001%
47	7.316	1871	1874	1877	rBV2	159	127	0.02%	0.003%
48	7.370	1888	1891	1894	rBV2	142	131	0.02%	0.003%
49	7.502	1929	1932	1935	rBV	283	183	0.03%	0.004%
50	7.560	1939	1950	1973	rVV2	73410	128280	20.58%	2.572%
51	7.714	1995	1998	2000	rBV2	443	309	0.05%	0.006%
52	7.753	2007	2010	2013	rBV	124	117	0.02%	0.002%
53	7.798	2023	2024	2027	rBV	249	82	0.01%	0.002%
54	7.891	2041	2053	2074	rBV	261387	460883	73.95%	9.242%
55	8.177	2131	2142	2159	rBV	50616	87973	14.11%	1.764%
56	8.303	2178	2181	2183	rBV	169	101	0.02%	0.002%
57	8.357	2193	2198	2201	rBV2	191	232	0.04%	0.005%
58	8.553	2257	2259	2265	rBV2	238	198	0.03%	0.004%
59	8.627	2272	2282	2310	rBV	151681	304229	48.81%	6.100%
60	8.910	2367	2370	2375	rBV3	282	212	0.03%	0.004%
61	8.952	2381	2383	2384	rVB	151	39	0.01%	0.001%
62	9.090	2424	2426	2429	rBV2	163	65	0.01%	0.001%
63	9.357	2507	2509	2513	rBV	266	166	0.03%	0.003%
64	9.412	2513	2526	2549	rBV	336212	571665	91.72%	11.463%
65	9.592	2580	2582	2589	rVB3	333	304	0.05%	0.006%
66	9.624	2589	2592	2597	rBV2	315	266	0.04%	0.005%
67	9.692	2611	2613	2614	rBV	279	114	0.02%	0.002%
68	10.106	2739	2742	2744	rBV2	252	167	0.03%	0.003%
69	10.184	2762	2766	2768	rBV2	300	230	0.04%	0.005%
70	10.274	2790	2794	2798	rBV2	272	266	0.04%	0.005%
71	10.451	2847	2849	2852	rBV	201	118	0.02%	0.002%
72	10.750	2930	2942	2960	rBV	220956	360420	57.83%	7.227%
73	10.885	2981	2984	2990	rBV	308	235	0.04%	0.005%
74	11.045	3031	3034	3038	rBV2	360	274	0.04%	0.005%
75	11.164	3068	3071	3073	rBV	159	115	0.02%	0.002%
76	11.470	3163	3166	3171	rBV2	331	321	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059560.D
Acq On : 27 Jun 2024 13:54
Operator : MD/SY
Sample : P3062-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

77	11.743	3248	3251	3252	rBV2	721	420	0.07%	0.008%
78	11.807	3259	3271	3295	rBV	300119	501684	80.49%	10.060%
79	12.187	3377	3389	3410	rBV	247193	422967	67.86%	8.481%
80	13.229	3710	3713	3715	rBV3	368	226	0.04%	0.005%
81	13.592	3823	3826	3833	rBV2	468	601	0.10%	0.012%
82	14.116	3986	3989	3992	rBV3	782	620	0.10%	0.012%
83	14.341	4052	4059	4060	rBV	851	857	0.14%	0.017%




Sum of corrected areas: 4986957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059560.D
Acq On : 27 Jun 2024 13:54
Operator : MD/SY
Sample : P3062-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

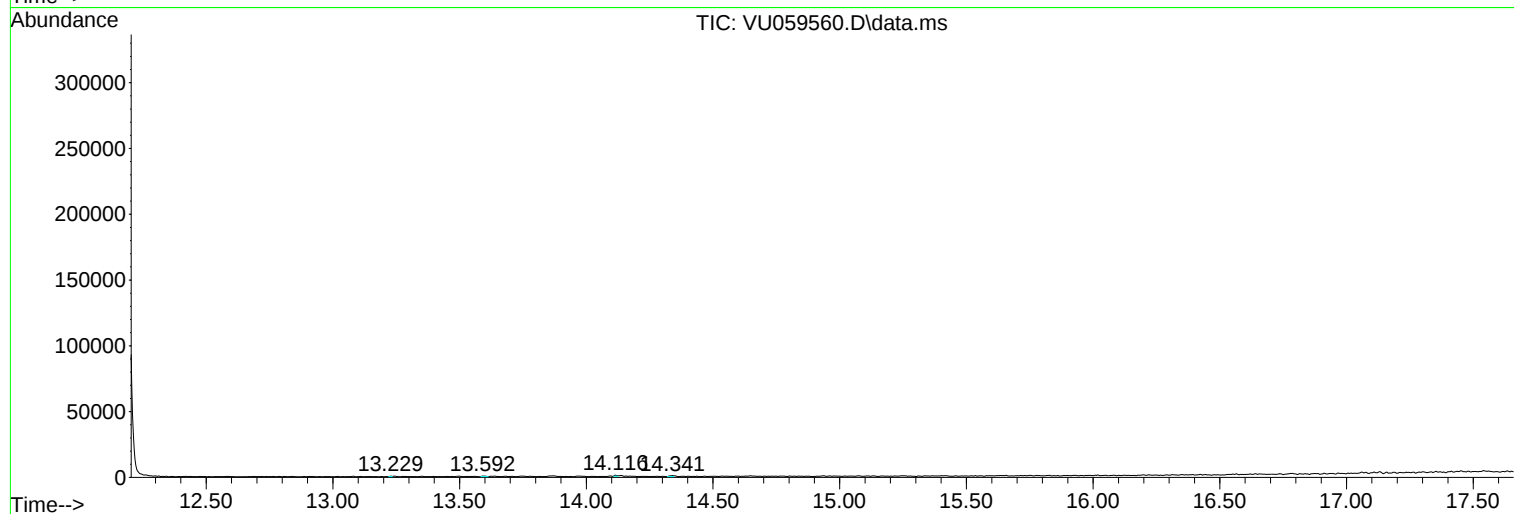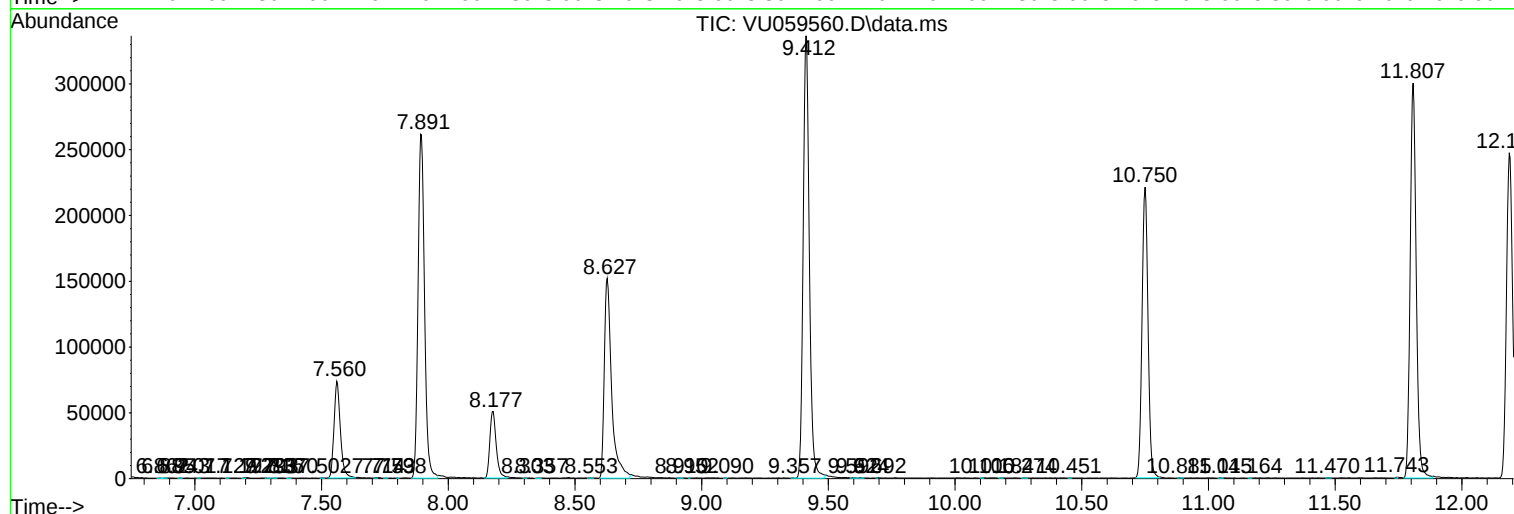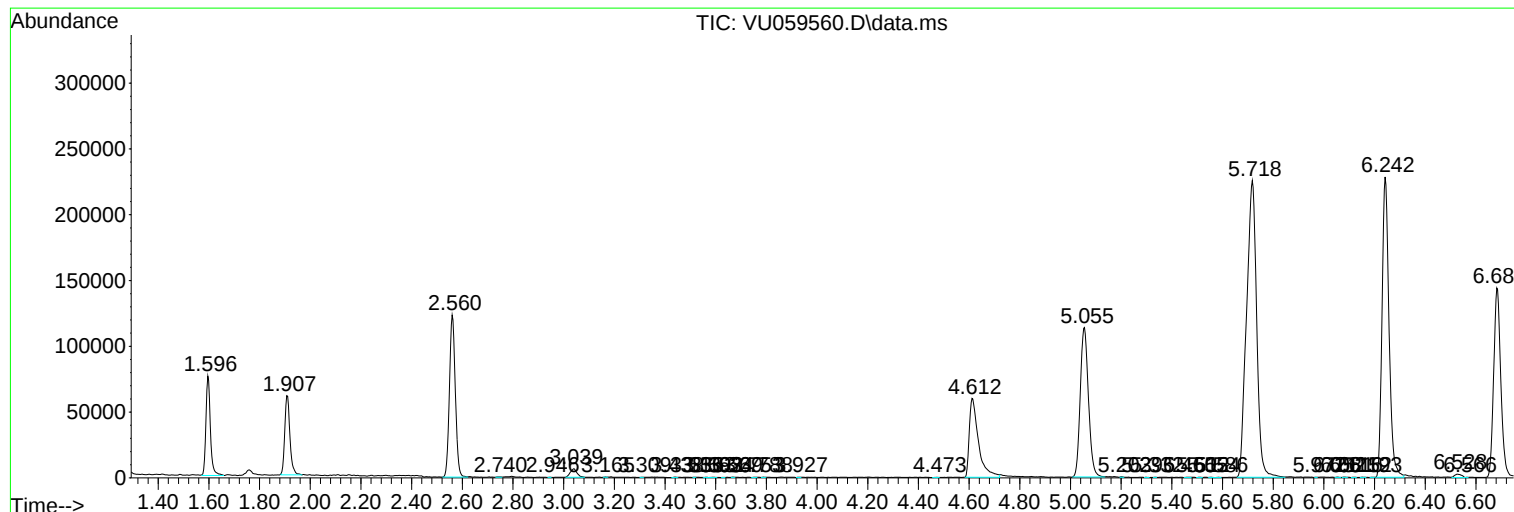

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059560.D
Acq On : 27 Jun 2024 13:54
Operator : MD/SY
Sample : P3062-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059560.D
Acq On : 27 Jun 2024 13:54
Operator : MD/SY
Sample : P3062-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc