


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062724\
Data File : VU059545.D
Acq On : 27 Jun 2024 07:44
Operator : MD/SY
Sample : BFB069
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB069

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Thu Jun 27 04:10:00 2024

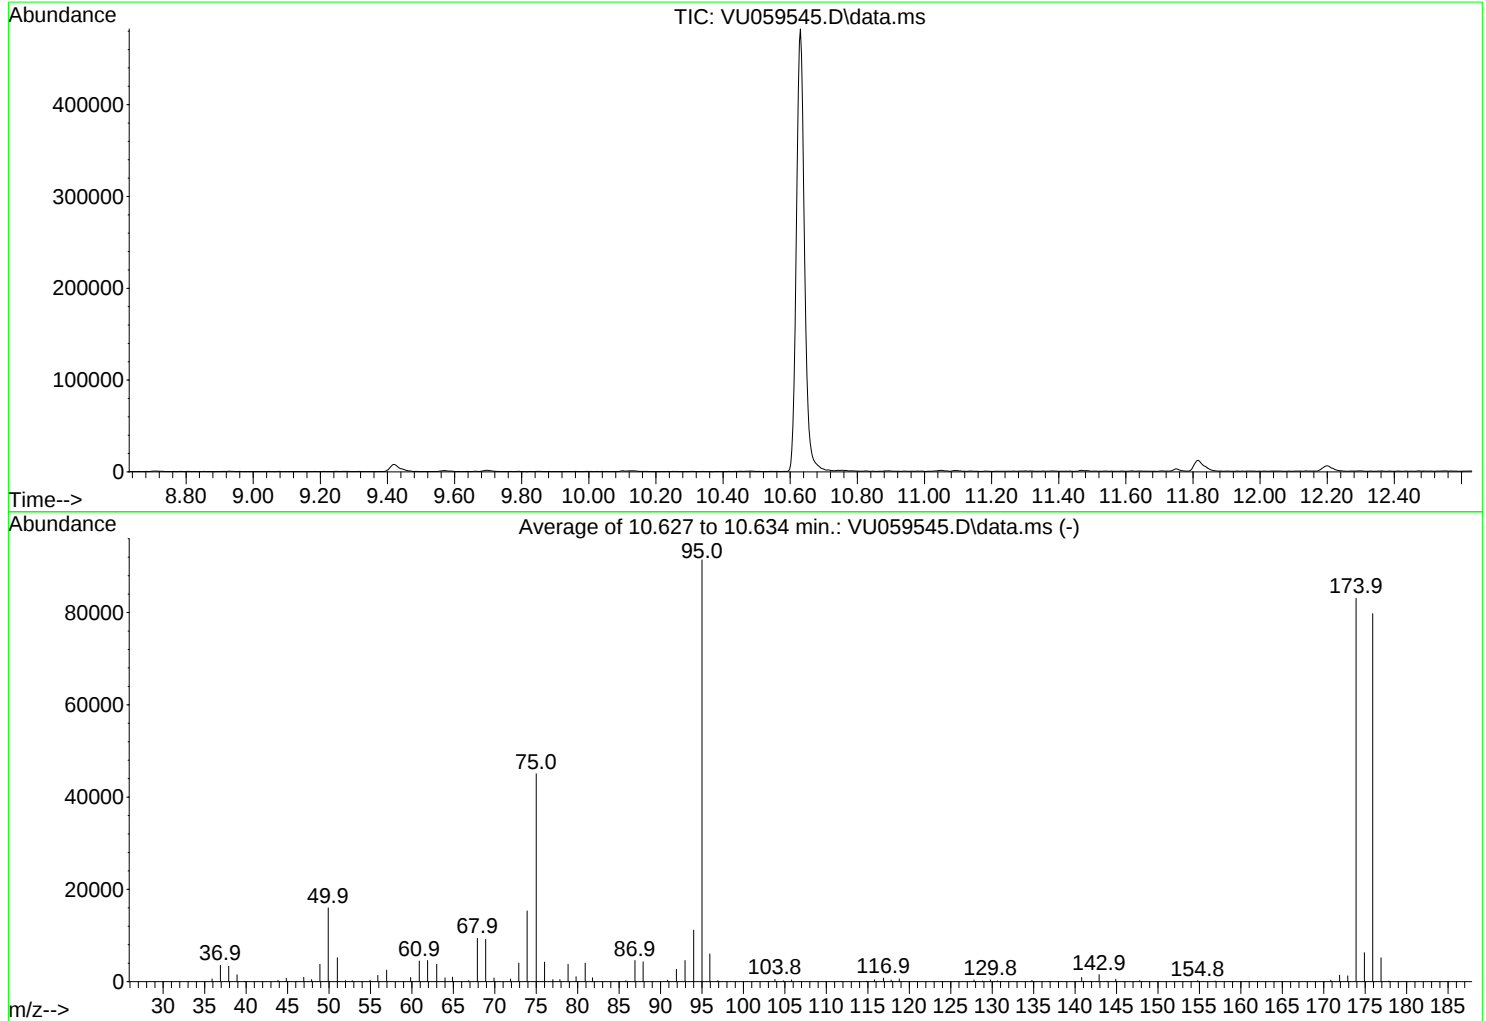

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	15986	PASS
75	95	30	80	49.3	45067	PASS
95	95	100	100	100.0	91432	PASS
96	95	5	9	6.6	5999	PASS
173	174	0.00	2	1.5	1245	PASS
174	95	50	120	90.9	83093	PASS
175	174	5	9	7.6	6280	PASS
176	174	95	101	96.0	79781	PASS
177	176	5	9	6.5	5185	PASS

m/z	Abundance
39.80	158.0
43.80	420.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	526.0
36.90	3545.0
37.90	3453.0
38.90	1526.0
39.80	243.0
43.90	719.0
44.80	784.0
46.10	124.0
46.90	1095.0
47.90	466.0
48.90	3953.0
49.90	16432.0
51.00	5306.0
52.00	216.0
52.80	174.0
53.90	117.0
54.90	294.0
55.90	1397.0
56.90	2404.0
59.80	969.0
60.90	4807.0
61.90	4598.0
63.00	3882.0
64.00	968.0
64.90	883.0
66.80	193.0
67.90	9525.0
68.90	9206.0
69.90	712.0
71.90	509.0
72.90	4051.0
73.90	15787.0
75.00	45120.0
76.00	4482.0
77.00	448.0
77.90	478.0
78.90	3804.0
79.80	1143.0
80.90	4013.0
81.80	768.0
82.90	105.0
85.70	191.0
86.90	4637.0
87.90	4408.0
90.80	345.0
91.90	2694.0
93.00	4584.0
94.00	11457.0
95.00	91336.0
96.00	6428.0
96.90	176.0
102.90	109.0
103.80	427.0
104.80	236.0
105.80	407.0
111.80	134.0
114.80	109.0
115.80	353.0
116.90	778.0
117.80	328.0
118.80	560.0
127.80	358.0
128.90	130.0
129.80	380.0
130.70	160.0
134.80	279.0
136.80	117.0
140.80	840.0
142.90	1497.0
143.80	105.0
144.90	525.0
145.80	137.0
147.80	207.0
154.80	252.0
156.90	140.0
170.90	291.0
171.90	1384.0
172.90	1252.0
173.90	81576.0
174.90	6378.0
175.90	78440.0
176.90	5118.0
177.90	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	590.0
36.90	3698.0
37.90	3453.0
38.90	1516.0
39.80	251.0
43.90	738.0
44.90	691.0
46.10	107.0
47.00	972.0
47.90	454.0
48.90	3882.0
49.90	16400.0
51.00	5408.0
52.00	217.0
52.80	208.0
55.00	352.0
55.90	1402.0
56.90	2565.0
59.90	921.0
60.90	4599.0
61.90	4779.0
63.00	3867.0
64.00	870.0
64.90	982.0
66.90	212.0
67.90	9674.0
68.90	9447.0
69.90	852.0
71.90	587.0
72.90	4134.0
73.90	15716.0
75.00	46480.0
76.00	4365.0
77.00	483.0
77.90	451.0
78.80	3784.0
79.80	1128.0
80.90	4122.0
81.80	855.0
85.80	191.0
86.90	4798.0
87.90	4397.0
90.90	318.0
91.90	2772.0
93.00	4779.0
94.00	11478.0
95.00	93952.0
96.00	6231.0
96.90	227.0
103.80	531.0
104.80	230.0
105.80	412.0
106.80	112.0
111.80	127.0
114.80	102.0
115.80	414.0
116.90	792.0
117.80	354.0
118.80	630.0
127.80	383.0
128.80	126.0
129.80	404.0
130.60	170.0
134.80	309.0
140.80	959.0
142.90	1553.0
143.90	106.0
144.90	549.0
147.80	240.0
154.80	288.0
156.90	139.0
170.80	346.0
171.90	1418.0
172.90	1310.0
173.90	85712.0
174.90	6475.0
175.90	82376.0
176.90	5308.0
177.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	634.0
36.90	3435.0
37.90	3136.0
38.90	1480.0
39.80	216.0
43.90	688.0
44.90	579.0
46.90	775.0
47.90	412.0
48.90	3398.0
49.90	15126.0
51.00	4823.0
52.00	202.0
52.80	198.0
54.90	344.0
55.90	1265.0
57.00	2483.0
59.90	866.0
60.90	4066.0
61.90	4397.0
63.00	3602.0
64.00	714.0
64.90	1034.0
65.90	110.0
66.90	213.0
67.90	8918.0
68.90	8829.0
69.90	847.0
71.90	563.0
72.90	3899.0
73.90	14446.0
75.00	43600.0
76.00	3859.0
77.00	483.0
77.80	413.0
78.80	3639.0
79.80	992.0
80.90	3976.0
81.80	871.0
85.90	234.0
86.90	4362.0
87.90	4070.0
90.90	270.0
91.90	2572.0
92.90	4411.0
94.00	10577.0
95.00	89008.0
95.90	5337.0
96.90	230.0
103.80	518.0
104.80	178.0
105.80	372.0
106.80	123.0
108.00	105.0
114.90	105.0
115.80	440.0
116.90	738.0
117.80	332.0
118.80	629.0
127.80	380.0
128.90	137.0
129.80	392.0
130.60	171.0
134.80	256.0
140.80	949.0
141.80	109.0
142.90	1514.0
143.90	113.0
144.90	519.0
147.80	238.0
154.80	245.0
156.90	136.0
158.70	110.0
170.80	349.0
171.90	1337.0
172.90	1174.0
173.90	81992.0
174.90	5986.0
175.90	78528.0
176.90	5129.0
177.90	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069