

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059739.D
 Acq On : 02 Jul 2024 15:06
 Operator : MD/SY
 Sample : P3108-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 03 01:55:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 01:39:57 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	266705	50.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	265951	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152	119496	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.596	65	86941	50.771	ug/L	0.00
Spiked Amount	50.000	Range 60	- 135	Recovery	=	101.540%	
7) Chloroethane-d5		1.907	69	73713	51.176	ug/L	0.00
Spiked Amount	50.000	Range 70	- 130	Recovery	=	102.360%	
11) 1,1-Dichloroethene-d2		2.560	63	111863	36.770	ug/L	0.00
Spiked Amount	50.000	Range 60	- 125	Recovery	=	73.540%	
21) 2-Butanone-d5		4.612	46	131336	110.360	ug/L	0.00
Spiked Amount	100.000	Range 40	- 130	Recovery	=	110.360%	
24) Chloroform-d		5.052	84	162399	48.972	ug/L	0.00
Spiked Amount	50.000	Range 70	- 125	Recovery	=	97.940%	
26) 1,2-Dichloroethane-d4		5.692	65	100884	51.165	ug/L	0.00
Spiked Amount	50.000	Range 70	- 125	Recovery	=	102.320%	
32) Benzene-d6		5.718	84	338804	49.749	ug/L	0.00
Spiked Amount	50.000	Range 70	- 125	Recovery	=	99.500%	
36) 1,2-Dichloropropane-d6		6.682	67	105617	50.109	ug/L	0.00
Spiked Amount	50.000	Range 70	- 120	Recovery	=	100.220%	
41) Toluene-d8		7.891	98	299591	46.259	ug/L	0.00
Spiked Amount	50.000	Range 80	- 120	Recovery	=	92.520%	
43) trans-1,3-Dichloroprop...		8.174	79	47128	47.783	ug/L	0.00
Spiked Amount	50.000	Range 60	- 125	Recovery	=	95.560%	
47) 2-Hexanone-d5		8.624	63	91880	103.434	ug/L	0.00
Spiked Amount	100.000	Range 45	- 130	Recovery	=	103.430%	
56) 1,1,2,2-Tetrachloroeth...		10.750	84	164414	50.821	ug/L	0.00
Spiked Amount	50.000	Range 65	- 120	Recovery	=	101.640%	
66) 1,2-Dichlorobenzene-d4		12.187	152	113805	51.827	ug/L	0.00
Spiked Amount	50.000	Range 80	- 120	Recovery	=	103.660%	
Target Compounds							
37) 1,2-Dichloropropane		6.682	63	11040	5.585	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059739.D
Acq On : 02 Jul 2024 15:06
Operator : MD/SY
Sample : P3108-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jul 03 01:55:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 01:39:57 2024
Response via : Initial Calibration

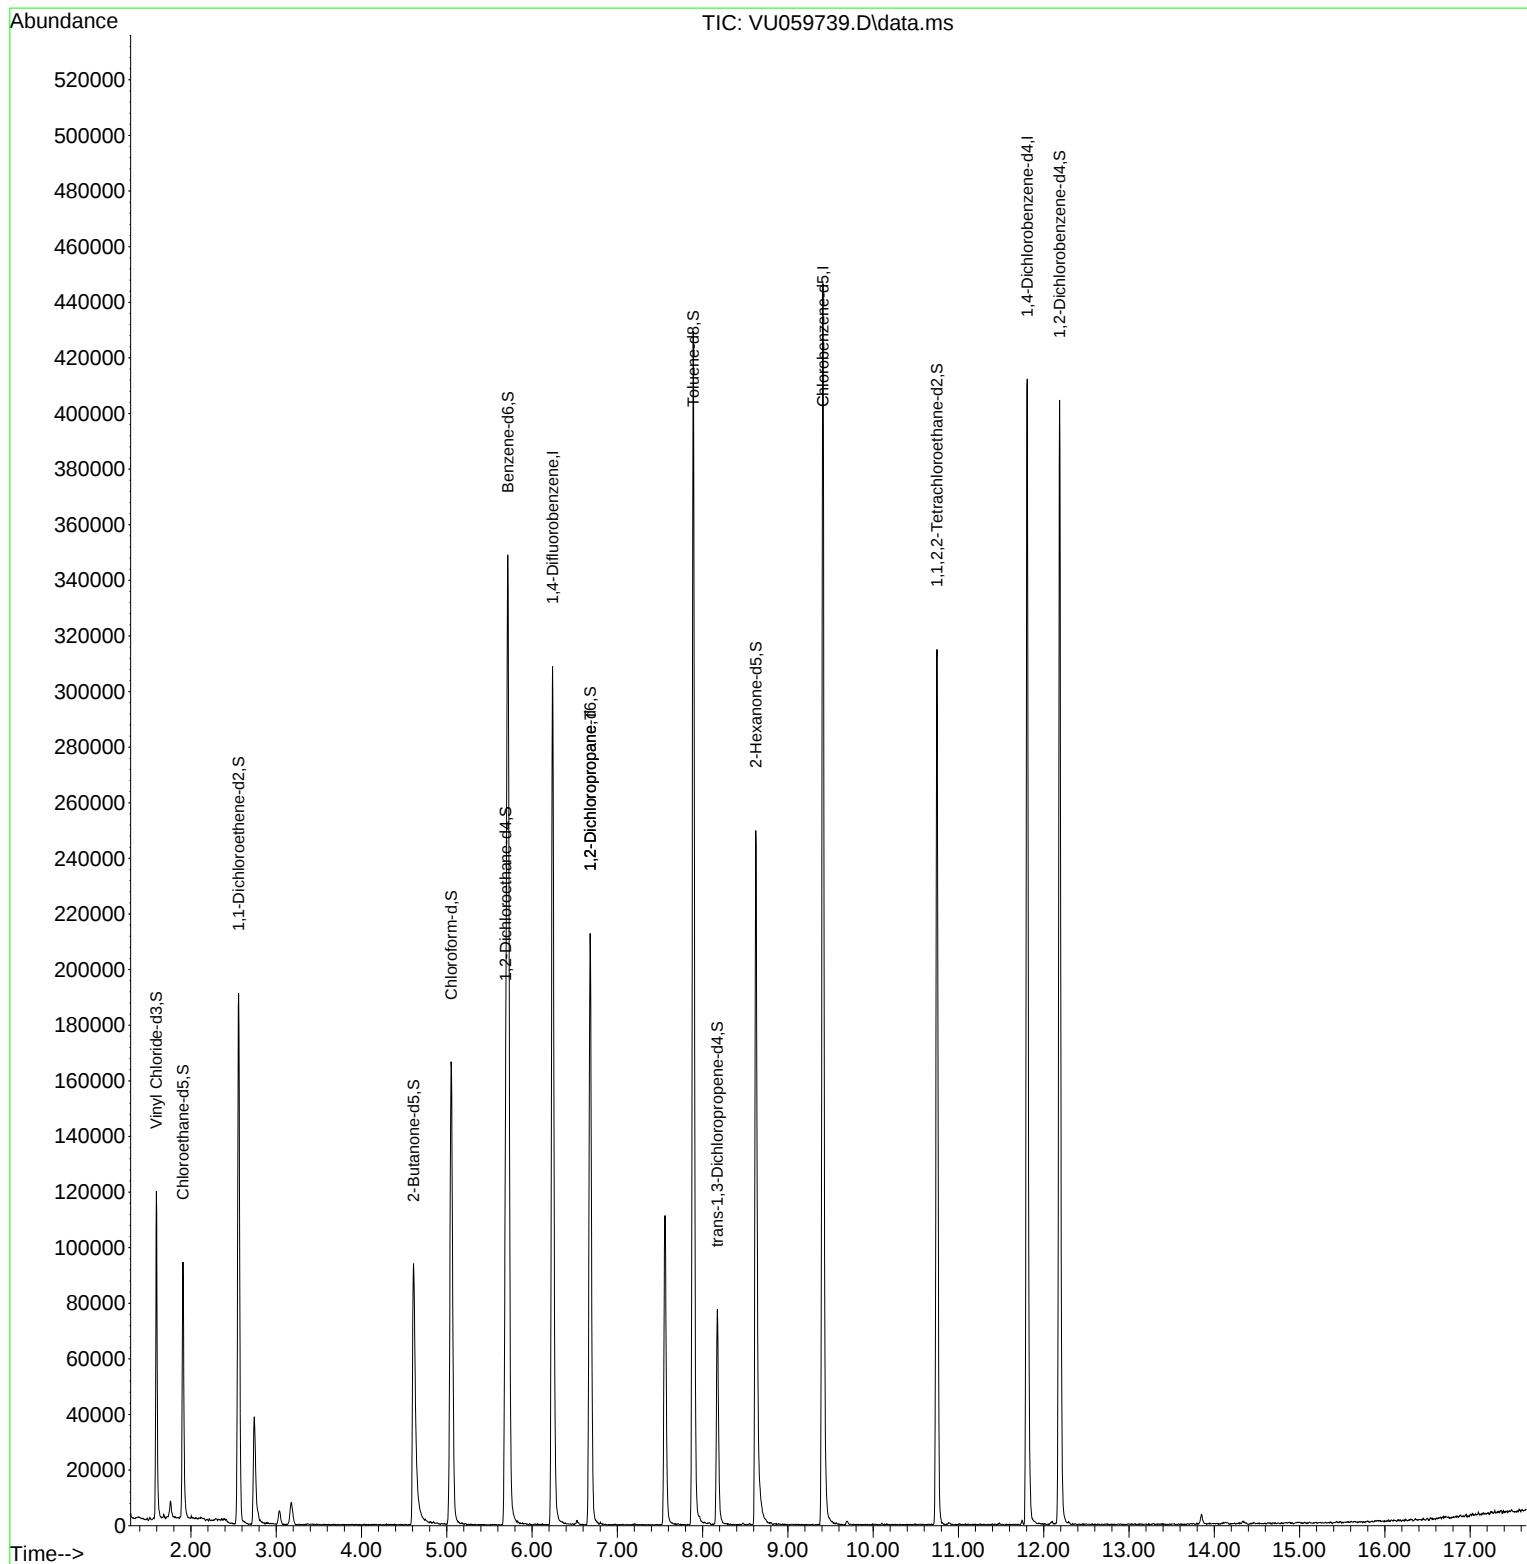

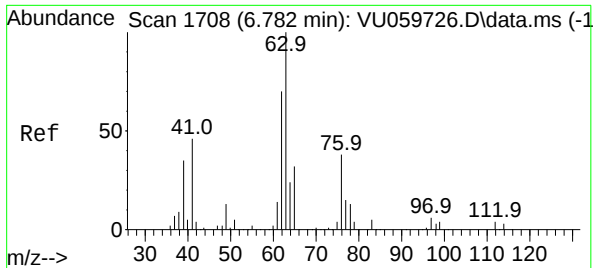

#37
 1,2-Dichloropropane
 Concen: 5.585 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU059739.D
 Acq: 02 Jul 2024 15:06

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 11040
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.6#

