

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059733.D
 Acq On : 02 Jul 2024 12:51
 Operator : MD/SY
 Sample : P3091-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DE9

Quant Time: Jul 03 01:53:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 03 01:39:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	297234	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	293443	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	131986	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	96666	50.652	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	101.300%	
7) Chloroethane-d5	1.907	69	81477	50.757	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	101.520%	
11) 1,1-Dichloroethene-d2	2.560	63	125502	37.016	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	74.040%	
21) 2-Butanone-d5	4.611	46	141221	106.478	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.480%	
24) Chloroform-d	5.052	84	175816	47.573	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.140%	
26) 1,2-Dichloroethane-d4	5.692	65	110721	50.386	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.780%	
32) Benzene-d6	5.721	84	374514	49.841	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.680%	
36) 1,2-Dichloropropane-d6	6.682	67	116027	49.890	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.780%	
41) Toluene-d8	7.891	98	339050	47.447	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.900%	
43) trans-1,3-Dichloroprop...	8.174	79	50565	46.464	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.920%	
47) 2-Hexanone-d5	8.624	63	101056	103.106	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	103.110%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	175097	49.053	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.100%	
66) 1,2-Dichlorobenzene-d4	12.187	152	125161	51.605	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.200%	
Target Compounds						
13) Acetone	2.618	43	16417	12.021	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059733.D
Acq On : 02 Jul 2024 12:51
Operator : MD/SY
Sample : P3091-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DE9

Quant Time: Jul 03 01:53:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 03 01:39:57 2024
Response via : Initial Calibration

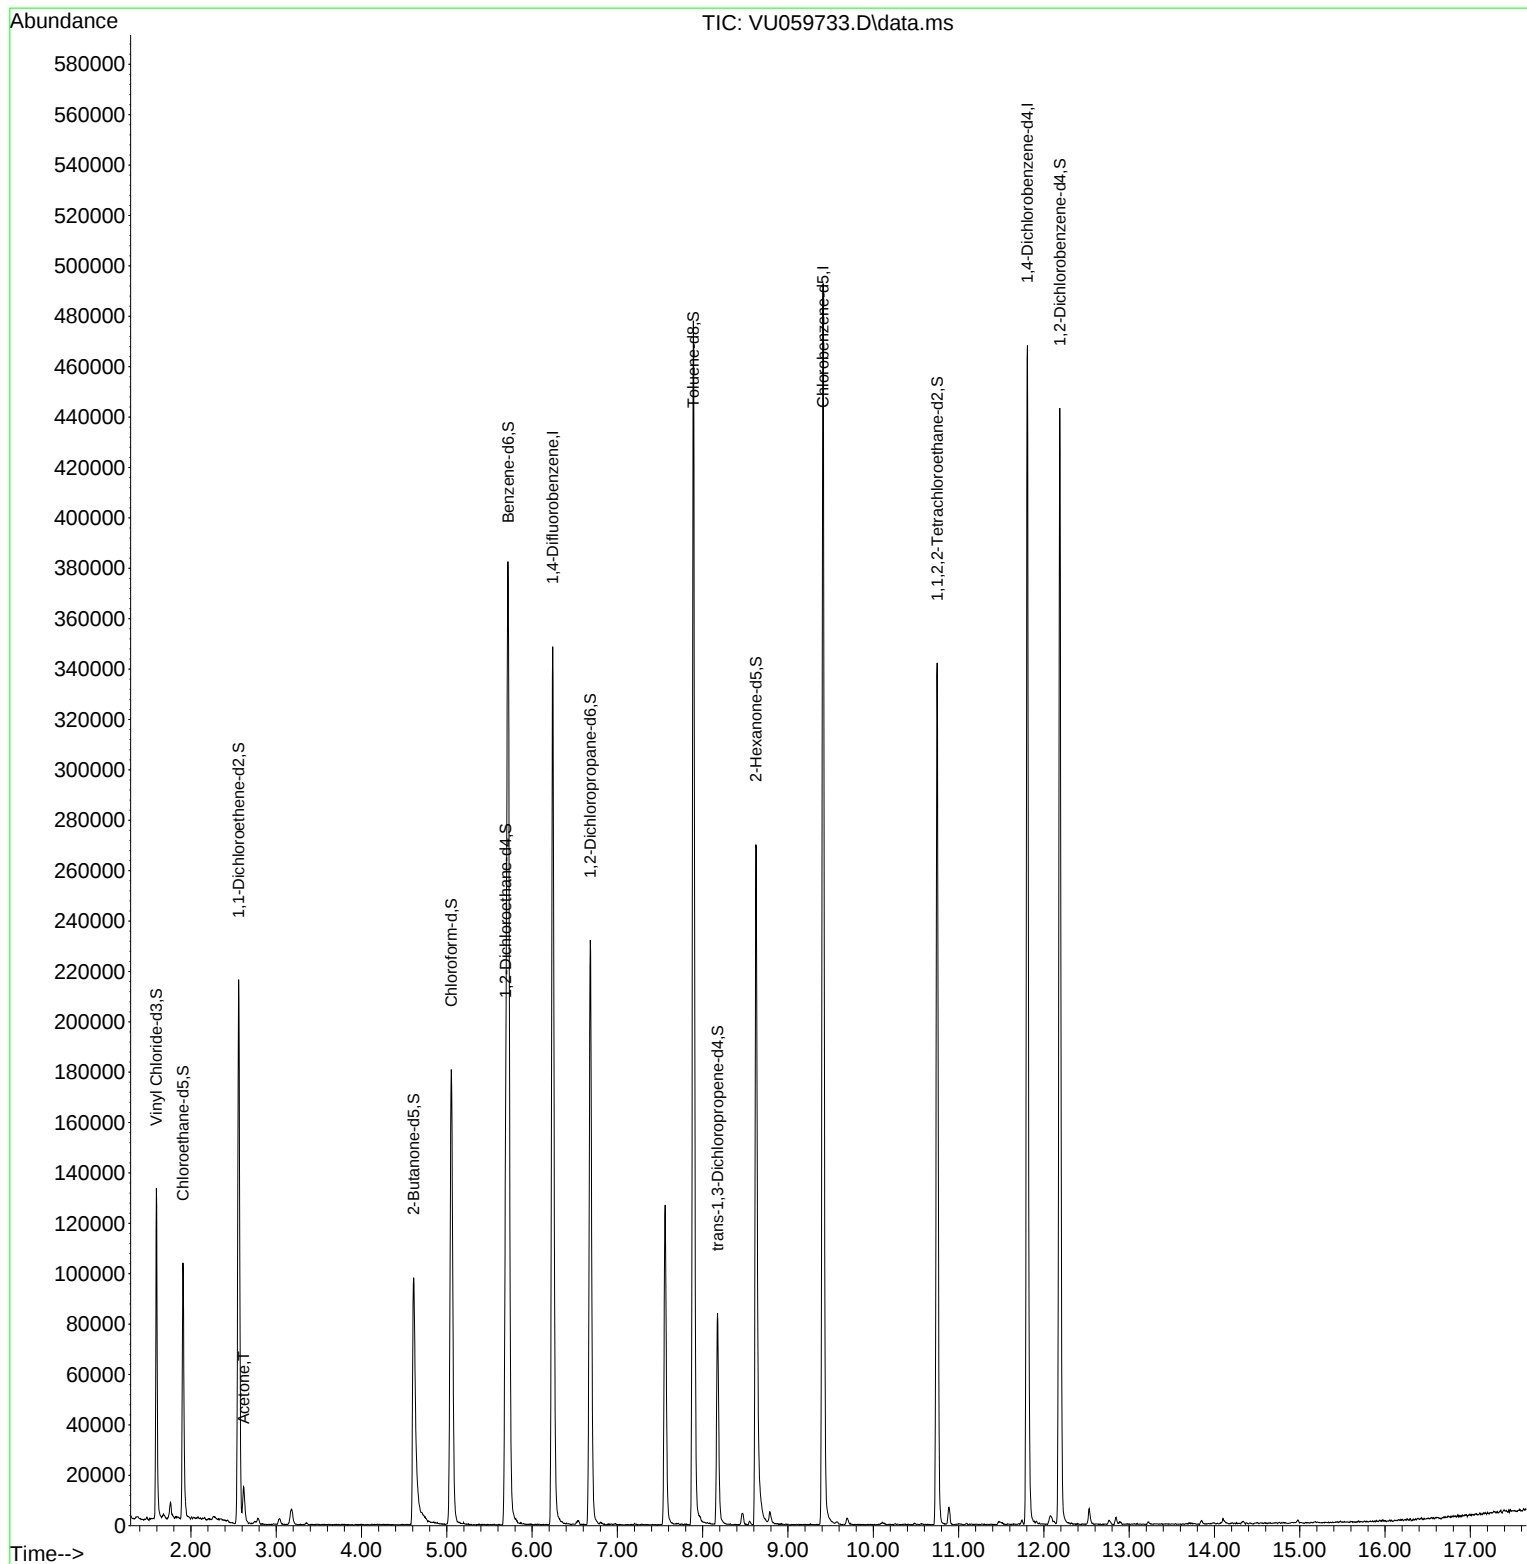

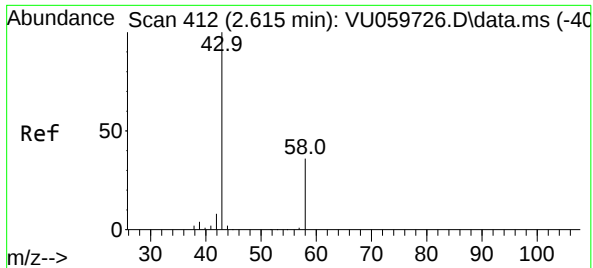

#13
 Acetone
 Concen: 12.021 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU059733.D
 Acq: 02 Jul 2024 12:51

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DE9

Tgt Ion:	43	Resp:	16417
Ion	Ratio	Lower	Upper
43	100		
58	36.7	0.0	73.8

