

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059732.D
 Acq On : 02 Jul 2024 12:28
 Operator : MD/SY
 Sample : P3091-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU059732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.460	45	53	87	rBV	167420	337981	31.55%	3.807%
2	1.595	88	95	107	rVB	135867	159551	14.89%	1.797%
3	1.907	184	192	208	rBV	103588	141527	13.21%	1.594%
4	2.560	383	395	407	rBV	226270	364678	34.04%	4.107%
5	2.618	407	413	432	rVB	14745	26549	2.48%	0.299%
6	2.747	447	453	458	rBV4	1492	2129	0.20%	0.024%
7	2.782	460	464	466	rBV2	1608	1442	0.13%	0.016%
8	3.036	535	543	554	rVB2	2367	4325	0.40%	0.049%
9	3.177	571	587	608	rVV	51345	120075	11.21%	1.352%
10	3.251	608	610	614	rVB	469	348	0.03%	0.004%
11	3.341	634	638	642	rBV2	962	867	0.08%	0.010%
12	3.425	659	664	669	rBV2	343	429	0.04%	0.005%
13	3.608	715	721	724	rBV2	273	344	0.03%	0.004%
14	3.782	771	775	780	rBV2	225	255	0.02%	0.003%
15	3.965	829	832	836	rVB	310	235	0.02%	0.003%
16	3.991	836	840	843	rBV	305	219	0.02%	0.002%
17	4.119	877	880	883	rBV	243	204	0.02%	0.002%
18	4.184	897	900	905	rVB2	318	282	0.03%	0.003%
19	4.373	955	959	963	rBV2	301	325	0.03%	0.004%
20	4.415	969	972	978	rVB2	286	305	0.03%	0.003%
21	4.473	986	990	995	rBV	201	229	0.02%	0.003%
22	4.557	1009	1016	1017	rBV2	237	246	0.02%	0.003%
23	4.611	1017	1033	1061	rBV	118202	304560	28.43%	3.430%
24	5.052	1150	1170	1199	rBV	186494	415509	38.78%	4.680%
25	5.322	1251	1254	1259	rBV2	429	366	0.03%	0.004%
26	5.357	1263	1265	1269	rVB	423	275	0.03%	0.003%
27	5.418	1281	1284	1288	rVB2	407	287	0.03%	0.003%
28	5.454	1288	1295	1297	rBV	405	306	0.03%	0.003%
29	5.470	1297	1300	1302	rBV2	354	241	0.02%	0.003%
30	5.483	1302	1304	1309	rVB2	424	297	0.03%	0.003%
31	5.521	1309	1316	1318	rBV2	194	207	0.02%	0.002%
32	5.717	1352	1377	1398	rBV2	391950	1071421	100.00%	12.067%
33	5.888	1427	1430	1436	rVB3	378	320	0.03%	0.004%
34	6.148	1508	1511	1514	rVB2	305	236	0.02%	0.003%
35	6.177	1514	1520	1524	rBV3	492	566	0.05%	0.006%
36	6.242	1524	1540	1563	rBV	347048	669505	62.49%	7.541%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059732.D
Acq On : 02 Jul 2024 12:28
Operator : MD/SY
Sample : P3091-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis

37	6.534	1622	1631	1644	rVB7	2376	4209	0.39%	0.047%
38	6.682	1664	1677	1697	rBV	238528	466105	43.50%	5.250%
39	6.849	1724	1729	1731	rBV	412	343	0.03%	0.004%
40	6.898	1736	1744	1746	rBV	340	481	0.04%	0.005%
41	6.949	1755	1760	1763	rBV	303	358	0.03%	0.004%
42	6.994	1772	1774	1777	rVB2	361	220	0.02%	0.002%
43	7.016	1777	1781	1787	rBV2	420	506	0.05%	0.006%
44	7.100	1802	1807	1809	rBV2	552	522	0.05%	0.006%
45	7.325	1874	1877	1884	rVB2	317	291	0.03%	0.003%
46	7.560	1938	1950	1975	rBV	128141	231891	21.64%	2.612%
47	7.695	1990	1992	1995	rBV2	296	246	0.02%	0.003%
48	7.717	1998	1999	2009	rVB2	500	515	0.05%	0.006%
49	7.791	2019	2022	2024	rBV2	349	255	0.02%	0.003%
50	7.804	2024	2026	2031	rVB3	648	373	0.03%	0.004%
51	7.891	2041	2053	2073	rBV	494872	860306	80.30%	9.690%
52	8.174	2129	2141	2165	rBV	87949	155616	14.52%	1.753%
53	8.463	2218	2231	2245	rBV2	11267	20709	1.93%	0.233%
54	8.518	2245	2248	2251	rVB	311	197	0.02%	0.002%
55	8.550	2251	2258	2270	rBV4	1639	2173	0.20%	0.024%
56	8.624	2270	2281	2319	rBV	272330	521526	48.68%	5.874%
57	8.791	2325	2333	2344	rVB6	3025	5212	0.49%	0.059%
58	8.978	2389	2391	2398	rVB2	348	303	0.03%	0.003%
59	9.267	2476	2481	2487	rBV3	255	339	0.03%	0.004%
60	9.412	2511	2526	2558	rBV	487580	832353	77.69%	9.375%
61	9.537	2563	2565	2568	rVV3	948	743	0.07%	0.008%
62	9.569	2568	2575	2580	rVV4	1434	2377	0.22%	0.027%
63	9.592	2580	2582	2585	rVV2	387	240	0.02%	0.003%
64	9.621	2588	2591	2596	rVB	262	241	0.02%	0.003%
65	9.695	2606	2614	2626	rBV4	2796	5194	0.48%	0.058%
66	10.097	2734	2739	2740	rBV3	782	574	0.05%	0.006%
67	10.251	2784	2787	2789	rBV	392	307	0.03%	0.003%
68	10.274	2791	2794	2801	rVV	319	385	0.04%	0.004%
69	10.421	2834	2840	2843	rBV2	297	327	0.03%	0.004%
70	10.749	2928	2942	2961	rBV	349629	568027	53.02%	6.398%
71	10.884	2974	2984	2997	rBV2	13480	22046	2.06%	0.248%
72	11.003	3014	3021	3027	rBV2	481	714	0.07%	0.008%
73	11.090	3043	3048	3051	rBV3	481	479	0.04%	0.005%
74	11.473	3158	3167	3169	rBV4	1124	1501	0.14%	0.017%
75	11.743	3245	3251	3259	rVB5	1721	2356	0.22%	0.027%
76	11.807	3259	3271	3292	rBV	463417	752377	70.22%	8.474%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059732.D
 Acq On : 02 Jul 2024 12:28
 Operator : MD/SY
 Sample : P3091-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.991	3325	3328	3332	rBV3	331	376	0.04%	0.004%
78	12.071	3345	3353	3370	rBV9	3534	9057	0.85%	0.102%
79	12.187	3377	3389	3413	rBV	454389	746947	69.72%	8.413%
80	12.482	3478	3481	3484	rVB2	397	307	0.03%	0.003%
81	12.531	3488	3496	3506	rVV4	5100	8460	0.79%	0.095%
82	12.765	3559	3569	3578	rVB	4112	5845	0.55%	0.066%
83	12.846	3586	3594	3601	rBV6	1941	2954	0.28%	0.033%
84	12.900	3605	3611	3615	rBV2	732	894	0.08%	0.010%
85	12.945	3621	3625	3626	rBV	445	298	0.03%	0.003%
86	13.126	3677	3681	3687	rVB2	434	463	0.04%	0.005%
87	13.154	3687	3690	3693	rBV	375	358	0.03%	0.004%
88	13.219	3706	3710	3711	rBV	825	521	0.05%	0.006%
89	13.302	3732	3736	3739	rBV	379	400	0.04%	0.005%
90	13.617	3830	3834	3837	rBV2	359	317	0.03%	0.004%
91	13.720	3860	3866	3872	rVV3	473	527	0.05%	0.006%
92	13.843	3896	3904	3905	rBV3	1499	1403	0.13%	0.016%
93	13.910	3921	3925	3927	rBV2	390	301	0.03%	0.003%
94	13.952	3935	3938	3941	rVB2	334	233	0.02%	0.003%
95	14.035	3961	3964	3969	rBV2	332	287	0.03%	0.003%
96	14.106	3974	3986	3993	rBV3	3066	5530	0.52%	0.062%
97	14.331	4052	4056	4068	rVB6	1748	2621	0.24%	0.030%
98	14.412	4077	4081	4083	rBV3	391	309	0.03%	0.003%
99	14.511	4109	4112	4116	rBV2	314	233	0.02%	0.003%
100	15.646	4461	4465	4467	rBV3	618	522	0.05%	0.006%




Sum of corrected areas: 8878741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059732.D
Acq On : 02 Jul 2024 12:28
Operator : MD/SY
Sample : P3091-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

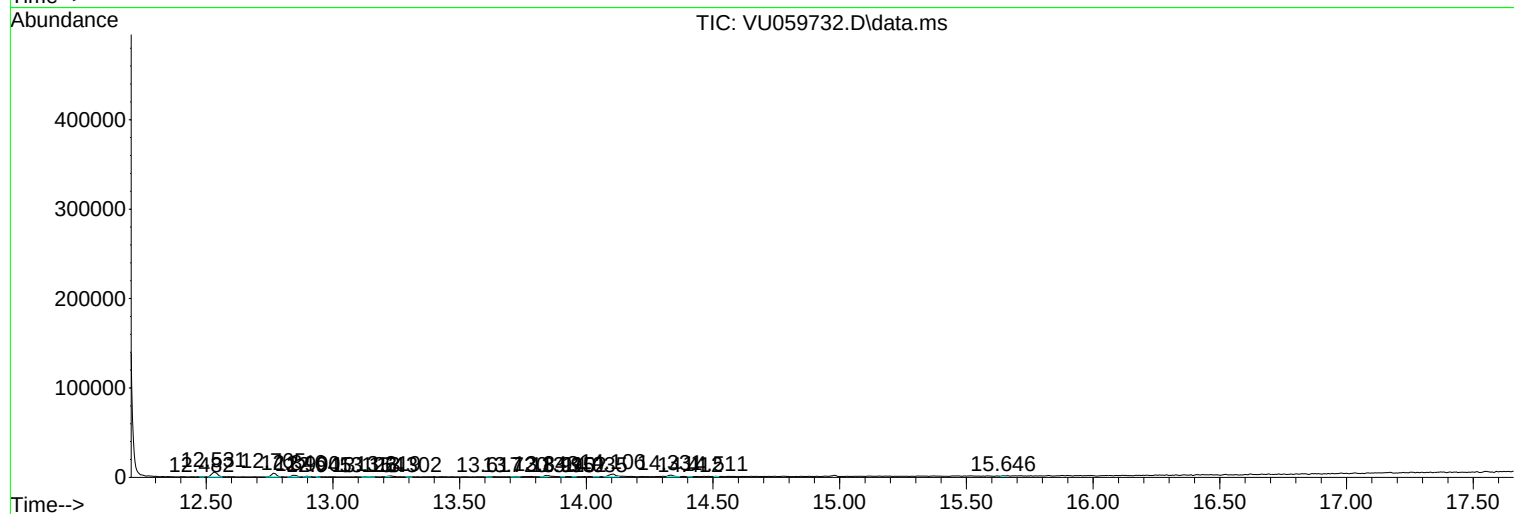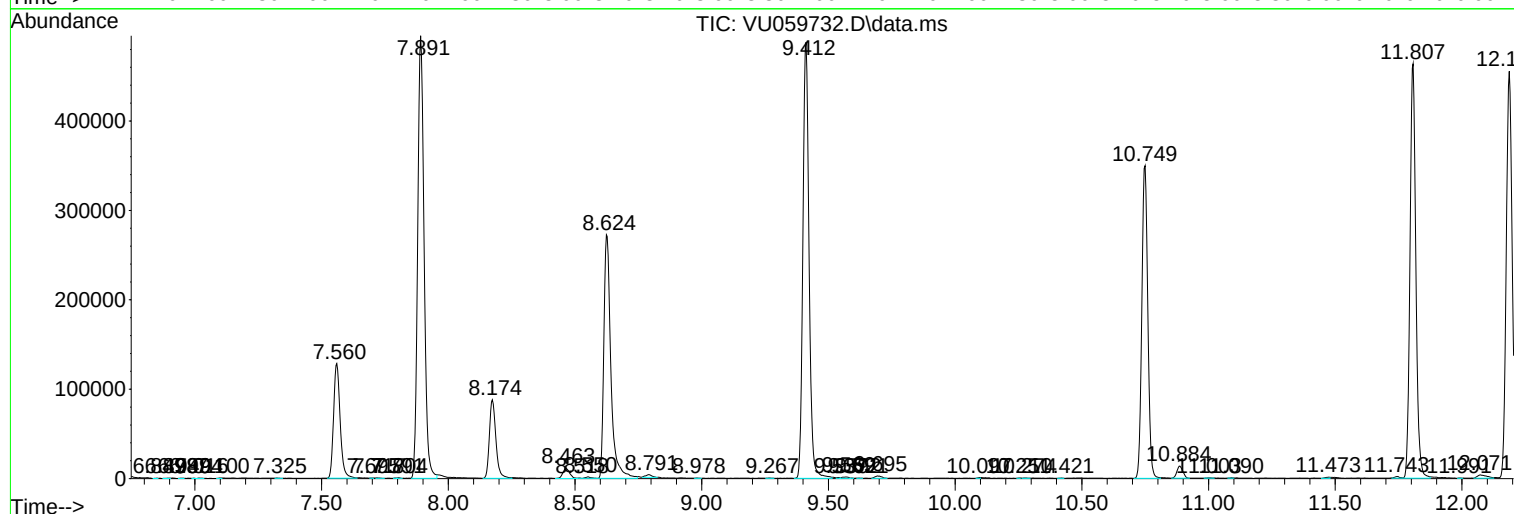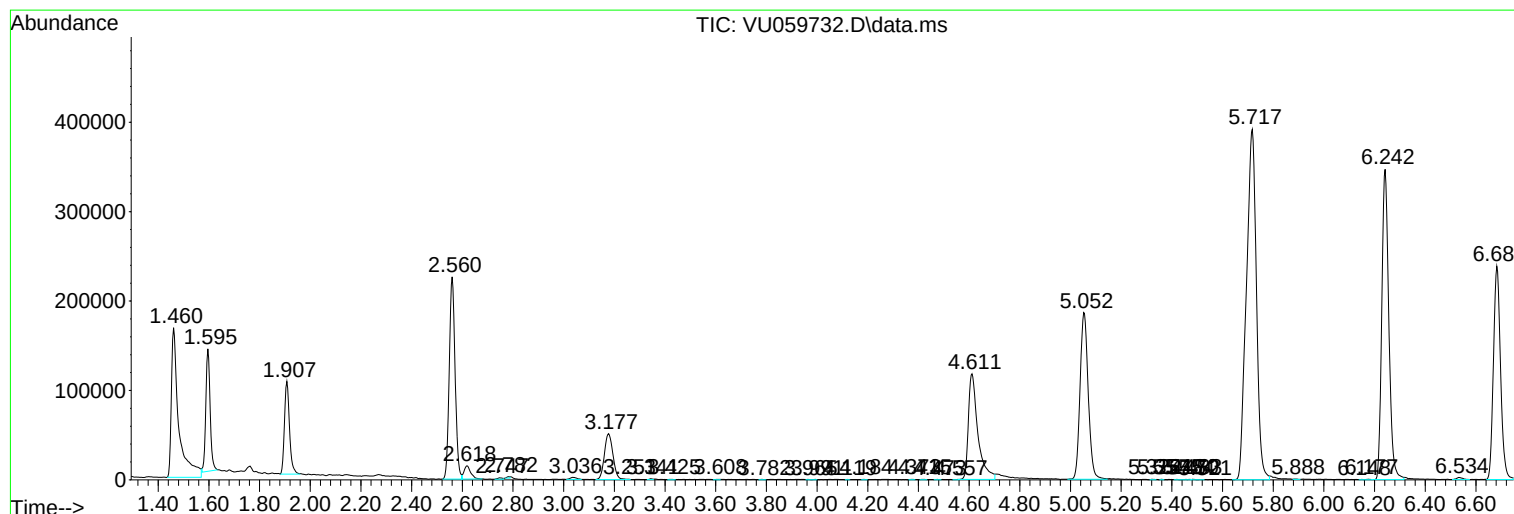

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059732.D
Acq On : 02 Jul 2024 12:28
Operator : MD/SY
Sample : P3091-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059732.D
Acq On : 02 Jul 2024 12:28
Operator : MD/SY
Sample : P3091-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------