

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059734.D
 Acq On : 02 Jul 2024 13:12
 Operator : MD/SY
 Sample : P3108-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	109	rBV	130018	150661	3.21%	1.069%
2	1.730	132	137	140	rBV3	2868	2961	0.06%	0.021%
3	1.907	184	192	212	rVB	100031	137571	2.93%	0.976%
4	2.560	382	395	406	rBV	215685	349694	7.46%	2.481%
5	2.618	406	413	432	rVB2	18495	32308	0.69%	0.229%
6	2.747	444	453	463	rBV3	5996	11787	0.25%	0.084%
7	2.843	480	483	485	rBV	299	201	0.00%	0.001%
8	3.039	532	544	553	rBV5	2351	4202	0.09%	0.030%
9	3.177	571	587	608	rVB	23414	54105	1.15%	0.384%
10	3.290	619	622	623	rBV	296	192	0.00%	0.001%
11	3.341	635	638	640	rBV2	309	225	0.00%	0.002%
12	3.396	646	655	659	rBV2	302	476	0.01%	0.003%
13	3.531	694	697	702	rVB2	293	274	0.01%	0.002%
14	3.557	702	705	707	rBV2	387	274	0.01%	0.002%
15	3.673	738	741	747	rVB2	222	231	0.00%	0.002%
16	3.721	752	756	760	rBV2	221	191	0.00%	0.001%
17	3.856	796	798	804	rVB2	269	243	0.01%	0.002%
18	3.991	836	840	843	rBV	269	227	0.00%	0.002%
19	4.203	904	906	910	rVB	299	231	0.00%	0.002%
20	4.306	934	938	944	rVB2	224	281	0.01%	0.002%
21	4.409	967	970	973	rVB2	271	222	0.00%	0.002%
22	4.608	1018	1032	1060	rBV	110455	286334	6.11%	2.032%
23	5.052	1154	1170	1193	rBV	181275	399168	8.51%	2.832%
24	5.216	1219	1221	1223	rVV	423	205	0.00%	0.001%
25	5.229	1223	1225	1230	rVB	339	233	0.00%	0.002%
26	5.277	1238	1240	1244	rVB2	372	255	0.01%	0.002%
27	5.357	1260	1265	1266	rBV	349	279	0.01%	0.002%
28	5.367	1266	1268	1271	rVV2	385	256	0.01%	0.002%
29	5.460	1294	1297	1302	rBV2	264	256	0.01%	0.002%
30	5.573	1329	1332	1337	rBV	284	278	0.01%	0.002%
31	5.714	1352	1376	1413	rBV2	382307	1075825	22.95%	7.634%
32	5.881	1426	1428	1432	rBV3	311	218	0.00%	0.002%
33	6.168	1510	1517	1523	rBV3	520	886	0.02%	0.006%
34	6.242	1523	1540	1564	rBV	339271	659766	14.07%	4.682%
35	6.531	1622	1630	1642	rVB7	1565	2718	0.06%	0.019%
36	6.682	1662	1677	1707	rBV	226823	452442	9.65%	3.210%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059734.D
 Acq On : 02 Jul 2024 13:12
 Operator : MD/SY
 Sample : P3108-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.804	1712	1715	1719	rVB	344	260	0.01%	0.002%
38	6.865	1731	1734	1738	rBV2	328	225	0.00%	0.002%
39	7.164	1822	1827	1829	rBV2	271	203	0.00%	0.001%
40	7.203	1833	1839	1844	rBV3	453	698	0.01%	0.005%
41	7.396	1895	1899	1902	rBV	242	212	0.00%	0.002%
42	7.457	1914	1918	1923	rVB2	208	242	0.01%	0.002%
43	7.496	1926	1930	1934	rBV	257	304	0.01%	0.002%
44	7.560	1937	1950	1972	rBV	126165	225314	4.81%	1.599%
45	7.788	2015	2021	2022	rBV	243	208	0.00%	0.001%
46	7.891	2039	2053	2073	rBV	475312	827273	17.65%	5.870%
47	8.129	2122	2127	2130	rBV3	275	257	0.01%	0.002%
48	8.174	2130	2141	2159	rBV	86310	149935	3.20%	1.064%
49	8.467	2222	2232	2240	rVB3	1584	2547	0.05%	0.018%
50	8.547	2252	2257	2267	rBV6	1153	1670	0.04%	0.012%
51	8.624	2270	2281	2313	rBV	264900	496005	10.58%	3.520%
52	8.968	2386	2388	2394	rVB2	287	221	0.00%	0.002%
53	9.042	2405	2411	2415	rBV2	192	211	0.00%	0.001%
54	9.203	2456	2461	2464	rBV	193	223	0.00%	0.002%
55	9.409	2513	2525	2531	rBV	502958	854458	18.23%	6.063%
56	9.611	2585	2588	2594	rVB3	818	704	0.02%	0.005%
57	9.647	2594	2599	2601	rBV	233	250	0.01%	0.002%
58	9.698	2606	2615	2631	rVB3	2612	4445	0.09%	0.032%
59	9.862	2661	2666	2670	rBV2	297	420	0.01%	0.003%
60	9.917	2679	2683	2688	rBV2	257	312	0.01%	0.002%
61	10.065	2726	2729	2734	rVB	244	207	0.00%	0.001%
62	10.103	2734	2741	2743	rBV4	904	1013	0.02%	0.007%
63	10.116	2743	2745	2753	rVB5	755	666	0.01%	0.005%
64	10.360	2817	2821	2826	rBV2	165	193	0.00%	0.001%
65	10.489	2855	2861	2865	rBV2	604	798	0.02%	0.006%
66	10.746	2929	2941	2966	rBV	337501	549818	11.73%	3.901%
67	10.891	2977	2986	2994	rVB3	2280	3721	0.08%	0.026%
68	11.097	3046	3050	3052	rBV	316	227	0.00%	0.002%
69	11.473	3159	3167	3172	rVB2	926	1283	0.03%	0.009%
70	11.740	3239	3250	3260	rBV2	92568	143710	3.07%	1.020%
71	11.804	3260	3270	3303	rVB2	507081	1037496	22.13%	7.362%
72	12.068	3342	3352	3367	rBV7	6541	14838	0.32%	0.105%
73	12.203	3376	3394	3425	rBV3	2536702	4688114	100.00%	33.266%
74	12.531	3492	3496	3502	rVB2	397	355	0.01%	0.003%
75	12.682	3538	3543	3545	rBV3	304	292	0.01%	0.002%
76	12.772	3565	3571	3576	rVV3	828	1061	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059734.D
 Acq On : 02 Jul 2024 13:12
 Operator : MD/SY
 Sample : P3108-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.833	3587	3590	3595	rVB3	349	275	0.01%	0.002%
78	12.862	3595	3599	3602	rBV2	334	300	0.01%	0.002%
79	13.000	3638	3642	3649	rVB3	564	570	0.01%	0.004%
80	13.206	3694	3706	3720	rBV2	28659	53176	1.13%	0.377%
81	13.322	3732	3742	3751	rVB6	3997	6038	0.13%	0.043%
82	13.450	3780	3782	3785	rBV	341	224	0.00%	0.002%
83	13.492	3792	3795	3798	rBV2	377	262	0.01%	0.002%
84	13.518	3798	3803	3805	rBV3	414	351	0.01%	0.002%
85	13.646	3839	3843	3844	rBV	273	208	0.00%	0.001%
86	13.685	3853	3855	3862	rBV3	298	341	0.01%	0.002%
87	13.772	3878	3882	3884	rVB2	330	256	0.01%	0.002%
88	13.833	3886	3901	3921	rBV	560859	881024	18.79%	6.252%
89	13.933	3929	3932	3938	rBV3	432	457	0.01%	0.003%
90	14.090	3971	3981	3991	rBV	3715	6214	0.13%	0.044%
91	14.219	4019	4021	4024	rBV2	423	245	0.01%	0.002%
92	14.322	4040	4053	4073	rBV	264996	428399	9.14%	3.040%
93	14.521	4110	4115	4117	rBV2	458	473	0.01%	0.003%
94	14.730	4171	4180	4195	rVV3	8661	16517	0.35%	0.117%
95	14.843	4209	4215	4216	rBV3	738	637	0.01%	0.005%
96	15.244	4338	4340	4344	rBV3	521	398	0.01%	0.003%
97	15.412	4386	4392	4400	rVB4	6112	8426	0.18%	0.060%
98	15.515	4422	4424	4427	rBV2	468	242	0.01%	0.002%
99	15.698	4478	4481	4483	rBV2	554	372	0.01%	0.003%
100	15.994	4563	4573	4586	rBV2	31900	51344	1.10%	0.364%




Sum of corrected areas: 14092814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059734.D
Acq On : 02 Jul 2024 13:12
Operator : MD/SY
Sample : P3108-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ST5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

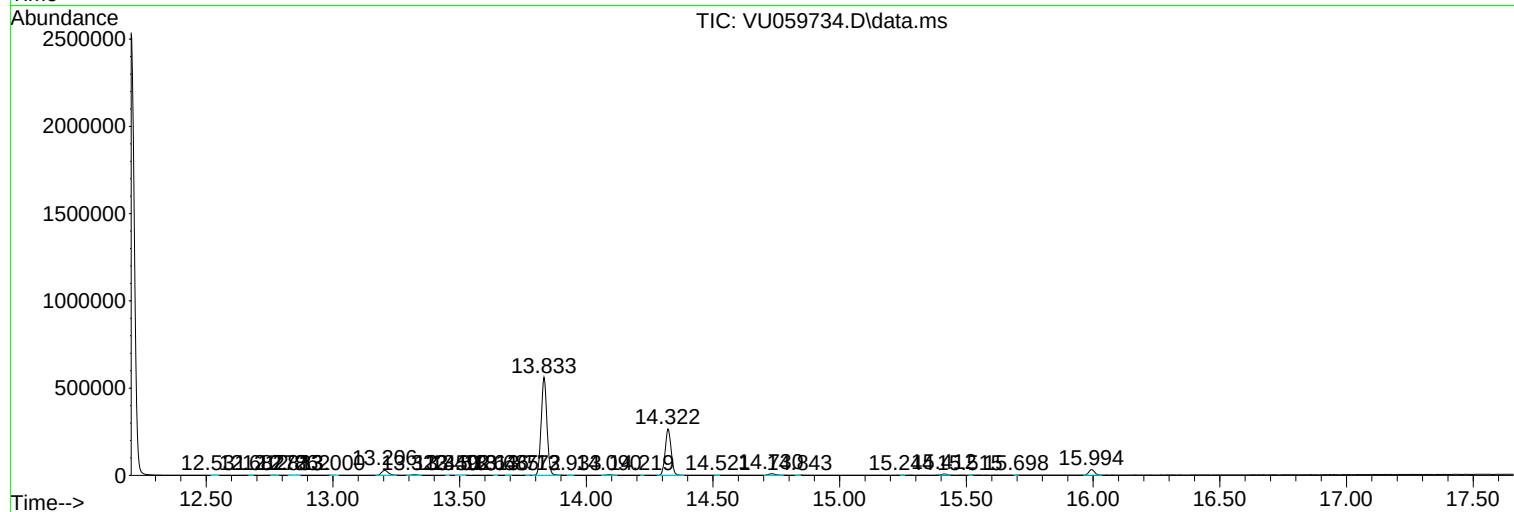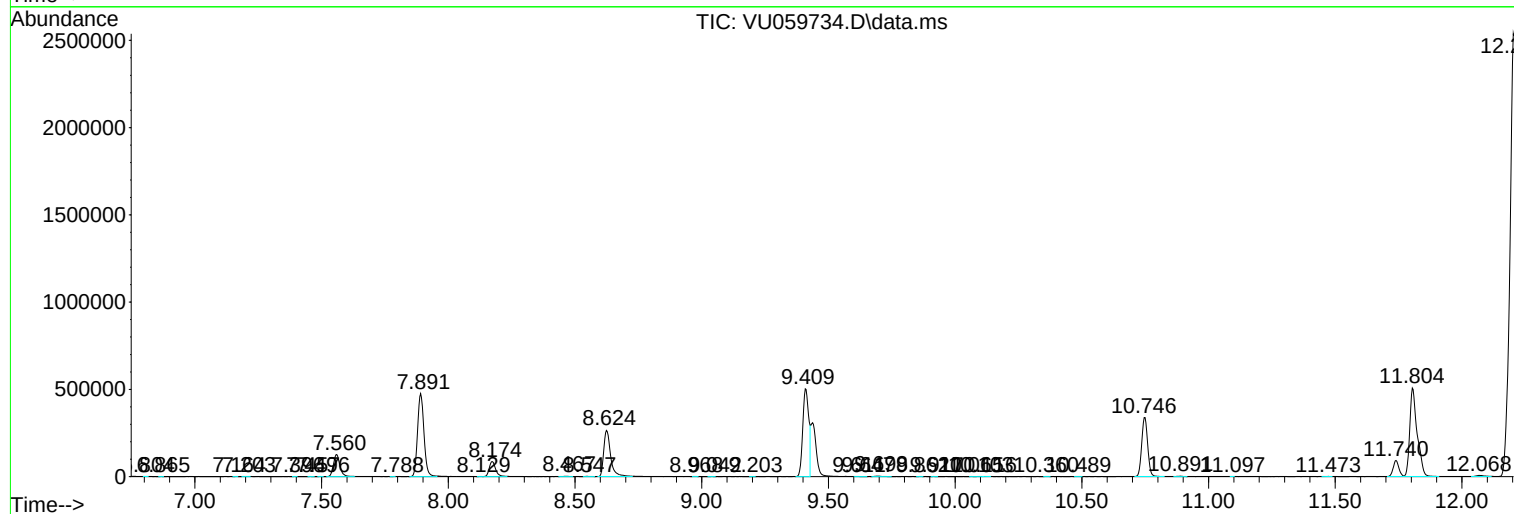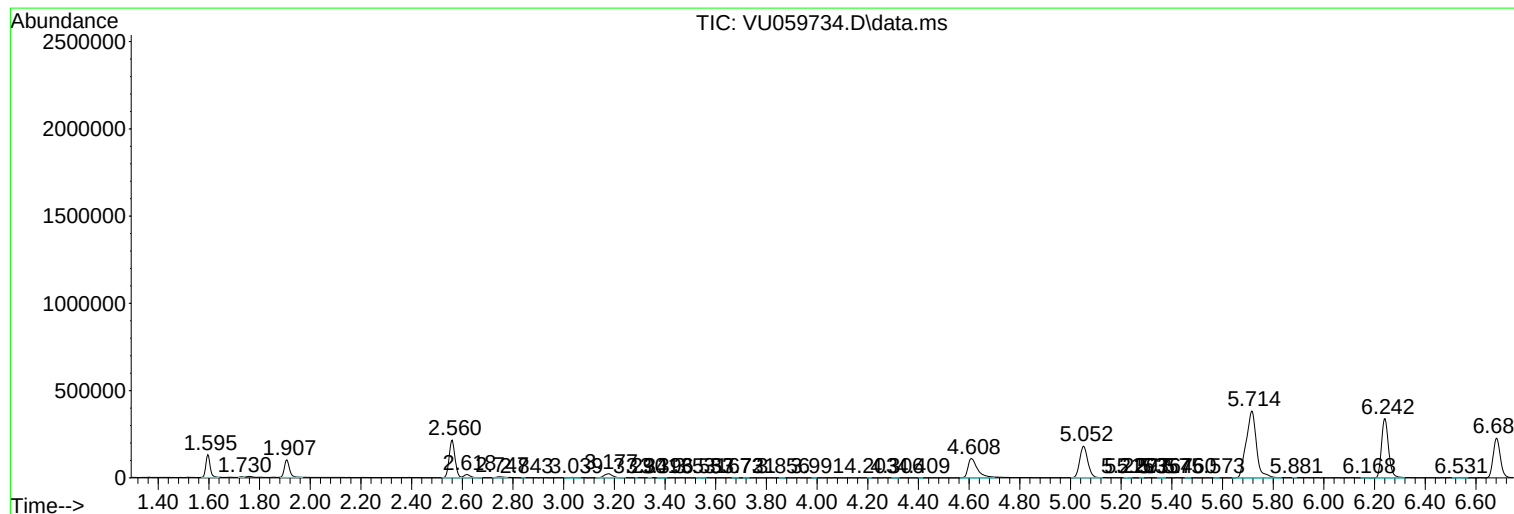

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059734.D
Acq On : 02 Jul 2024 13:12
Operator : MD/SY
Sample : P3108-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ST5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059734.D
Acq On : 02 Jul 2024 13:12
Operator : MD/SY
Sample : P3108-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ST5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------