

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059740.D
 Acq On : 02 Jul 2024 15:29
 Operator : MD/SY
 Sample : P3108-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU059740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	112	rVB	111464	131605	9.90%	1.584%
2	1.908	184	192	205	rBV	88051	120201	9.05%	1.447%
3	2.560	382	395	408	rBV	185732	305482	22.99%	3.677%
4	2.695	435	437	441	rBV2	311	225	0.02%	0.003%
5	3.039	535	544	557	rVB4	5227	10323	0.78%	0.124%
6	3.252	605	610	617	rBV2	244	306	0.02%	0.004%
7	3.380	647	650	652	rVB	235	125	0.01%	0.002%
8	3.396	652	655	657	rBV2	243	188	0.01%	0.002%
9	3.570	707	709	711	rBV	190	74	0.01%	0.001%
10	3.657	732	736	740	rVB	272	239	0.02%	0.003%
11	3.824	784	788	792	rVB	151	179	0.01%	0.002%
12	3.846	792	795	798	rBV	247	203	0.02%	0.002%
13	3.862	798	800	803	rBV	196	128	0.01%	0.002%
14	3.901	810	812	816	rBB2	234	164	0.01%	0.002%
15	4.120	877	880	886	rBV2	289	244	0.02%	0.003%
16	4.190	901	902	905	rBV2	133	75	0.01%	0.001%
17	4.316	933	941	946	rBV2	298	548	0.04%	0.007%
18	4.422	972	974	978	rBV	158	111	0.01%	0.001%
19	4.612	1017	1033	1070	rBV2	90592	231571	17.43%	2.788%
20	5.055	1152	1171	1199	rBV	162662	361396	27.20%	4.350%
21	5.358	1261	1265	1267	rBV3	333	256	0.02%	0.003%
22	5.457	1294	1296	1298	rBV2	148	98	0.01%	0.001%
23	5.470	1298	1300	1302	rVV2	291	165	0.01%	0.002%
24	5.486	1302	1305	1307	rVB2	185	123	0.01%	0.001%
25	5.608	1338	1343	1345	rBV2	319	239	0.02%	0.003%
26	5.718	1356	1377	1409	rBV2	336217	918194	69.10%	11.053%
27	5.920	1438	1440	1445	rVB2	417	269	0.02%	0.003%
28	5.943	1445	1447	1449	rBV	334	200	0.02%	0.002%
29	6.030	1470	1474	1477	rVB2	318	245	0.02%	0.003%
30	6.052	1477	1481	1483	rBV3	279	261	0.02%	0.003%
31	6.113	1498	1500	1503	rBV	348	222	0.02%	0.003%
32	6.136	1503	1507	1509	rBV	253	118	0.01%	0.001%
33	6.168	1514	1517	1518	rBV2	262	171	0.01%	0.002%
34	6.242	1527	1540	1558	rBV	321937	616946	46.43%	7.427%
35	6.521	1620	1627	1628	rBV3	1343	1166	0.09%	0.014%
36	6.637	1660	1663	1664	rBV	194	127	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059740.D
 Acq On : 02 Jul 2024 15:29
 Operator : MD/SY
 Sample : P3108-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.682	1664	1677	1706	rVV	203757	403736	30.38%	4.860%
38	6.833	1723	1724	1726	rVB2	242	70	0.01%	0.001%
39	6.859	1729	1732	1734	rVB2	253	100	0.01%	0.001%
40	6.898	1740	1744	1746	rBV	312	179	0.01%	0.002%
41	6.968	1763	1766	1768	rBV2	193	166	0.01%	0.002%
42	7.026	1781	1784	1787	rBV	178	107	0.01%	0.001%
43	7.052	1787	1792	1797	rBV2	261	249	0.02%	0.003%
44	7.139	1816	1819	1823	rVB2	247	197	0.01%	0.002%
45	7.181	1829	1832	1834	rBV2	281	224	0.02%	0.003%
46	7.261	1854	1857	1860	rVB	220	137	0.01%	0.002%
47	7.277	1860	1862	1863	rBV	170	69	0.01%	0.001%
48	7.293	1865	1867	1870	rBV2	157	81	0.01%	0.001%
49	7.354	1880	1886	1889	rBV2	276	314	0.02%	0.004%
50	7.374	1889	1892	1895	rBV2	227	205	0.02%	0.002%
51	7.447	1912	1915	1918	rBV	223	172	0.01%	0.002%
52	7.499	1929	1931	1933	rVB	220	88	0.01%	0.001%
53	7.521	1933	1938	1939	rBV2	312	303	0.02%	0.004%
54	7.560	1939	1950	1971	rVV	108101	195124	14.68%	2.349%
55	7.779	2015	2018	2021	rBV	216	153	0.01%	0.002%
56	7.891	2040	2053	2075	rBV	414812	718840	54.10%	8.653%
57	8.123	2124	2125	2131	rVB2	199	123	0.01%	0.001%
58	8.174	2131	2141	2163	rBV2	74672	130729	9.84%	1.574%
59	8.351	2193	2196	2198	rBV	271	157	0.01%	0.002%
60	8.370	2198	2202	2205	rVB2	329	263	0.02%	0.003%
61	8.402	2209	2212	2213	rBV	290	130	0.01%	0.002%
62	8.454	2225	2228	2229	rBV2	537	307	0.02%	0.004%
63	8.541	2251	2255	2257	rBV2	509	390	0.03%	0.005%
64	8.628	2270	2282	2316	rBV	235980	440968	33.19%	5.308%
65	8.898	2364	2366	2372	rVB2	501	328	0.02%	0.004%
66	8.923	2372	2374	2377	rVB	310	180	0.01%	0.002%
67	8.946	2379	2381	2383	rBV	168	68	0.01%	0.001%
68	9.045	2409	2412	2414	rBV2	266	182	0.01%	0.002%
69	9.209	2460	2463	2467	rBV2	196	171	0.01%	0.002%
70	9.264	2476	2480	2482	rBV	199	132	0.01%	0.002%
71	9.316	2492	2496	2499	rVB2	189	167	0.01%	0.002%
72	9.345	2500	2505	2508	rBV2	247	233	0.02%	0.003%
73	9.412	2514	2526	2557	rBV	468106	884257	66.55%	10.645%
74	9.611	2584	2588	2594	rBV3	657	717	0.05%	0.009%
75	9.695	2607	2614	2625	rVB4	1549	2637	0.20%	0.032%
76	9.936	2683	2689	2690	rBV2	147	178	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059740.D
 Acq On : 02 Jul 2024 15:29
 Operator : MD/SY
 Sample : P3108-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ST5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.062	2725	2728	2730	rBV	171	145	0.01%	0.002%
78	10.203	2768	2772	2777	rBV	352	350	0.03%	0.004%
79	10.299	2800	2802	2804	rBV	195	97	0.01%	0.001%
80	10.631	2901	2905	2906	rBV	164	135	0.01%	0.002%
81	10.701	2924	2927	2929	rBV	316	222	0.02%	0.003%
82	10.750	2929	2942	2964	rVV	305206	501962	37.78%	6.043%
83	10.885	2976	2984	2987	rBV2	942	1042	0.08%	0.013%
84	11.068	3038	3041	3046	rBV	235	266	0.02%	0.003%
85	11.135	3059	3062	3065	rBV2	324	263	0.02%	0.003%
86	11.174	3072	3074	3078	rBV2	151	153	0.01%	0.002%
87	11.261	3098	3101	3103	rBV2	240	168	0.01%	0.002%
88	11.666	3222	3227	3234	rBV2	312	496	0.04%	0.006%
89	11.743	3241	3251	3259	rBV2	15702	23628	1.78%	0.284%
90	11.807	3260	3271	3298	rVB	450117	763168	57.43%	9.187%
91	12.007	3330	3333	3339	rVB2	469	381	0.03%	0.005%
92	12.081	3352	3356	3360	rBV2	913	801	0.06%	0.010%
93	12.196	3377	3392	3419	rBV2	542648	1328752	100.00%	15.995%
94	12.975	3631	3634	3635	rBV2	293	178	0.01%	0.002%
95	13.219	3702	3710	3718	rBV4	3481	5710	0.43%	0.069%
96	13.331	3741	3745	3748	rBV3	649	611	0.05%	0.007%
97	13.592	3821	3826	3830	rBV2	385	491	0.04%	0.006%
98	13.836	3892	3902	3918	rBV2	81005	130266	9.80%	1.568%
99	13.965	3938	3942	3948	rBV3	568	678	0.05%	0.008%
100	14.328	4043	4055	4068	rBV2	37013	62176	4.68%	0.748%




Sum of corrected areas: 8307157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059740.D
Acq On : 02 Jul 2024 15:29
Operator : MD/SY
Sample : P3108-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C05T5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

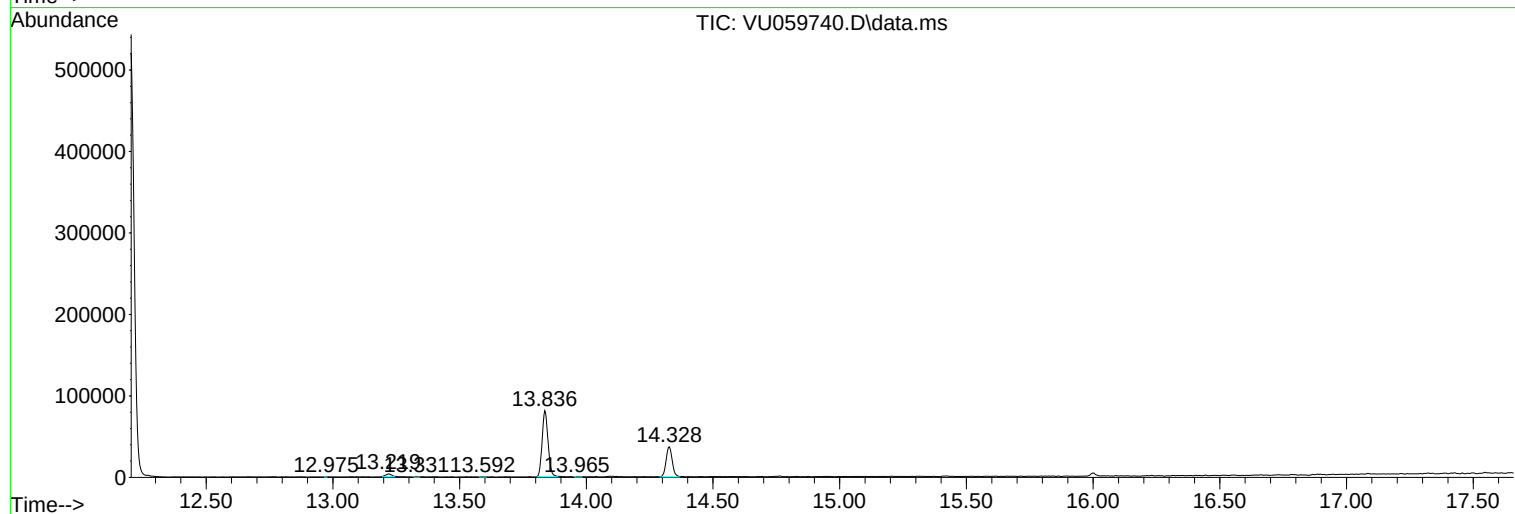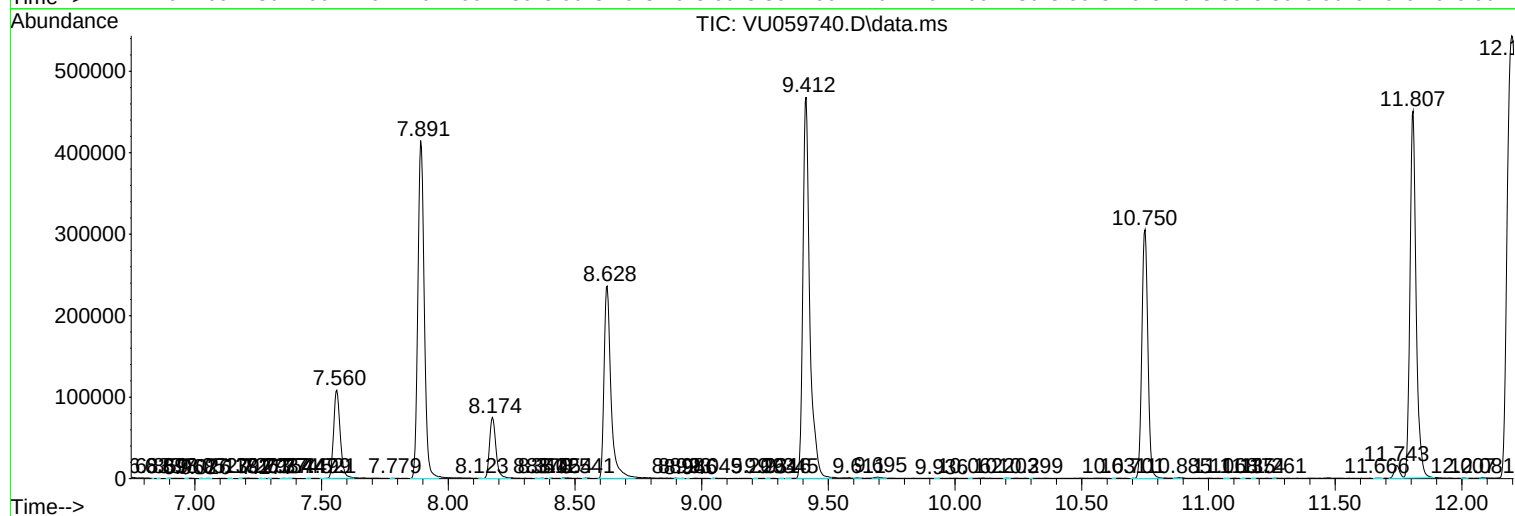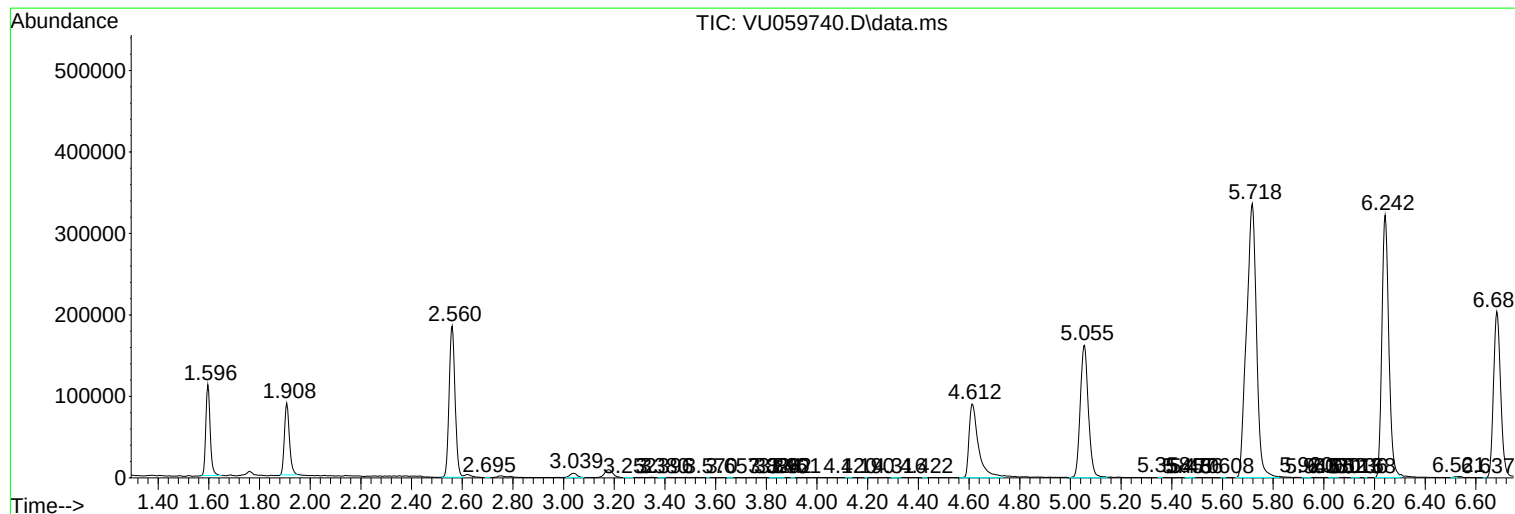

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059740.D
Acq On : 02 Jul 2024 15:29
Operator : MD/SY
Sample : P3108-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ST5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059740.D
Acq On : 02 Jul 2024 15:29
Operator : MD/SY
Sample : P3108-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ST5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------