

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059745.D
 Acq On : 02 Jul 2024 17:29
 Operator : MD/SY
 Sample : P3091-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	110	rBV	110743	129238	14.52%	1.894%
2	1.907	184	192	212	rVB	86025	119018	13.37%	1.744%
3	2.560	383	395	416	rBV	176743	288968	32.46%	4.235%
4	2.689	433	435	437	rBV	255	108	0.01%	0.002%
5	3.042	535	545	557	rVB5	2744	5518	0.62%	0.081%
6	3.103	561	564	568	rVB2	283	193	0.02%	0.003%
7	3.393	651	654	658	rBV2	194	162	0.02%	0.002%
8	3.785	773	776	778	rBV	198	139	0.02%	0.002%
9	3.836	789	792	796	rBV	346	324	0.04%	0.005%
10	3.888	804	808	813	rBV2	235	204	0.02%	0.003%
11	3.917	813	817	820	rBV2	189	167	0.02%	0.002%
12	3.968	829	833	835	rBV	207	166	0.02%	0.002%
13	4.000	840	843	845	rBV2	231	134	0.02%	0.002%
14	4.126	880	882	887	rBV	203	201	0.02%	0.003%
15	4.248	917	920	924	rVB2	279	218	0.02%	0.003%
16	4.290	927	933	935	rBV	239	266	0.03%	0.004%
17	4.435	975	978	981	rVB	194	157	0.02%	0.002%
18	4.454	981	984	985	rBV	157	98	0.01%	0.001%
19	4.470	986	989	993	rBV	214	137	0.02%	0.002%
20	4.492	993	996	1001	rBV	191	190	0.02%	0.003%
21	4.573	1019	1021	1023	rBV	265	106	0.01%	0.002%
22	4.611	1023	1033	1069	rBV	84426	212346	23.86%	3.112%
23	4.997	1150	1153	1155	rBV	265	214	0.02%	0.003%
24	5.052	1156	1170	1194	rVV	156214	346457	38.92%	5.077%
25	5.245	1228	1230	1233	rBV2	325	217	0.02%	0.003%
26	5.283	1239	1242	1244	rVB2	406	245	0.03%	0.004%
27	5.299	1244	1247	1250	rBV2	176	142	0.02%	0.002%
28	5.364	1263	1267	1269	rBV2	375	271	0.03%	0.004%
29	5.428	1284	1287	1290	rVV2	222	149	0.02%	0.002%
30	5.447	1290	1293	1298	rVB2	317	293	0.03%	0.004%
31	5.480	1299	1303	1306	rBV2	210	215	0.02%	0.003%
32	5.518	1313	1315	1319	rVB	219	114	0.01%	0.002%
33	5.563	1326	1329	1332	rBV	161	124	0.01%	0.002%
34	5.618	1343	1346	1349	rBV2	264	160	0.02%	0.002%
35	5.717	1356	1377	1410	rBV2	322282	890136	100.00%	13.044%
36	5.981	1456	1459	1463	rBV3	306	275	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059745.D
 Acq On : 02 Jul 2024 17:29
 Operator : MD/SY
 Sample : P3091-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.042	1475	1478	1480	rBV	340	239	0.03%	0.004%
38	6.161	1511	1515	1519	rBV3	351	276	0.03%	0.004%
39	6.242	1528	1540	1565	rBV	281478	542883	60.99%	7.955%
40	6.505	1619	1622	1623	rBV2	300	131	0.01%	0.002%
41	6.534	1623	1631	1636	rBV5	1588	2808	0.32%	0.041%
42	6.682	1664	1677	1699	rBV	201764	394035	44.27%	5.774%
43	6.814	1717	1718	1725	rVB4	419	287	0.03%	0.004%
44	6.878	1735	1738	1741	rVB2	195	114	0.01%	0.002%
45	6.904	1742	1746	1752	rBV	250	277	0.03%	0.004%
46	6.952	1757	1761	1765	rBV2	160	128	0.01%	0.002%
47	6.984	1768	1771	1775	rBV2	286	190	0.02%	0.003%
48	7.097	1804	1806	1810	rVB2	249	119	0.01%	0.002%
49	7.274	1853	1861	1863	rBV2	223	249	0.03%	0.004%
50	7.299	1867	1869	1872	rVB2	231	147	0.02%	0.002%
51	7.322	1872	1876	1879	rBV	240	137	0.02%	0.002%
52	7.344	1879	1883	1885	rBV2	246	223	0.03%	0.003%
53	7.560	1938	1950	1972	rBV	102505	186092	20.91%	2.727%
54	7.750	2005	2009	2016	rBV2	328	294	0.03%	0.004%
55	7.891	2041	2053	2072	rBV	397270	689193	77.43%	10.100%
56	8.132	2126	2128	2130	rBV	211	104	0.01%	0.002%
57	8.174	2130	2141	2158	rBV2	71730	123785	13.91%	1.814%
58	8.351	2190	2196	2199	rBV	249	309	0.03%	0.005%
59	8.409	2210	2214	2218	rBV2	232	237	0.03%	0.003%
60	8.502	2239	2243	2249	rBV	285	336	0.04%	0.005%
61	8.547	2253	2257	2265	rVB4	1840	2514	0.28%	0.037%
62	8.627	2271	2282	2321	rBV	228057	435857	48.97%	6.387%
63	8.926	2372	2375	2377	rBV2	253	115	0.01%	0.002%
64	8.987	2392	2394	2395	rBV	219	114	0.01%	0.002%
65	9.196	2457	2459	2462	rBV	172	99	0.01%	0.001%
66	9.251	2473	2476	2480	rBV	180	168	0.02%	0.002%
67	9.293	2484	2489	2490	rBV2	176	181	0.02%	0.003%
68	9.335	2497	2502	2505	rBV	275	270	0.03%	0.004%
69	9.412	2513	2526	2559	rBV	414470	703206	79.00%	10.305%
70	9.695	2603	2614	2621	rBV4	1615	3184	0.36%	0.047%
71	9.775	2635	2639	2643	rBV	286	200	0.02%	0.003%
72	9.846	2657	2661	2667	rVB	229	271	0.03%	0.004%
73	9.878	2668	2671	2673	rBV2	177	134	0.02%	0.002%
74	9.965	2695	2698	2702	rVB2	313	212	0.02%	0.003%
75	10.029	2715	2718	2720	rBV2	184	121	0.01%	0.002%
76	10.093	2734	2738	2745	rBV3	497	684	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
 Data File : VU059745.D
 Acq On : 02 Jul 2024 17:29
 Operator : MD/SY
 Sample : P3091-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.290	2797	2799	2803	rVB	228	124	0.01%	0.002%
78	10.354	2816	2819	2824	rBV2	231	267	0.03%	0.004%
79	10.466	2851	2854	2856	rBV2	377	242	0.03%	0.004%
80	10.630	2904	2905	2910	rBV2	140	89	0.01%	0.001%
81	10.675	2916	2919	2922	rBV2	308	247	0.03%	0.004%
82	10.749	2929	2942	2961	rBV	300196	489549	55.00%	7.174%
83	10.878	2977	2982	2985	rBV	454	314	0.04%	0.005%
84	10.994	3015	3018	3020	rBV	221	142	0.02%	0.002%
85	11.142	3061	3064	3067	rBV2	202	139	0.02%	0.002%
86	11.190	3073	3079	3082	rBV2	249	298	0.03%	0.004%
87	11.209	3082	3085	3089	rBV	248	201	0.02%	0.003%
88	11.421	3149	3151	3155	rVB2	214	143	0.02%	0.002%
89	11.470	3162	3166	3167	rBV2	431	305	0.03%	0.004%
90	11.553	3189	3192	3196	rBV2	294	252	0.03%	0.004%
91	11.611	3208	3210	3213	rBV2	199	161	0.02%	0.002%
92	11.749	3247	3253	3259	rBV4	974	1418	0.16%	0.021%
93	11.807	3259	3271	3290	rBV	377726	622784	69.97%	9.126%
94	12.187	3377	3389	3415	rBV	368749	617750	69.40%	9.053%
95	12.688	3542	3545	3547	rBV	352	209	0.02%	0.003%
96	12.936	3619	3622	3624	rBV	344	251	0.03%	0.004%
97	13.412	3767	3770	3771	rBV	341	205	0.02%	0.003%
98	13.862	3903	3910	3918	rVB3	964	1195	0.13%	0.018%
99	14.248	4027	4030	4033	rBV	400	261	0.03%	0.004%
100	14.341	4054	4059	4060	rBV3	650	479	0.05%	0.007%


Sum of corrected areas: 6824018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059745.D
Acq On : 02 Jul 2024 17:29
Operator : MD/SY
Sample : P3091-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

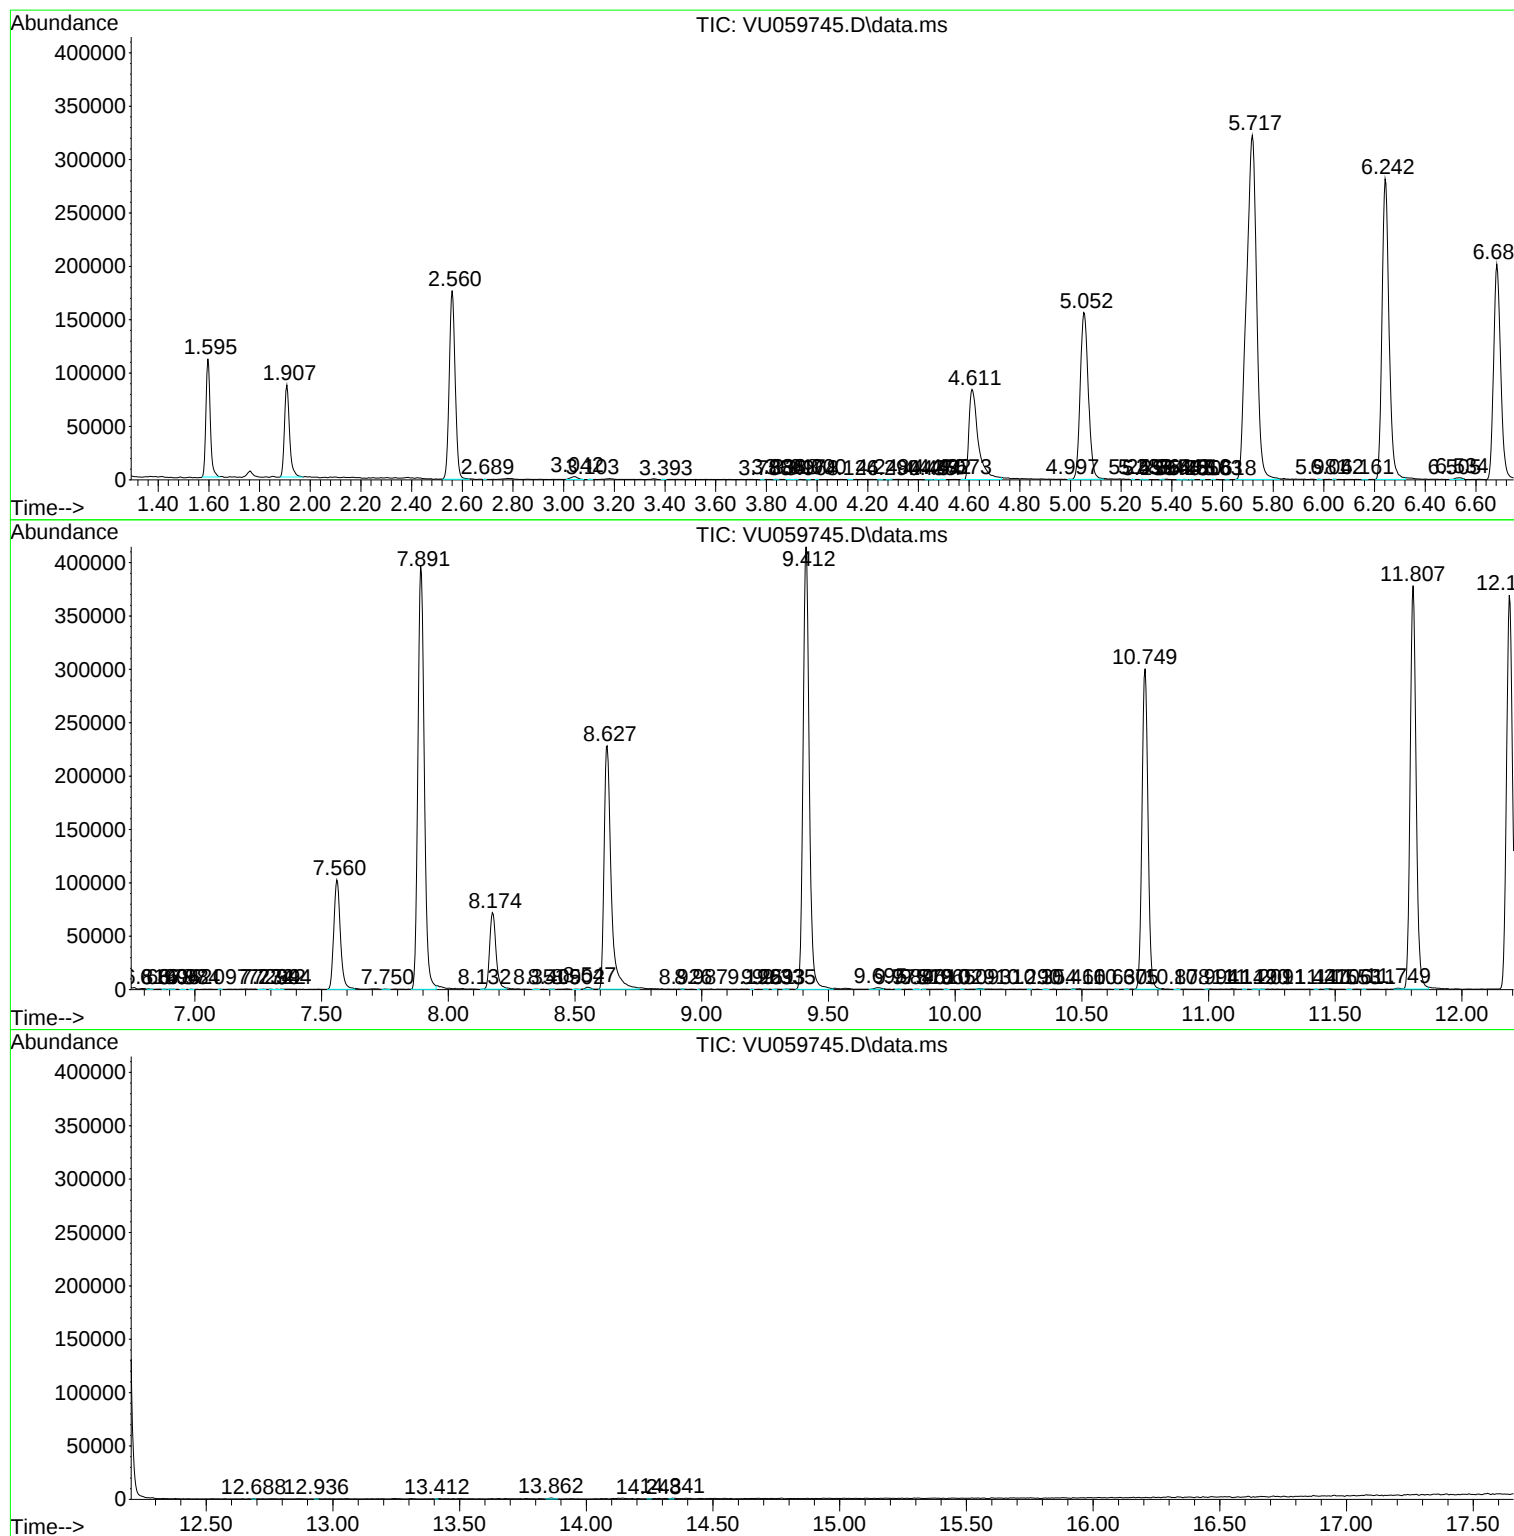

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059745.D
Acq On : 02 Jul 2024 17:29
Operator : MD/SY
Sample : P3091-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059745.D
Acq On : 02 Jul 2024 17:29
Operator : MD/SY
Sample : P3091-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc