


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070224\
Data File : VU059723.D
Acq On : 02 Jul 2024 07:54
Operator : MD/SY
Sample : BFB070
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB070

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Wed Jul 03 01:39:57 2024

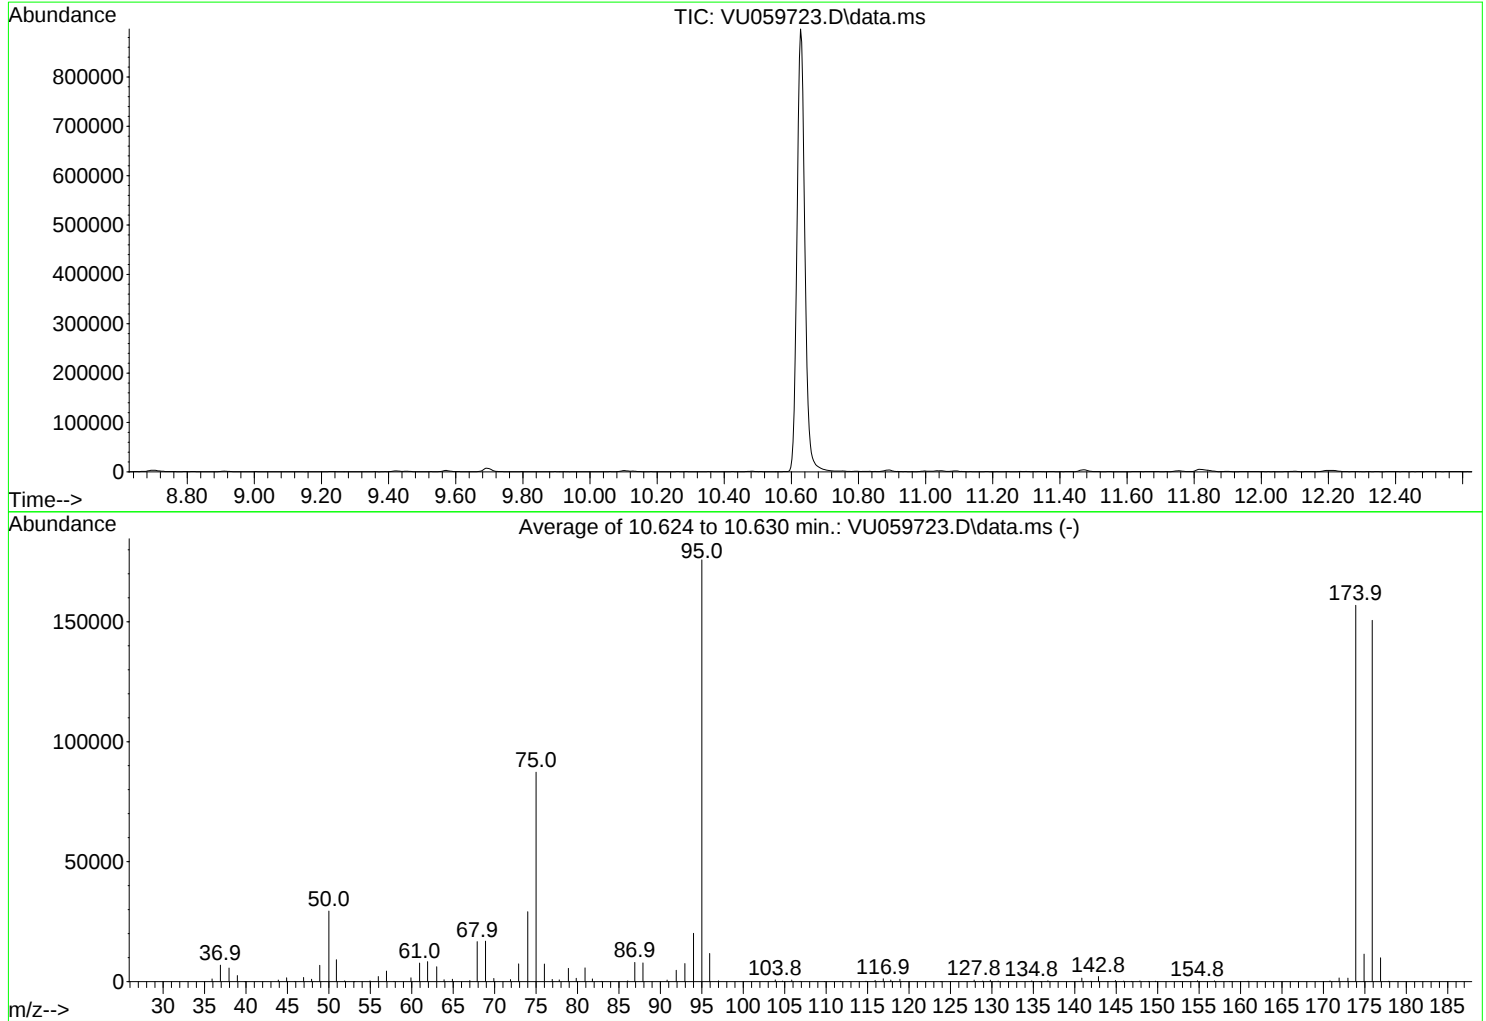

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	29443	PASS
75	95	30	80	49.7	87312	PASS
95	95	100	100	100.0	175808	PASS
96	95	5	9	6.7	11715	PASS
173	174	0.00	2	0.9	1450	PASS
174	95	50	120	89.2	156864	PASS
175	174	5	9	7.3	11511	PASS
176	174	95	101	96.0	150613	PASS
177	176	5	9	6.6	9927	PASS

m/z	Abundance
39.80	189.0
43.90	391.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1056.0
36.90	6564.0
37.90	5520.0
38.90	2559.0
40.00	199.0
43.90	1069.0
44.90	1625.0
45.90	103.0
47.00	1745.0
47.90	941.0
48.90	6753.0
50.00	29088.0
50.90	9046.0
51.90	374.0
55.00	360.0
56.00	2027.0
56.90	4350.0
57.90	149.0
59.90	1731.0
60.90	7918.0
61.90	8380.0
63.00	5965.0
63.90	883.0
64.90	1034.0
67.00	442.0
67.90	16301.0
68.90	16776.0
69.90	1363.0
71.90	892.0
72.90	7106.0
74.00	28952.0
75.00	84112.0
76.00	7210.0
77.00	819.0
77.80	731.0
78.90	5294.0
79.80	1331.0
80.90	5722.0
81.80	1111.0
82.80	142.0
86.00	308.0
86.90	7626.0
87.90	7756.0
90.80	685.0
91.90	4631.0
93.00	7183.0
94.00	19288.0
95.00	170112.0
96.00	11473.0
97.00	345.0
103.90	689.0
104.70	208.0
105.80	709.0
106.80	155.0
111.70	121.0
112.80	144.0
114.80	188.0
115.90	559.0
116.90	1176.0
117.80	611.0
118.90	1017.0
127.90	683.0
128.90	271.0
129.80	534.0
130.80	277.0
134.80	338.0
135.80	101.0
136.70	373.0
140.80	1402.0
142.00	200.0
142.80	2021.0
144.00	104.0
144.90	499.0
145.90	279.0
146.90	116.0
147.90	375.0
148.90	119.0
149.80	203.0
154.80	482.0
156.90	314.0
159.00	149.0
160.90	235.0
170.80	408.0
171.90	1516.0
173.00	1438.0
173.90	148608.0
174.90	10995.0
175.90	143360.0
176.90	9600.0
177.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1164.0
36.90	7154.0
38.00	5851.0
39.00	2683.0
40.00	201.0
43.90	1079.0
44.90	1635.0
45.90	144.0
47.00	1759.0
47.90	1058.0
48.90	7041.0
50.00	30336.0
50.90	9404.0
51.90	367.0
53.00	100.0
54.90	356.0
55.90	2135.0
57.00	4610.0
57.90	158.0
59.90	1686.0
61.00	8005.0
61.90	8616.0
63.00	6392.0
63.90	870.0
64.90	1065.0
67.00	470.0
67.90	17240.0
68.90	17544.0
69.90	1359.0
71.90	907.0
72.90	7587.0
74.00	30248.0
75.00	90184.0
76.00	7566.0
77.00	998.0
77.80	767.0
78.90	5777.0
79.90	1440.0
80.90	5973.0
81.80	1116.0
82.80	141.0
86.00	333.0
86.90	8247.0
87.90	8094.0
90.80	694.0
91.90	4885.0
93.00	7786.0
94.00	20768.0
95.00	181952.0
96.00	12180.0
97.00	318.0
103.90	732.0
104.80	283.0
105.90	702.0
106.80	175.0
109.80	117.0
111.70	165.0
112.80	118.0
114.80	222.0
115.90	539.0
116.90	1209.0
117.80	696.0
118.90	1027.0
127.90	727.0
128.90	261.0
129.80	640.0
130.80	273.0
134.80	331.0
136.80	370.0
140.80	1521.0
141.90	224.0
142.90	2268.0
144.00	100.0
144.90	500.0
145.90	277.0
146.80	127.0
147.90	372.0
148.90	132.0
149.80	220.0
152.80	147.0
154.80	430.0
156.80	322.0
158.90	138.0
160.90	231.0
170.80	336.0
171.90	1572.0
172.90	1510.0
173.90	161984.0
174.90	11796.0
175.90	155136.0
176.90	10240.0
177.90	237.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1147.0
36.90	6893.0
37.90	5725.0
39.00	2422.0
39.90	198.0
43.90	1039.0
44.90	1480.0
45.90	174.0
46.90	1650.0
47.90	976.0
48.90	6619.0
50.00	28904.0
50.90	8976.0
51.90	368.0
55.00	349.0
55.90	2219.0
57.00	4319.0
57.80	191.0
59.90	1478.0
61.00	7350.0
61.90	8041.0
63.00	6279.0
63.90	739.0
64.90	934.0
67.00	490.0
67.90	16440.0
68.90	16362.0
69.90	1236.0
71.90	829.0
72.90	7573.0
74.00	28288.0
75.00	87640.0
76.00	7239.0
76.90	1048.0
77.80	750.0
78.90	5654.0
79.90	1475.0
80.90	5599.0
81.80	1092.0
82.90	133.0
86.10	294.0
86.90	8176.0
87.90	7652.0
90.80	609.0
91.90	4771.0
92.90	7612.0
94.00	20456.0
95.00	175360.0
95.90	11491.0
97.00	303.0
103.80	710.0
104.80	346.0
105.90	681.0
106.90	176.0
109.80	146.0
111.80	172.0
114.80	225.0
115.90	507.0
116.90	1180.0
117.80	684.0
118.90	962.0
123.80	111.0
127.80	681.0
128.90	245.0
129.80	687.0
130.70	230.0
134.80	265.0
136.80	386.0
140.90	1533.0
141.90	214.0
142.90	2207.0
144.90	440.0
145.90	217.0
146.80	119.0
147.80	312.0
148.90	121.0
149.70	211.0
152.80	162.0
154.80	386.0
156.80	294.0
158.70	146.0
160.90	187.0
170.80	208.0
171.90	1562.0
172.90	1403.0
173.90	160000.0
174.90	11741.0
175.90	153344.0
176.90	9942.0
177.90	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070