

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070524\
 Data File : VU059868.D
 Acq On : 05 Jul 2024 19:13
 Operator : MD/SY
 Sample : P3137-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN2

Quant Time: Jul 06 03:06:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 06 02:59:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	137010	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	146534	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	61212	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	41460	4.352	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.000%
7) Chloroethane-d5	1.911	69	40203	4.386	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.560	65	17149	4.339	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.800%
20) 2-Butanone-d5	4.615	46	73001	37.199	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.400%
24) Chloroform-d	5.055	84	90955	4.651	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.695	65	39792	4.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
32) Benzene-d6	5.721	84	169358	4.199	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	6.685	67	54229	4.388	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.800%
41) Toluene-d8	7.894	98	136427	3.639	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.800%
43) trans-1,3-Dichloroprop...	8.177	79	15423	3.986	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.631	63	55357	34.430	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.860%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	39843	3.902	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	52810	4.847	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						Qvalue
13) Acetone	2.621	43	13895	10.915	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070524\
Data File : VU059868.D
Acq On : 05 Jul 2024 19:13
Operator : MD/SY
Sample : P3137-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZN2


Quant Time: Jul 06 03:06:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 06 02:59:52 2024
Response via : Initial Calibration

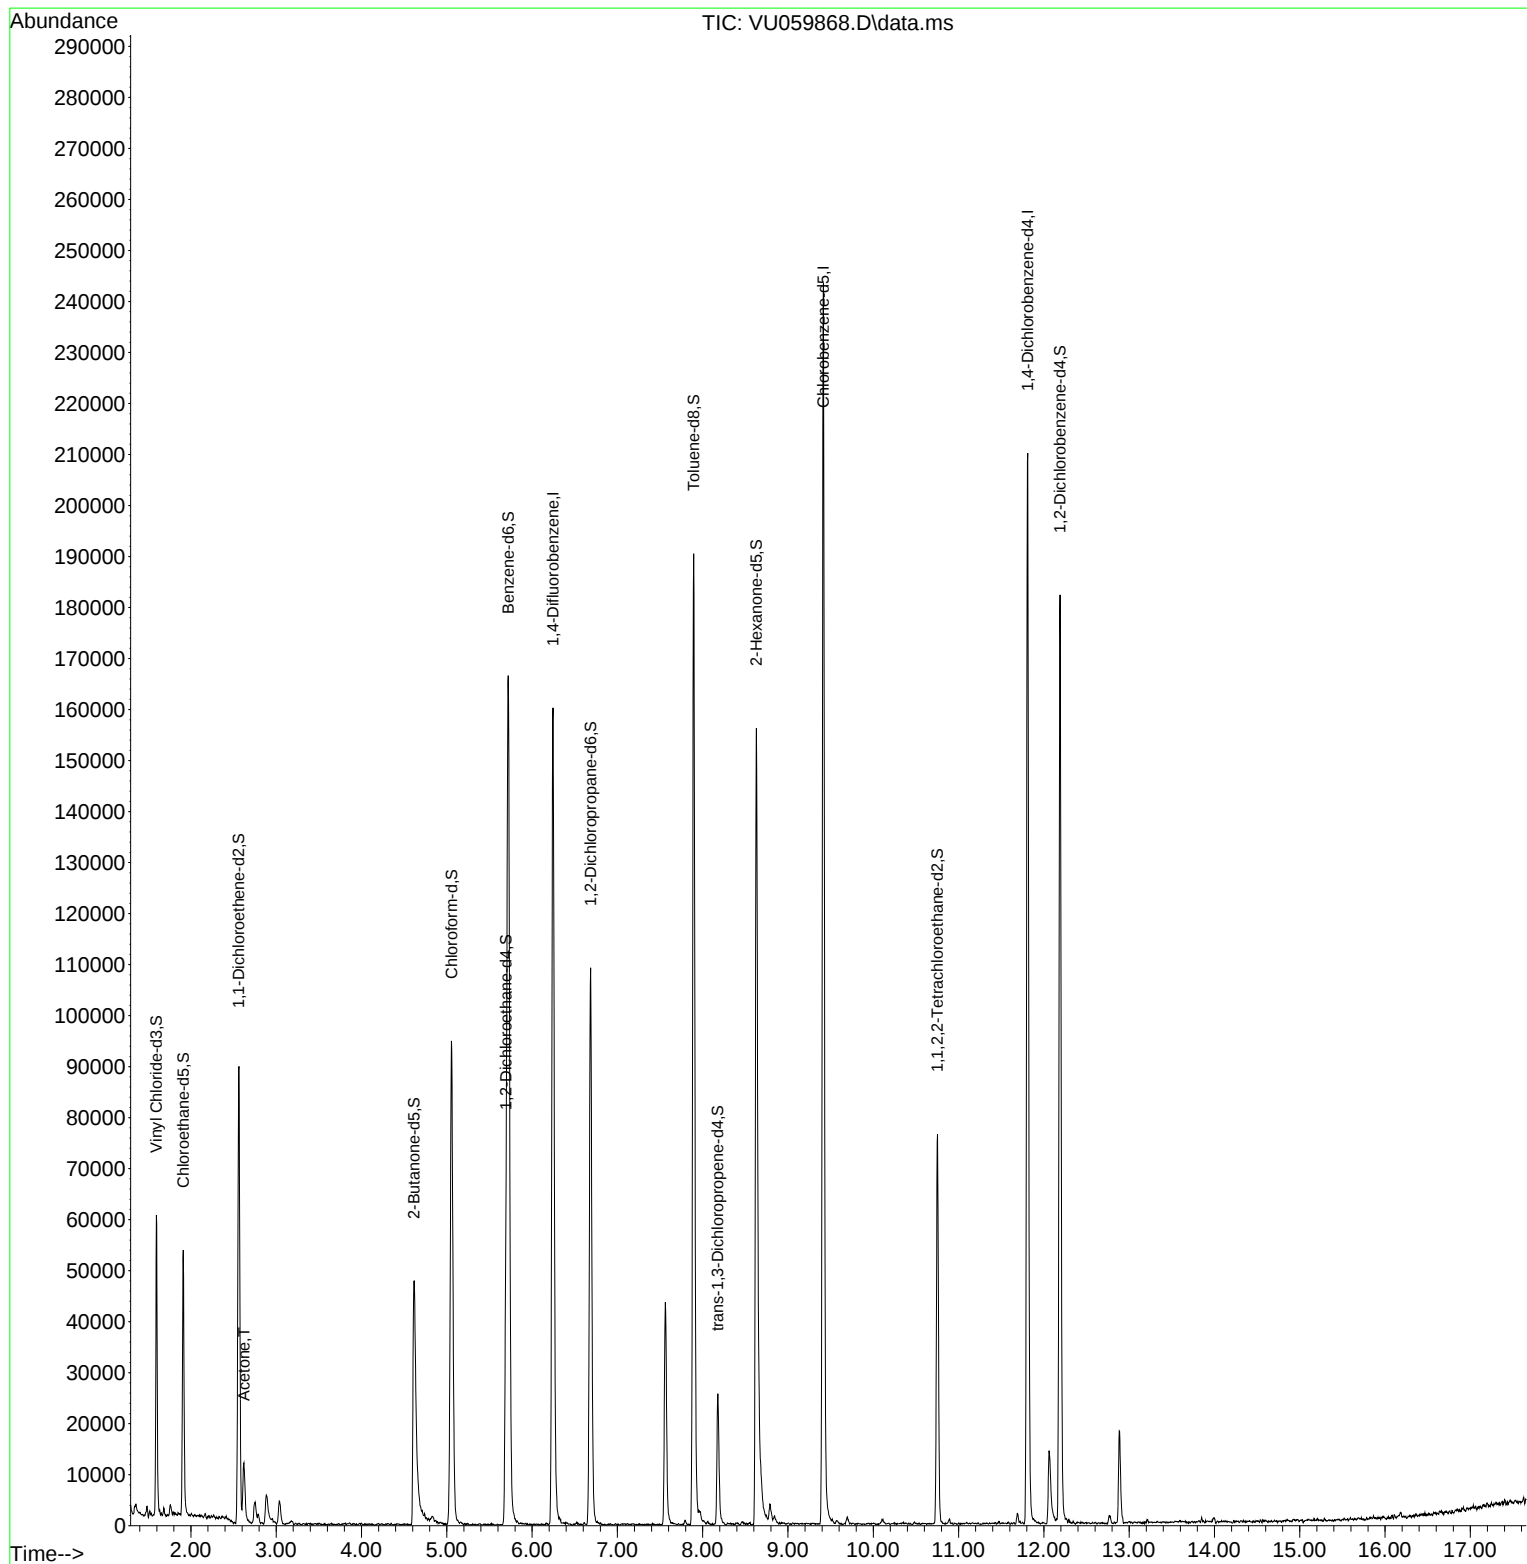

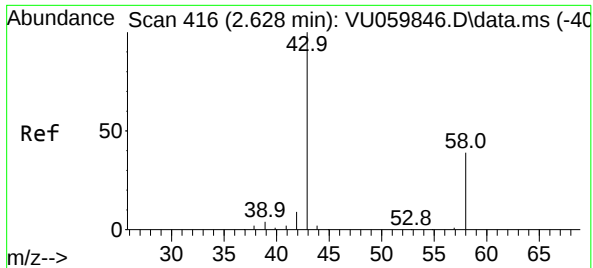

#13
 Acetone
 Concen: 10.915 ug/L
 RT: 2.621 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU059868.D
 Acq: 05 Jul 2024 19:13

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN2

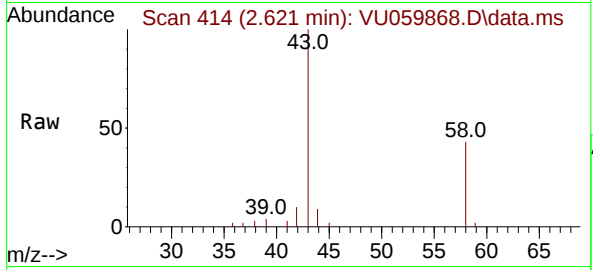

Tgt Ion: 43 Resp: 13895
 Ion Ratio Lower Upper
 43 100
 58 39.7 0.0 68.0

