


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU070720\
 Data File : VU039309.D
 Acq On : 07 Jul 2020 11:00
 Operator : SY/MD
 Sample : BFB26
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jul 07 12:54:12 2020

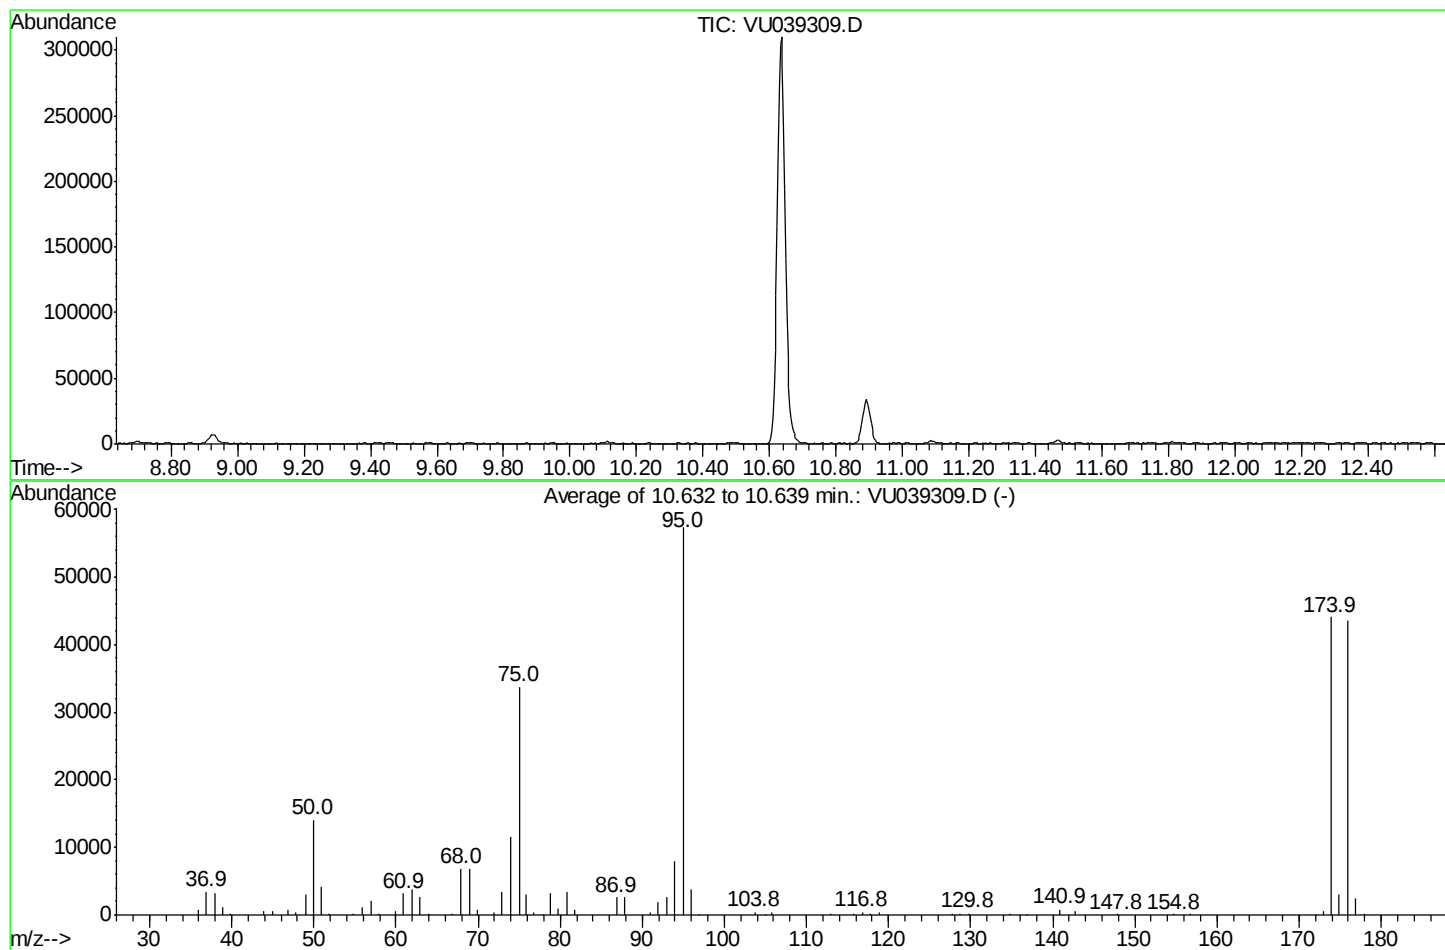

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	14035	PASS
75	95	30	80	58.9	33773	PASS
95	95	100	100	100.0	57322	PASS
96	95	5	9	6.7	3849	PASS
173	174	0.00	2	1.3	569	PASS
174	95	50	120	76.9	44064	PASS
175	174	5	9	6.9	3056	PASS
176	174	95	101	98.8	43538	PASS
177	176	5	9	5.9	2560	PASS

m/z	Abundance
35.90	767.0
36.90	3607.0
37.90	3317.0
38.90	1170.0
39.80	145.0
43.90	1032.0
44.90	686.0
46.90	770.0
47.80	407.0
48.90	3302.0
50.00	14247.0
51.00	4152.0
51.90	217.0
54.80	203.0
56.00	1307.0
57.00	2274.0
57.90	146.0
59.90	661.0
60.90	3398.0
62.00	3847.0
62.90	2574.0
63.90	251.0
66.90	197.0
67.90	7016.0
69.00	6994.0
69.90	707.0
72.00	402.0
72.90	3404.0
74.00	12023.0
75.00	34744.0
75.90	3011.0
76.80	455.0
77.90	177.0
78.90	3248.0
79.80	976.0
80.90	3588.0
81.80	773.0
86.90	2585.0
87.90	2691.0
90.90	275.0
91.90	1942.0
92.90	2547.0
94.00	7963.0
95.00	57680.0
96.00	4042.0
96.90	111.0
103.80	419.0
105.70	423.0
113.00	112.0
115.80	246.0
116.90	490.0
117.80	276.0
118.90	378.0
127.80	224.0
128.70	130.0
129.70	129.0
134.80	144.0
136.80	105.0
140.90	767.0
142.80	700.0
147.80	152.0
154.70	129.0
156.80	113.0
172.10	120.0
173.00	599.0
173.90	43784.0
174.90	3290.0
175.90	42632.0
176.90	2563.0
178.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	712.0
36.90	3532.0
37.90	3373.0
38.90	1260.0
39.90	150.0
43.90	968.0
44.90	667.0
46.90	733.0
47.80	415.0
48.90	3168.0
50.00	14516.0
51.00	4221.0
51.90	225.0
54.90	250.0
55.90	1259.0
57.00	2239.0
57.90	135.0
59.90	681.0
60.90	3214.0
61.90	3833.0
63.00	2742.0
64.00	229.0
66.80	197.0
68.00	6996.0
68.90	6968.0
69.90	781.0
72.00	403.0
73.00	3472.0
74.00	12050.0
75.00	34824.0
75.90	3025.0
76.80	453.0
77.90	204.0
78.80	3259.0
79.80	973.0
80.90	3555.0
81.80	746.0
86.90	2683.0
87.90	2669.0
90.90	331.0
91.90	1955.0
93.00	2659.0
94.00	8216.0
95.00	59008.0
96.00	3994.0
103.80	419.0
104.90	111.0
105.70	325.0
112.90	114.0
115.80	277.0
116.90	463.0
117.80	283.0
118.90	382.0
127.80	200.0
128.80	150.0
129.80	210.0
134.80	137.0
136.80	106.0
140.90	772.0
142.80	654.0
147.80	125.0
154.70	147.0
156.80	137.0
172.10	142.0
173.00	581.0
173.90	45392.0
174.90	3126.0
175.90	44904.0
176.90	2658.0
178.00	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	575.0
36.90	3089.0
37.90	3194.0
38.90	1228.0
39.90	122.0
43.90	876.0
44.90	650.0
46.90	669.0
47.90	415.0
49.00	2792.0
49.90	13342.0
50.90	3856.0
51.90	223.0
54.90	279.0
55.90	1112.0
57.00	1949.0
57.90	106.0
59.90	657.0
60.90	2838.0
61.90	3467.0
63.00	2715.0
64.00	218.0
66.70	165.0
68.00	6481.0
68.90	6388.0
69.90	728.0
71.90	359.0
73.00	3281.0
74.00	10825.0
75.00	31752.0
75.90	2787.0
76.80	448.0
77.90	196.0
78.80	3022.0
79.80	871.0
80.90	3115.0
81.80	697.0
86.90	2519.0
87.90	2424.0
90.90	332.0
91.90	1852.0
93.00	2642.0
94.00	7864.0
95.00	55280.0
96.00	3513.0
103.70	420.0
105.00	109.0
105.70	251.0
112.90	113.0
115.80	314.0
116.80	440.0
117.90	262.0
118.80	313.0
127.80	159.0
128.80	150.0
129.80	256.0
134.80	108.0
140.90	736.0
142.80	593.0
147.80	102.0
154.80	178.0
156.80	127.0
173.00	529.0
173.90	43016.0
174.90	2753.0
175.90	43080.0
176.90	2461.0
177.90	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Scan 2877 (10.591 min): VU039309.D
BFB26

m/z	Abundance
43.90	360.0
78.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26