

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049687.D
 Acq On : 12 Jul 2022 10:49
 Operator : SY/MD
 Sample : VU0712MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	67	rVB2	3477	4696	0.49%	0.067%
2	1.597	72	80	99	rVB	127012	146257	15.37%	2.074%
3	1.906	167	176	196	rVB	92830	125253	13.16%	1.776%
4	2.256	279	285	288	rBV4	654	751	0.08%	0.011%
5	2.314	301	303	310	rVB2	691	526	0.06%	0.007%
6	2.369	315	320	321	rBV2	749	636	0.07%	0.009%
7	2.565	368	381	398	rVV	191055	308747	32.44%	4.377%
8	2.735	431	434	437	rVB	306	178	0.02%	0.003%
9	2.790	444	451	453	rBV3	658	709	0.07%	0.010%
10	2.896	482	484	490	rVB2	224	173	0.02%	0.002%
11	2.925	490	493	497	rBV2	160	169	0.02%	0.002%
12	2.948	498	500	504	rVB2	363	189	0.02%	0.003%
13	3.041	520	529	543	rVB3	4112	7145	0.75%	0.101%
14	3.189	566	575	579	rBV3	754	1221	0.13%	0.017%
15	3.591	698	700	704	rVV2	217	162	0.02%	0.002%
16	3.658	718	721	725	rBV2	252	233	0.02%	0.003%
17	3.838	771	777	779	rBV	228	258	0.03%	0.004%
18	3.877	787	789	795	rVB	235	202	0.02%	0.003%
19	4.427	956	960	966	rBV2	145	171	0.02%	0.002%
20	4.510	983	986	993	rVB2	224	228	0.02%	0.003%
21	4.623	1008	1021	1056	rBV	110019	276012	29.00%	3.913%
22	4.970	1124	1129	1131	rVB	191	168	0.02%	0.002%
23	5.063	1141	1158	1178	rBV	173783	379030	39.83%	5.374%
24	5.169	1188	1191	1196	rVB2	390	326	0.03%	0.005%
25	5.198	1196	1200	1202	rBV	256	215	0.02%	0.003%
26	5.214	1202	1205	1207	rVV2	277	149	0.02%	0.002%
27	5.272	1219	1223	1224	rBV2	439	229	0.02%	0.003%
28	5.369	1250	1253	1260	rBV2	394	423	0.04%	0.006%
29	5.620	1324	1331	1334	rBV2	275	294	0.03%	0.004%
30	5.722	1342	1363	1385	rBV2	350656	951718	100.00%	13.493%
31	5.899	1414	1418	1420	rBV	337	241	0.03%	0.003%
32	5.976	1440	1442	1449	rVB3	259	188	0.02%	0.003%
33	6.247	1512	1526	1553	rBV	278984	530595	55.75%	7.523%
34	6.340	1553	1555	1562	rVB3	408	377	0.04%	0.005%
35	6.449	1585	1589	1593	rVB3	351	343	0.04%	0.005%
36	6.472	1593	1596	1601	rBV2	176	167	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049687.D
 Acq On : 12 Jul 2022 10:49
 Operator : SY/MD
 Sample : VU0712MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.533	1605	1615	1623	rBV6	1609	2788	0.29%	0.040%
38	6.629	1640	1645	1650	rBV2	153	189	0.02%	0.003%
39	6.690	1650	1664	1685	rBV	227250	444796	46.74%	6.306%
40	6.803	1696	1699	1705	rBV2	492	471	0.05%	0.007%
41	7.076	1781	1784	1789	rBV2	175	155	0.02%	0.002%
42	7.140	1801	1804	1806	rVB	283	182	0.02%	0.003%
43	7.157	1806	1809	1812	rBV2	293	259	0.03%	0.004%
44	7.192	1812	1820	1824	rVB3	750	1122	0.12%	0.016%
45	7.256	1836	1840	1845	rBV	151	164	0.02%	0.002%
46	7.282	1846	1848	1853	rVB2	176	160	0.02%	0.002%
47	7.510	1916	1919	1920	rBV	247	157	0.02%	0.002%
48	7.565	1923	1936	1952	rVV	116656	204563	21.49%	2.900%
49	7.690	1972	1975	1976	rBV	387	202	0.02%	0.003%
50	7.796	2002	2008	2016	rVB4	1123	1302	0.14%	0.018%
51	7.896	2026	2039	2061	rBV	408466	705891	74.17%	10.008%
52	8.179	2116	2127	2146	rBV	78043	132549	13.93%	1.879%
53	8.443	2206	2209	2212	rBV2	327	273	0.03%	0.004%
54	8.632	2254	2268	2311	rBV2	304890	576642	60.59%	8.175%
55	8.787	2314	2316	2321	rVV2	554	532	0.06%	0.008%
56	8.870	2339	2342	2345	rBV	226	148	0.02%	0.002%
57	8.941	2362	2364	2370	rVB	227	169	0.02%	0.002%
58	9.111	2413	2417	2419	rBV2	210	176	0.02%	0.002%
59	9.417	2498	2512	2531	rBV	385856	627931	65.98%	8.902%
60	9.565	2556	2558	2559	rBV	374	147	0.02%	0.002%
61	9.661	2584	2588	2593	rBV	276	239	0.03%	0.003%
62	9.693	2593	2598	2608	rBV3	448	551	0.06%	0.008%
63	9.980	2683	2687	2690	rBV2	319	329	0.03%	0.005%
64	10.092	2718	2722	2723	rBV	343	225	0.02%	0.003%
65	10.478	2837	2842	2845	rBV3	378	442	0.05%	0.006%
66	10.523	2851	2856	2859	rBV2	313	317	0.03%	0.004%
67	10.616	2882	2885	2888	rBV2	292	228	0.02%	0.003%
68	10.642	2888	2893	2896	rVV3	593	504	0.05%	0.007%
69	10.754	2916	2928	2948	rVV	299706	478457	50.27%	6.783%
70	10.986	2994	3000	3005	rBV2	277	375	0.04%	0.005%
71	11.092	3028	3033	3039	rBV	282	453	0.05%	0.006%
72	11.121	3039	3042	3047	rVB2	340	271	0.03%	0.004%
73	11.237	3075	3078	3084	rVB2	447	428	0.04%	0.006%
74	11.269	3084	3088	3089	rBV	247	157	0.02%	0.002%
75	11.468	3146	3150	3158	rVB3	659	907	0.10%	0.013%
76	11.536	3168	3171	3175	rBV	452	434	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049687.D
 Acq On : 12 Jul 2022 10:49
 Operator : SY/MD
 Sample : VU0712MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.745	3232	3236	3242	rBV4	863	1117	0.12%	0.016%
78	11.812	3245	3257	3274	rBV	328204	528803	55.56%	7.497%
79	12.137	3355	3358	3363	rBV	256	159	0.02%	0.002%
80	12.192	3363	3375	3393	rBV	340153	558441	58.68%	7.917%
81	12.677	3524	3526	3531	rBV2	218	190	0.02%	0.003%
82	12.838	3572	3576	3579	rBV2	279	228	0.02%	0.003%
83	12.947	3606	3610	3616	rVB3	317	364	0.04%	0.005%
84	12.976	3616	3619	3622	rBV2	291	261	0.03%	0.004%
85	13.156	3673	3675	3678	rBV	297	237	0.02%	0.003%
86	13.217	3690	3694	3702	rVB5	1246	1600	0.17%	0.023%
87	13.674	3834	3836	3839	rVB	374	190	0.02%	0.003%
88	13.700	3839	3844	3851	rBV2	517	652	0.07%	0.009%
89	13.754	3858	3861	3864	rBV	230	197	0.02%	0.003%
90	13.844	3881	3889	3898	rVB4	4781	6607	0.69%	0.094%
91	13.992	3931	3935	3938	rBV	391	311	0.03%	0.004%
92	14.044	3946	3951	3954	rBV2	382	344	0.04%	0.005%
93	14.089	3956	3965	3976	rBV	11528	18797	1.98%	0.266%
94	14.188	3993	3996	3999	rVB2	370	238	0.03%	0.003%
95	14.330	4033	4040	4051	rVB5	6130	9436	0.99%	0.134%
96	14.539	4103	4105	4112	rVB3	371	288	0.03%	0.004%
97	14.658	4138	4142	4145	rBV	428	426	0.04%	0.006%
98	14.748	4163	4170	4172	rBV	403	522	0.05%	0.007%
99	14.790	4180	4183	4184	rBV3	269	184	0.02%	0.003%
100	15.134	4288	4290	4294	rBV3	324	183	0.02%	0.003%




Sum of corrected areas: 7053439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049687.D
Acq On : 12 Jul 2022 10:49
Operator : SY/MD
Sample : VU0712MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

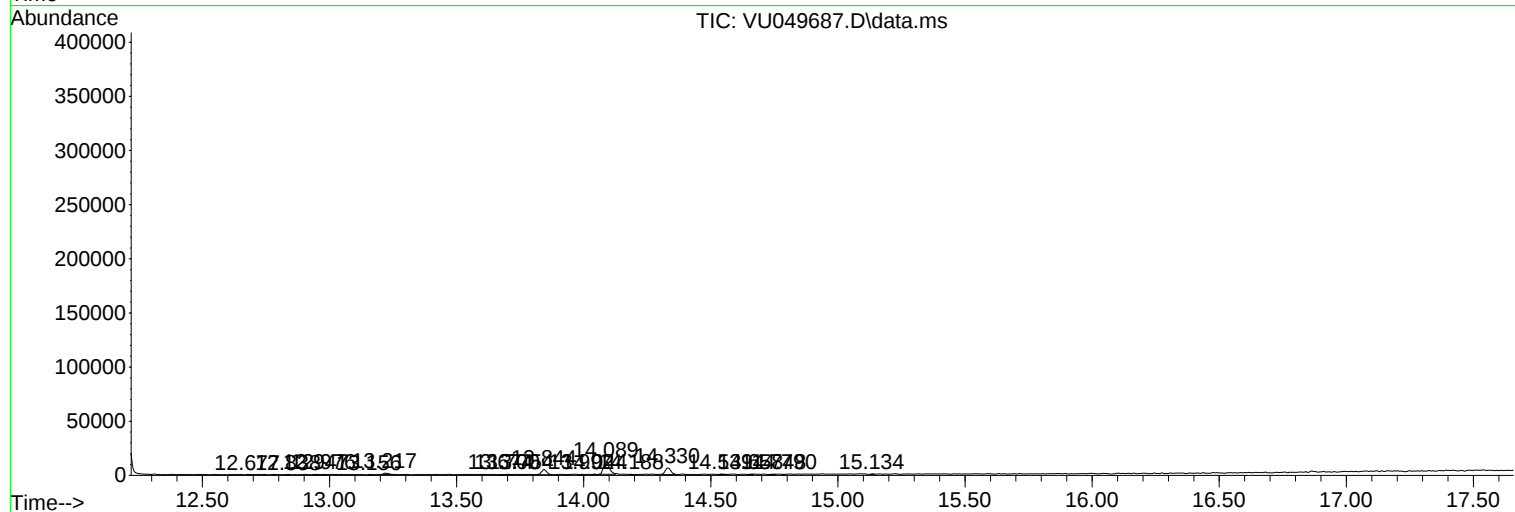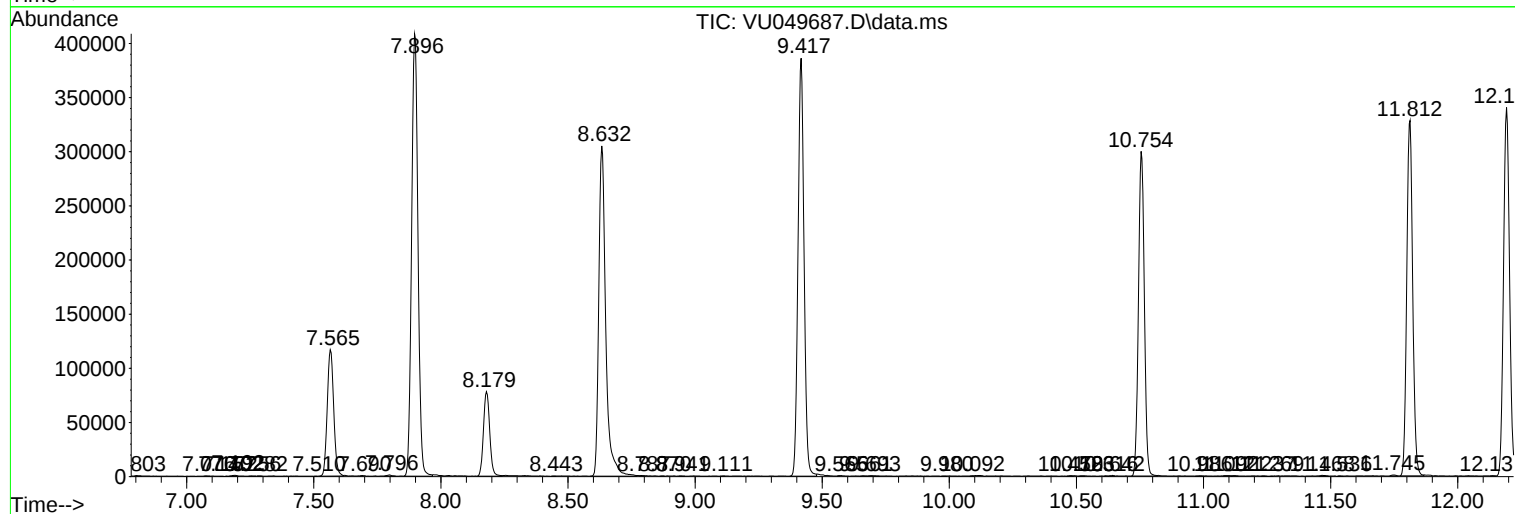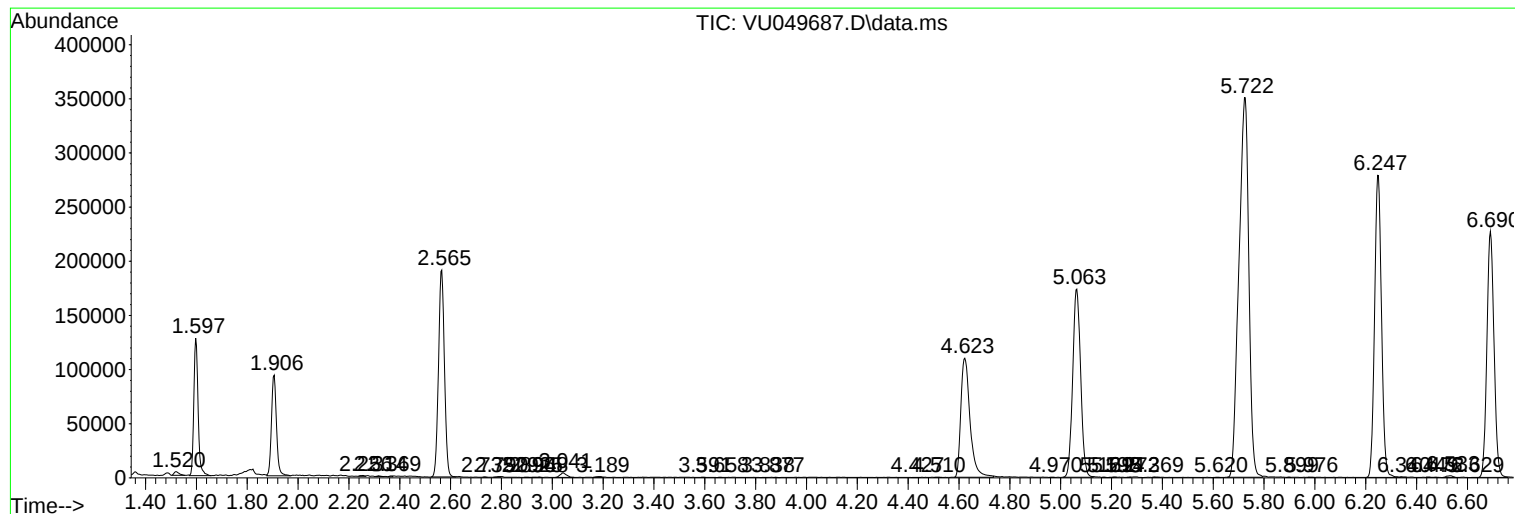

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049687.D
Acq On : 12 Jul 2022 10:49
Operator : SY/MD
Sample : VU0712MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049687.D
Acq On : 12 Jul 2022 10:49
Operator : SY/MD
Sample : VU0712MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc