

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049688.D
 Acq On : 12 Jul 2022 11:13
 Operator : SY/MD
 Sample : VU0712WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.360	3	6	11	rVB2	2318	1822	0.20%	0.027%
2	1.598	72	80	99	rVB	120613	135994	14.79%	1.994%
3	1.903	166	175	193	rVB	88026	116919	12.72%	1.715%
4	2.315	300	303	304	rBV2	567	300	0.03%	0.004%
5	2.324	304	306	311	rVB3	793	675	0.07%	0.010%
6	2.562	368	380	398	rBV	178512	289484	31.49%	4.246%
7	2.659	407	410	417	rVB	362	342	0.04%	0.005%
8	2.790	444	451	457	rBV2	469	699	0.08%	0.010%
9	2.922	488	492	496	rBV2	291	253	0.03%	0.004%
10	3.041	520	529	540	rVB4	3884	6530	0.71%	0.096%
11	3.183	563	573	579	rBV3	1570	2845	0.31%	0.042%
12	3.289	600	606	610	rBV	373	359	0.04%	0.005%
13	3.356	622	627	630	rBV2	224	236	0.03%	0.003%
14	3.524	676	679	684	rBV2	190	156	0.02%	0.002%
15	3.636	708	714	717	rBV2	216	248	0.03%	0.004%
16	3.691	726	731	733	rBV2	162	158	0.02%	0.002%
17	3.948	800	811	812	rBV2	180	267	0.03%	0.004%
18	3.974	817	819	826	rVB	198	175	0.02%	0.003%
19	4.138	865	870	876	rVB2	228	254	0.03%	0.004%
20	4.437	957	963	967	rBV2	175	195	0.02%	0.003%
21	4.620	1007	1020	1061	rVV	111991	274991	29.92%	4.033%
22	4.851	1088	1092	1094	rVB2	310	201	0.02%	0.003%
23	5.064	1140	1158	1178	rBV	166014	360738	39.24%	5.291%
24	5.231	1207	1210	1212	rBV	269	190	0.02%	0.003%
25	5.289	1222	1228	1233	rBV2	514	625	0.07%	0.009%
26	5.372	1249	1254	1257	rBV3	462	430	0.05%	0.006%
27	5.446	1272	1277	1281	rBV2	228	242	0.03%	0.004%
28	5.469	1281	1284	1289	rBV2	298	254	0.03%	0.004%
29	5.610	1325	1328	1331	rBV2	215	166	0.02%	0.002%
30	5.723	1341	1363	1386	rBV2	341493	919236	100.00%	13.481%
31	5.932	1422	1428	1430	rBV2	293	305	0.03%	0.004%
32	6.003	1444	1450	1453	rBV2	289	261	0.03%	0.004%
33	6.048	1459	1464	1466	rBV2	270	255	0.03%	0.004%
34	6.247	1512	1526	1542	rBV	269805	505169	54.96%	7.409%
35	6.523	1606	1612	1624	rVB3	1356	2172	0.24%	0.032%
36	6.601	1634	1636	1639	rVB	261	156	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049688.D
 Acq On : 12 Jul 2022 11:13
 Operator : SY/MD
 Sample : VU0712WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.691	1649	1664	1681	rBV	218497	421475	45.85%	6.181%
38	6.793	1694	1696	1697	rBV2	430	163	0.02%	0.002%
39	6.806	1697	1700	1705	rVV3	685	448	0.05%	0.007%
40	6.977	1750	1753	1756	rBV2	250	189	0.02%	0.003%
41	7.183	1814	1817	1823	rBV3	656	634	0.07%	0.009%
42	7.276	1843	1846	1848	rBV	224	160	0.02%	0.002%
43	7.382	1876	1879	1884	rVB2	221	195	0.02%	0.003%
44	7.453	1899	1901	1906	rVB	281	175	0.02%	0.003%
45	7.482	1906	1910	1914	rBV2	281	308	0.03%	0.005%
46	7.565	1922	1936	1951	rBV	114782	197103	21.44%	2.891%
47	7.793	2001	2007	2012	rBV2	423	561	0.06%	0.008%
48	7.896	2025	2039	2057	rBV	392233	671440	73.04%	9.847%
49	8.060	2087	2090	2094	rVB3	329	183	0.02%	0.003%
50	8.089	2097	2099	2105	rVB3	556	363	0.04%	0.005%
51	8.179	2113	2127	2144	rBV	76181	126278	13.74%	1.852%
52	8.330	2168	2174	2177	rVB2	274	290	0.03%	0.004%
53	8.353	2178	2181	2184	rBV2	262	196	0.02%	0.003%
54	8.633	2255	2268	2306	rBV2	298469	571809	62.20%	8.386%
55	8.826	2324	2328	2331	rVB3	259	168	0.02%	0.002%
56	8.864	2337	2340	2344	rBV3	246	217	0.02%	0.003%
57	8.938	2361	2363	2368	rVB2	359	271	0.03%	0.004%
58	8.964	2368	2371	2374	rBV2	209	208	0.02%	0.003%
59	9.121	2417	2420	2423	rBV2	262	212	0.02%	0.003%
60	9.160	2429	2432	2434	rBV2	215	159	0.02%	0.002%
61	9.366	2492	2496	2499	rBV	214	183	0.02%	0.003%
62	9.417	2499	2512	2538	rBV	372074	610438	66.41%	8.953%
63	9.697	2594	2599	2602	rBV2	368	390	0.04%	0.006%
64	9.825	2636	2639	2643	rVB2	226	160	0.02%	0.002%
65	9.928	2668	2671	2677	rBV2	212	188	0.02%	0.003%
66	10.099	2720	2724	2729	rBV3	343	399	0.04%	0.006%
67	10.147	2735	2739	2742	rBV2	283	212	0.02%	0.003%
68	10.253	2768	2772	2774	rBV	219	160	0.02%	0.002%
69	10.362	2803	2806	2811	rBV2	341	427	0.05%	0.006%
70	10.485	2841	2844	2846	rVV2	464	284	0.03%	0.004%
71	10.613	2881	2884	2888	rBV2	259	184	0.02%	0.003%
72	10.649	2892	2895	2900	rBV2	314	374	0.04%	0.005%
73	10.694	2906	2909	2912	rBV2	202	158	0.02%	0.002%
74	10.755	2916	2928	2948	rBV	297596	472041	51.35%	6.923%
75	11.044	3015	3018	3021	rBV	296	206	0.02%	0.003%
76	11.083	3026	3030	3036	rBV3	293	333	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
 Data File : VU049688.D
 Acq On : 12 Jul 2022 11:13
 Operator : SY/MD
 Sample : VU0712WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.288	3091	3094	3098	rBV2	237	247	0.03%	0.004%
78	11.314	3099	3102	3112	rVB2	302	364	0.04%	0.005%
79	11.472	3147	3151	3156	rVB2	437	443	0.05%	0.006%
80	11.748	3233	3237	3242	rBV2	593	537	0.06%	0.008%
81	11.813	3244	3257	3280	rVV	333385	534720	58.17%	7.842%
82	12.112	3347	3350	3354	rVB	250	198	0.02%	0.003%
83	12.192	3363	3375	3395	rBV	346778	562016	61.14%	8.242%
84	12.321	3411	3415	3422	rVB3	510	618	0.07%	0.009%
85	12.369	3424	3430	3432	rBV2	361	431	0.05%	0.006%
86	12.999	3623	3626	3628	rBV2	246	168	0.02%	0.002%
87	13.214	3690	3693	3695	rBV2	476	332	0.04%	0.005%
88	13.414	3752	3755	3759	rBV2	424	327	0.04%	0.005%
89	13.719	3848	3850	3853	rVB	329	164	0.02%	0.002%
90	13.845	3883	3889	3896	rBV5	1677	2460	0.27%	0.036%
91	13.890	3900	3903	3908	rBV3	416	394	0.04%	0.006%
92	13.960	3922	3925	3929	rBV	245	173	0.02%	0.003%
93	14.092	3956	3966	3973	rBV3	4030	6791	0.74%	0.100%
94	14.330	4035	4040	4050	rVB4	2141	3029	0.33%	0.044%
95	14.391	4057	4059	4064	rBV2	367	291	0.03%	0.004%
96	14.478	4083	4086	4095	rVB3	452	519	0.06%	0.008%
97	14.558	4108	4111	4114	rBV	471	340	0.04%	0.005%
98	14.648	4136	4139	4141	rBV2	305	217	0.02%	0.003%
99	15.388	4367	4369	4370	rBV	378	155	0.02%	0.002%
100	16.201	4617	4622	4626	rBV5	1001	946	0.10%	0.014%




Sum of corrected areas: 6818524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049688.D
Acq On : 12 Jul 2022 11:13
Operator : SY/MD
Sample : VU0712WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

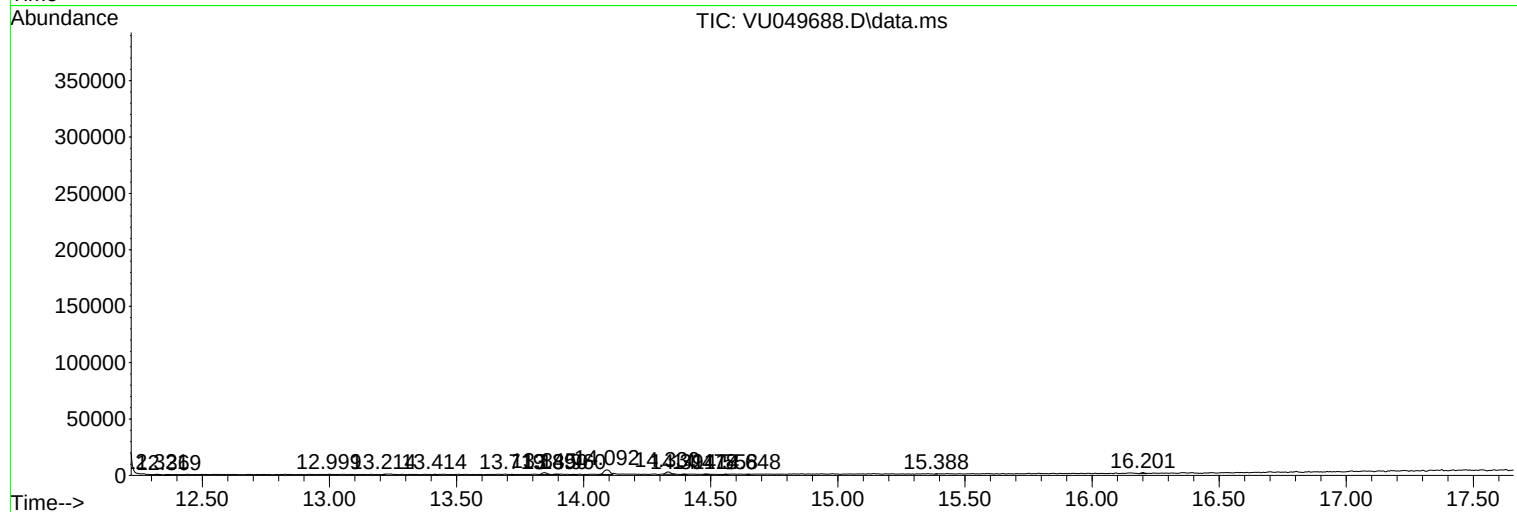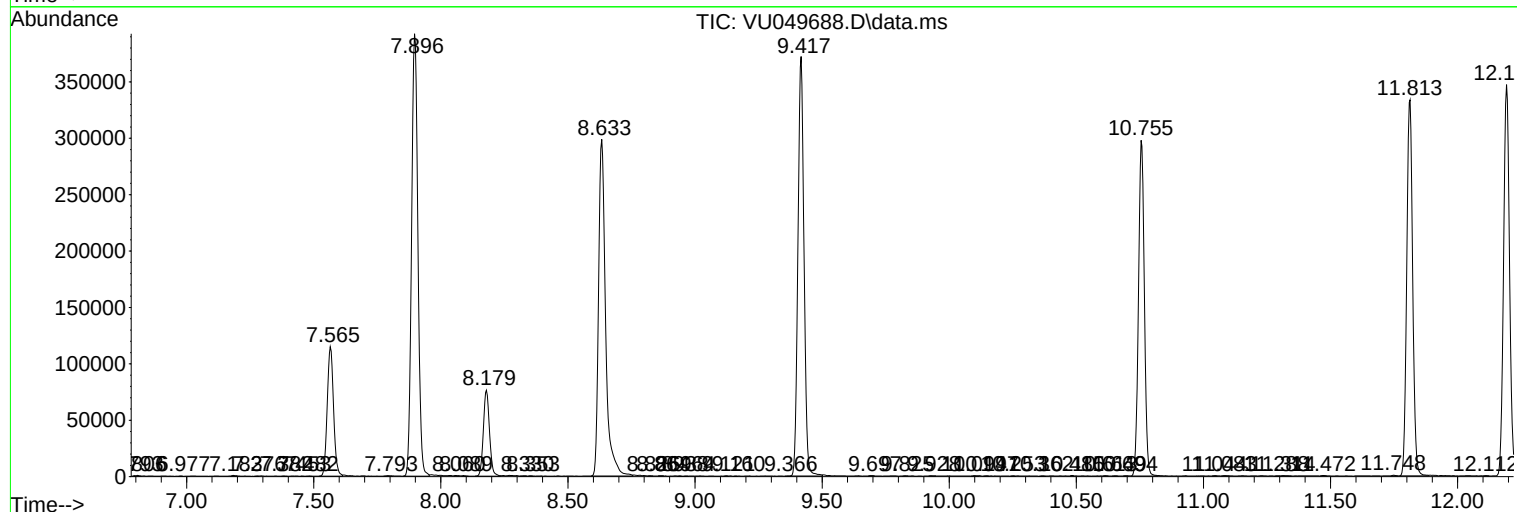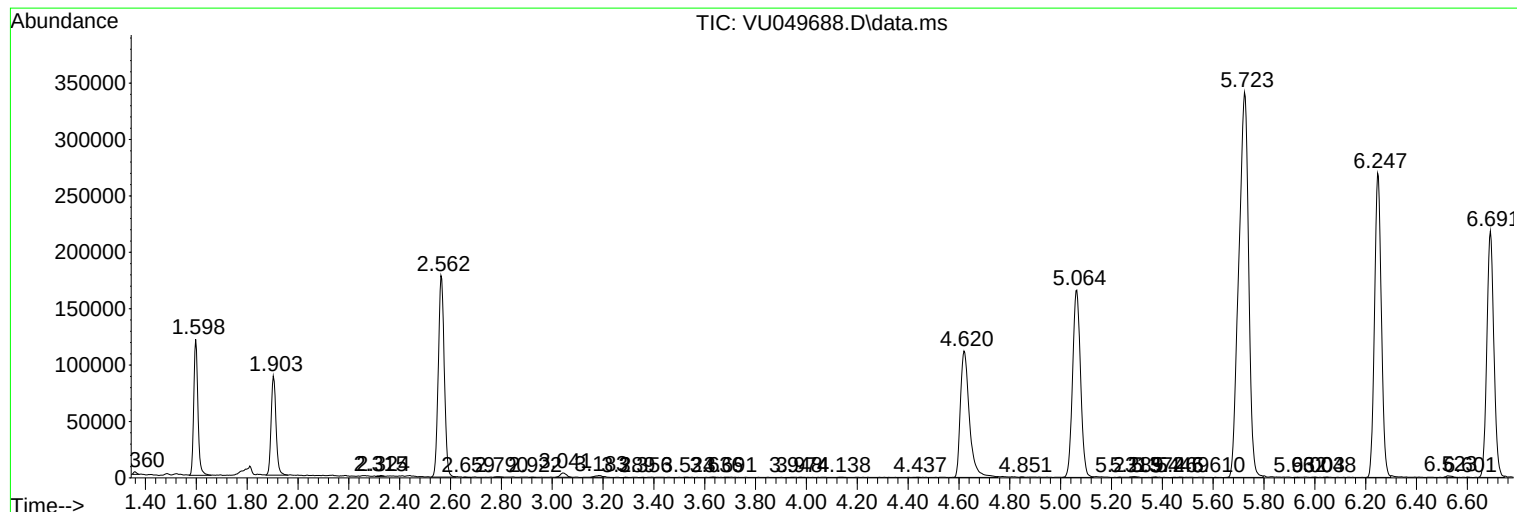

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049688.D
Acq On : 12 Jul 2022 11:13
Operator : SY/MD
Sample : VU0712WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049688.D
Acq On : 12 Jul 2022 11:13
Operator : SY/MD
Sample : VU0712WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------