


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071222\
Data File : VU049685.D
Acq On : 12 Jul 2022 08:55
Operator : SY/MD
Sample : BFB102
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB102

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Wed Jul 13 06:51:38 2022

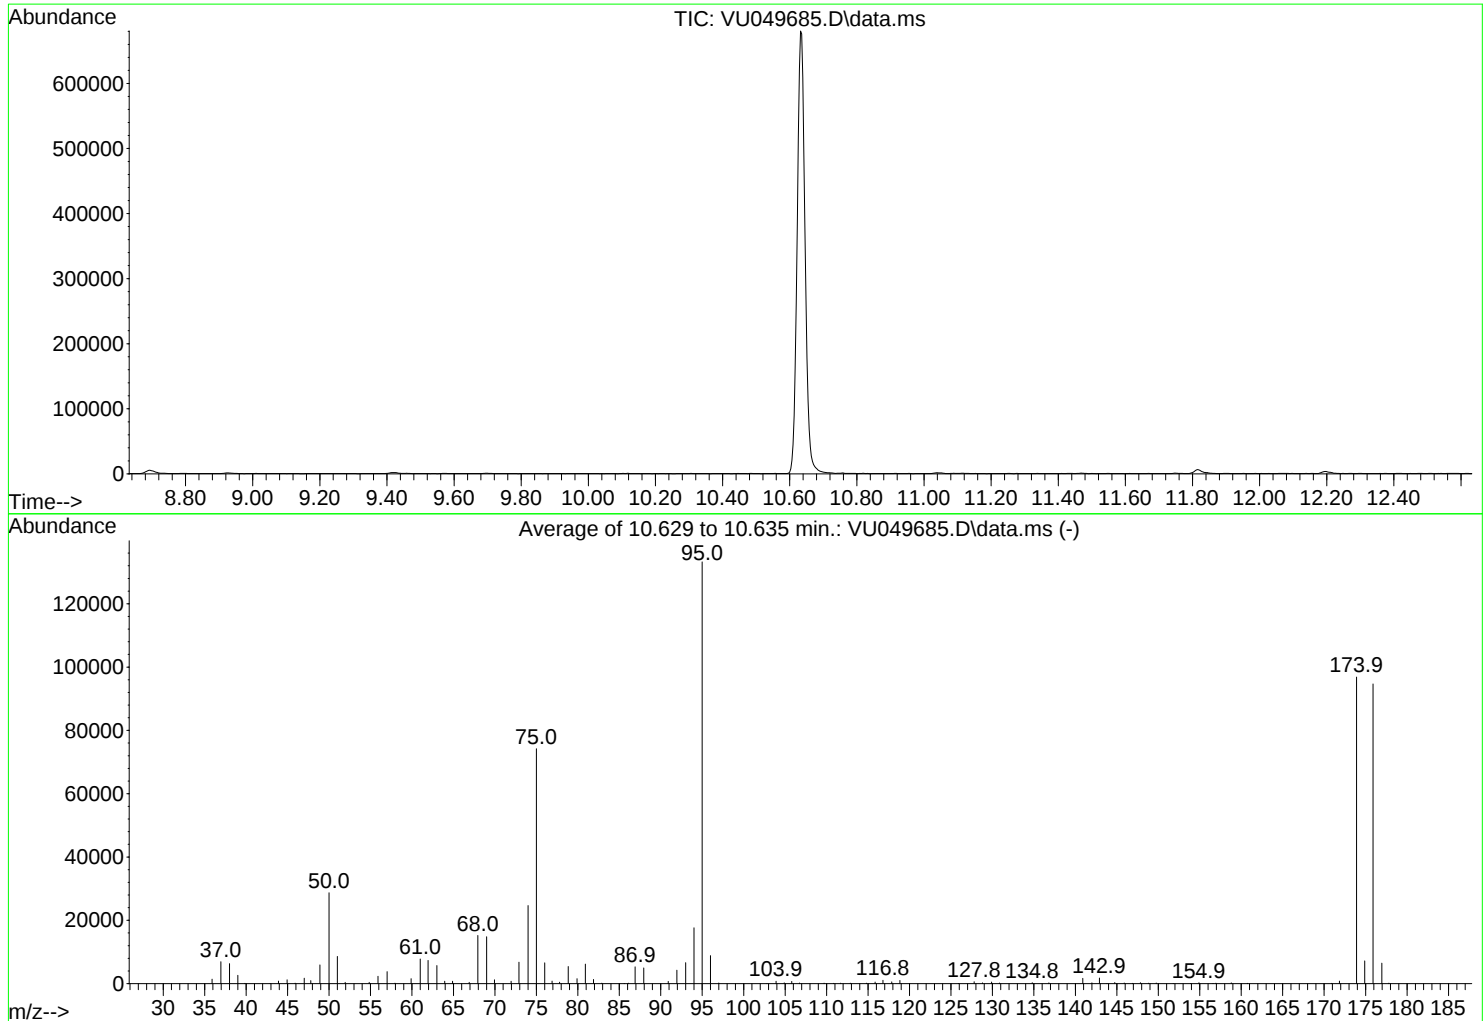

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	28723	PASS
75	95	30	80	55.7	74179	PASS
95	95	100	100	100.0	133245	PASS
96	95	5	9	6.6	8830	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.7	96829	PASS
175	174	5	9	7.4	7169	PASS
176	174	95	101	97.8	94669	PASS
177	176	5	9	6.8	6484	PASS

Scan 2876 (10.587 min): VU049685.D\data.ms
BFB102

m/z	Abundance
39.80	140.0
43.90	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1416.0
36.90	6675.0
38.00	5979.0
39.00	2502.0
40.00	279.0
43.90	1178.0
45.00	1192.0
45.90	183.0
47.00	1751.0
47.80	924.0
48.90	5911.0
50.00	27856.0
51.00	7886.0
52.00	406.0
54.90	421.0
55.90	2242.0
57.00	3758.0
57.90	154.0
59.90	1543.0
61.00	7273.0
61.90	6838.0
63.00	5316.0
64.00	809.0
64.90	722.0
66.90	336.0
67.90	14665.0
69.00	14397.0
69.90	1032.0
72.00	743.0
72.90	6350.0
74.00	23488.0
75.00	70312.0
76.00	6352.0
76.90	685.0
77.80	464.0
78.90	5095.0
79.90	1451.0
80.90	5952.0
81.90	1214.0
82.90	181.0
85.60	105.0
86.10	119.0
86.90	5047.0
87.90	4827.0
90.90	792.0
92.00	4119.0
93.00	6093.0
94.00	16960.0
95.00	126200.0
96.00	8501.0
97.10	226.0
103.90	713.0
104.90	222.0
105.80	739.0
106.80	200.0
109.70	141.0
110.80	118.0
111.70	112.0
112.80	169.0
114.80	149.0
115.90	468.0
116.80	1014.0
117.80	441.0
118.80	958.0
125.90	123.0
127.80	569.0
128.80	252.0
129.90	466.0
130.90	233.0
134.80	262.0
136.80	226.0
140.90	1574.0
142.00	243.0
142.90	1548.0
144.80	370.0
145.90	148.0
147.90	248.0
148.80	115.0
149.70	119.0
154.90	298.0
157.00	154.0
158.80	212.0
160.80	122.0
171.90	733.0
173.90	89960.0
174.90	6708.0
175.90	87272.0
176.90	6239.0
177.80	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1511.0
36.90	7088.0
38.00	6636.0
39.00	2726.0
40.00	267.0
43.90	1216.0
44.90	1263.0
45.90	173.0
47.00	1788.0
47.80	984.0
48.90	6063.0
50.00	29640.0
51.00	8986.0
52.00	388.0
54.90	396.0
55.90	2406.0
57.00	3905.0
58.00	142.0
59.90	1604.0
61.00	8096.0
62.00	7600.0
63.00	5842.0
63.90	796.0
64.90	762.0
66.90	393.0
67.90	15748.0
69.00	15393.0
69.90	1235.0
72.00	756.0
72.90	7053.0
74.00	25408.0
75.00	76520.0
76.00	6824.0
76.90	838.0
77.80	488.0
78.90	5597.0
79.90	1622.0
80.90	6377.0
81.90	1362.0
82.90	169.0
86.10	185.0
86.90	5517.0
87.90	5042.0
90.90	718.0
92.00	4430.0
93.00	6850.0
94.00	18136.0
95.00	137728.0
96.00	9135.0
97.00	211.0
103.90	770.0
104.90	256.0
105.80	748.0
106.80	219.0
109.70	127.0
110.80	109.0
111.70	141.0
112.90	176.0
114.80	172.0
115.90	513.0
116.80	1127.0
117.90	536.0
118.90	1050.0
127.80	634.0
128.80	257.0
129.90	518.0
130.90	228.0
134.80	325.0
136.80	262.0
140.90	1708.0
142.00	243.0
142.90	1818.0
144.80	367.0
145.90	205.0
146.90	126.0
147.90	263.0
148.80	149.0
149.80	196.0
153.90	106.0
154.90	335.0
156.90	168.0
158.80	276.0
160.70	122.0
170.90	141.0
171.90	842.0
173.90	99672.0
174.90	7326.0
175.90	97392.0
176.90	6650.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1511.0
36.90	7088.0
38.00	6636.0
39.00	2726.0
40.00	267.0
43.90	1216.0
44.90	1263.0
45.90	173.0
47.00	1788.0
47.80	984.0
48.90	6063.0
50.00	29640.0
51.00	8986.0
52.00	388.0
54.90	396.0
55.90	2406.0
57.00	3905.0
58.00	142.0
59.90	1604.0
61.00	8096.0
62.00	7600.0
63.00	5842.0
63.90	796.0
64.90	762.0
66.90	393.0
67.90	15748.0
69.00	15393.0
69.90	1235.0
72.00	756.0
72.90	7053.0
74.00	25408.0
75.00	76520.0
76.00	6824.0
76.90	838.0
77.80	488.0
78.90	5597.0
79.90	1622.0
80.90	6377.0
81.90	1362.0
82.90	169.0
86.10	185.0
86.90	5517.0
87.90	5042.0
90.90	718.0
92.00	4430.0
93.00	6850.0
94.00	18136.0
95.00	137728.0
96.00	9135.0
97.00	211.0
103.90	770.0
104.90	256.0
105.80	748.0
106.80	219.0
109.70	127.0
110.80	109.0
111.70	141.0
112.90	176.0
114.80	172.0
115.90	513.0
116.80	1127.0
117.90	536.0
118.90	1050.0
127.80	634.0
128.80	257.0
129.90	518.0
130.90	228.0
134.80	325.0
136.80	262.0
140.90	1708.0
142.00	243.0
142.90	1818.0
144.80	367.0
145.90	205.0
146.90	126.0
147.90	263.0
148.80	149.0
149.80	196.0
153.90	106.0
154.90	335.0
156.90	168.0
158.80	276.0
160.70	122.0
170.90	141.0
171.90	842.0
173.90	99672.0
174.90	7326.0
175.90	97392.0
176.90	6650.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1351.0
37.00	6963.0
38.00	6414.0
39.00	2643.0
39.90	234.0
42.90	102.0
43.90	1162.0
44.90	1157.0
45.90	144.0
47.00	1642.0
47.80	944.0
48.90	5855.0
50.00	28672.0
51.00	8974.0
51.90	357.0
54.80	353.0
55.90	2315.0
57.00	3718.0
57.90	146.0
59.90	1517.0
61.00	8062.0
62.00	7585.0
63.00	6013.0
63.90	748.0
64.90	725.0
66.90	426.0
68.00	15195.0
69.00	14592.0
70.00	1348.0
71.90	724.0
72.90	6886.0
74.00	25080.0
75.00	75704.0
76.00	6521.0
76.90	970.0
77.80	458.0
78.80	5606.0
79.90	1574.0
80.90	6202.0
81.90	1323.0
82.90	124.0
86.10	242.0
86.90	5382.0
88.00	4996.0
90.90	603.0
91.90	4158.0
93.00	6997.0
94.00	17864.0
95.00	135808.0
96.00	8853.0
96.90	232.0
102.80	106.0
103.90	834.0
104.90	249.0
105.80	692.0
106.70	171.0
109.70	121.0
110.90	115.0
111.70	151.0
112.90	160.0
114.80	163.0
115.80	506.0
116.80	1066.0
117.90	668.0
118.90	986.0
127.80	619.0
128.80	266.0
129.90	493.0
130.80	224.0
134.80	322.0
136.80	299.0
140.90	1689.0
142.00	227.0
142.90	1959.0
143.80	109.0
144.70	305.0
145.90	264.0
146.90	151.0
147.80	339.0
148.90	154.0
149.80	255.0
151.80	102.0
154.90	355.0
156.60	165.0
156.90	165.0
158.80	282.0
160.70	131.0
170.90	145.0
171.80	890.0
173.90	100856.0
174.90	7473.0
175.90	99344.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

177.006562.0

177.80135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102