


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072020\
 Data File : VU039564.D
 Acq On : 20 Jul 2020 09:02
 Operator : SY/MD
 Sample : BFB05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jul 21 06:02:44 2020

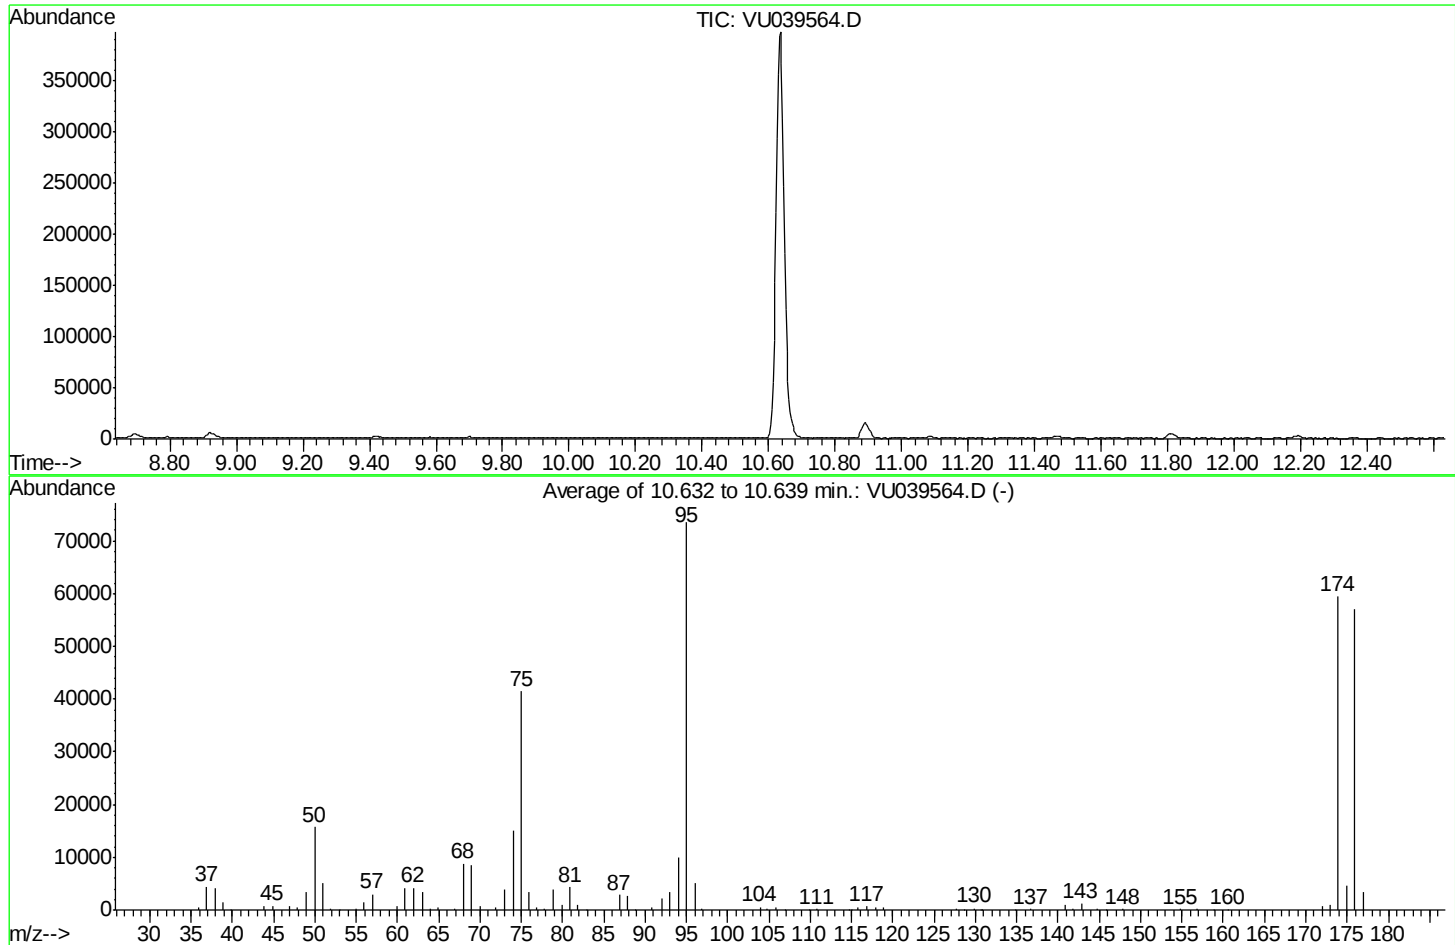

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	15729	PASS
75	95	30	80	56.4	41493	PASS
95	95	100	100	100.0	73528	PASS
96	95	5	9	6.8	4988	PASS
173	174	0.00	2	1.5	918	PASS
174	95	50	120	80.9	59448	PASS
175	174	5	9	7.8	4652	PASS
176	174	95	101	96.1	57122	PASS
177	176	5	9	6.1	3512	PASS

m/z	Abundance
35.90	1190.0
36.90	4609.0
38.00	4410.0
38.90	1618.0
39.80	251.0
43.90	991.0
44.90	836.0
47.00	834.0
47.90	470.0
48.90	3405.0
50.00	16262.0
51.00	5283.0
52.00	243.0
52.90	145.0
55.00	339.0
56.00	1650.0
57.00	2896.0
60.00	639.0
60.90	4267.0
61.90	4437.0
63.00	3490.0
63.90	409.0
64.90	539.0
66.90	260.0
68.00	9117.0
68.90	9051.0
69.90	695.0
72.00	429.0
72.90	4082.0
74.00	15184.0
75.00	43040.0
75.90	3538.0
76.90	518.0
77.90	332.0
78.90	4200.0
79.90	1163.0
80.90	4466.0
81.80	1021.0
86.90	2882.0
87.90	2815.0
88.70	155.0
90.70	390.0
92.00	2400.0
92.90	3611.0
94.00	10548.0
95.00	74432.0
96.00	5237.0
96.80	125.0
103.90	603.0
104.80	187.0
105.80	417.0
106.80	121.0
109.80	160.0
110.90	165.0
115.80	368.0
116.80	647.0
117.80	431.0
118.90	577.0
127.70	317.0
128.80	126.0
129.90	304.0
130.60	154.0
134.90	149.0
136.70	197.0
140.90	1122.0
141.90	197.0
142.80	1113.0
144.80	159.0
145.80	122.0
147.90	180.0
155.00	157.0
156.90	166.0
158.80	112.0
160.60	111.0
171.90	677.0
173.00	906.0
173.90	59224.0
174.90	4916.0
175.90	57536.0
176.90	3546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
35.90	1057.0
36.90	4609.0
37.90	4393.0
38.90	1415.0
39.90	317.0
43.90	1006.0
44.90	803.0
47.00	826.0
47.90	487.0
48.90	3398.0
50.00	16243.0
51.00	5214.0
51.90	256.0
52.90	122.0
55.00	321.0
55.90	1587.0
57.00	3091.0
60.00	624.0
60.90	4232.0
61.90	4292.0
63.00	3514.0
63.90	368.0
64.90	469.0
67.00	264.0
67.90	9064.0
68.90	8659.0
70.00	742.0
72.00	393.0
72.90	4107.0
74.00	15592.0
75.00	42624.0
75.90	3658.0
76.90	458.0
77.80	310.0
78.90	4107.0
79.90	1057.0
80.90	4459.0
81.90	990.0
82.80	104.0
86.90	2956.0
87.90	2756.0
88.70	106.0
90.70	428.0
92.00	2372.0
92.90	3529.0
94.00	10387.0
95.00	75536.0
96.00	5174.0
96.90	136.0
103.90	583.0
104.70	146.0
105.80	481.0
106.90	115.0
109.80	143.0
110.90	152.0
114.70	123.0
115.80	385.0
116.80	701.0
117.80	447.0
118.80	620.0
127.80	282.0
128.60	118.0
129.90	310.0
130.90	178.0
134.90	130.0
136.80	233.0
140.90	1109.0
141.80	195.0
142.80	1163.0
144.70	174.0
145.70	131.0
147.90	173.0
154.80	171.0
156.90	148.0
158.80	111.0
160.60	103.0
171.90	641.0
173.00	978.0
173.90	61264.0
174.90	4783.0
175.90	58768.0
176.90	3554.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
35.90	918.0
36.90	4128.0
38.00	3827.0
38.90	1280.0
39.90	319.0
43.90	907.0
44.90	696.0
47.00	765.0
47.80	470.0
48.90	3220.0
50.00	14682.0
51.00	4683.0
51.90	249.0
55.00	279.0
55.90	1470.0
57.00	2953.0
59.90	596.0
60.90	3985.0
61.90	3787.0
63.00	3271.0
63.90	267.0
64.90	338.0
67.00	254.0
67.90	8321.0
69.00	7620.0
70.00	672.0
71.90	355.0
72.90	3824.0
74.00	14398.0
75.00	38816.0
76.00	3382.0
76.90	410.0
77.70	284.0
78.90	3656.0
79.90	926.0
80.90	4132.0
81.90	884.0
82.90	147.0
86.90	2811.0
87.90	2378.0
90.80	396.0
92.00	2159.0
92.90	3333.0
94.00	9272.0
95.00	70616.0
96.00	4555.0
96.90	146.0
103.90	506.0
104.70	109.0
105.80	458.0
110.80	123.0
114.70	128.0
115.00	129.0
115.80	368.0
116.90	687.0
117.90	411.0
118.80	598.0
127.80	264.0
128.60	117.0
129.90	250.0
130.80	160.0
134.80	114.0
136.80	227.0
140.90	1022.0
141.80	172.0
142.90	1126.0
144.70	145.0
145.70	122.0
147.90	147.0
154.70	196.0
156.90	152.0
172.00	536.0
173.00	870.0
173.90	57856.0
174.90	4258.0
175.90	55064.0
176.90	3436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

Scan 2876 (10.587 min): VU039564.D
BFB05

m/z	Abundance
35.80	461.0
38.00	108.0
39.90	189.0
43.90	319.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05