


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072224\
Data File : VU060080.D
Acq On : 22 Jul 2024 08:41
Operator : MD/SY
Sample : BFB176
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB176

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jul 23 07:21:00 2024

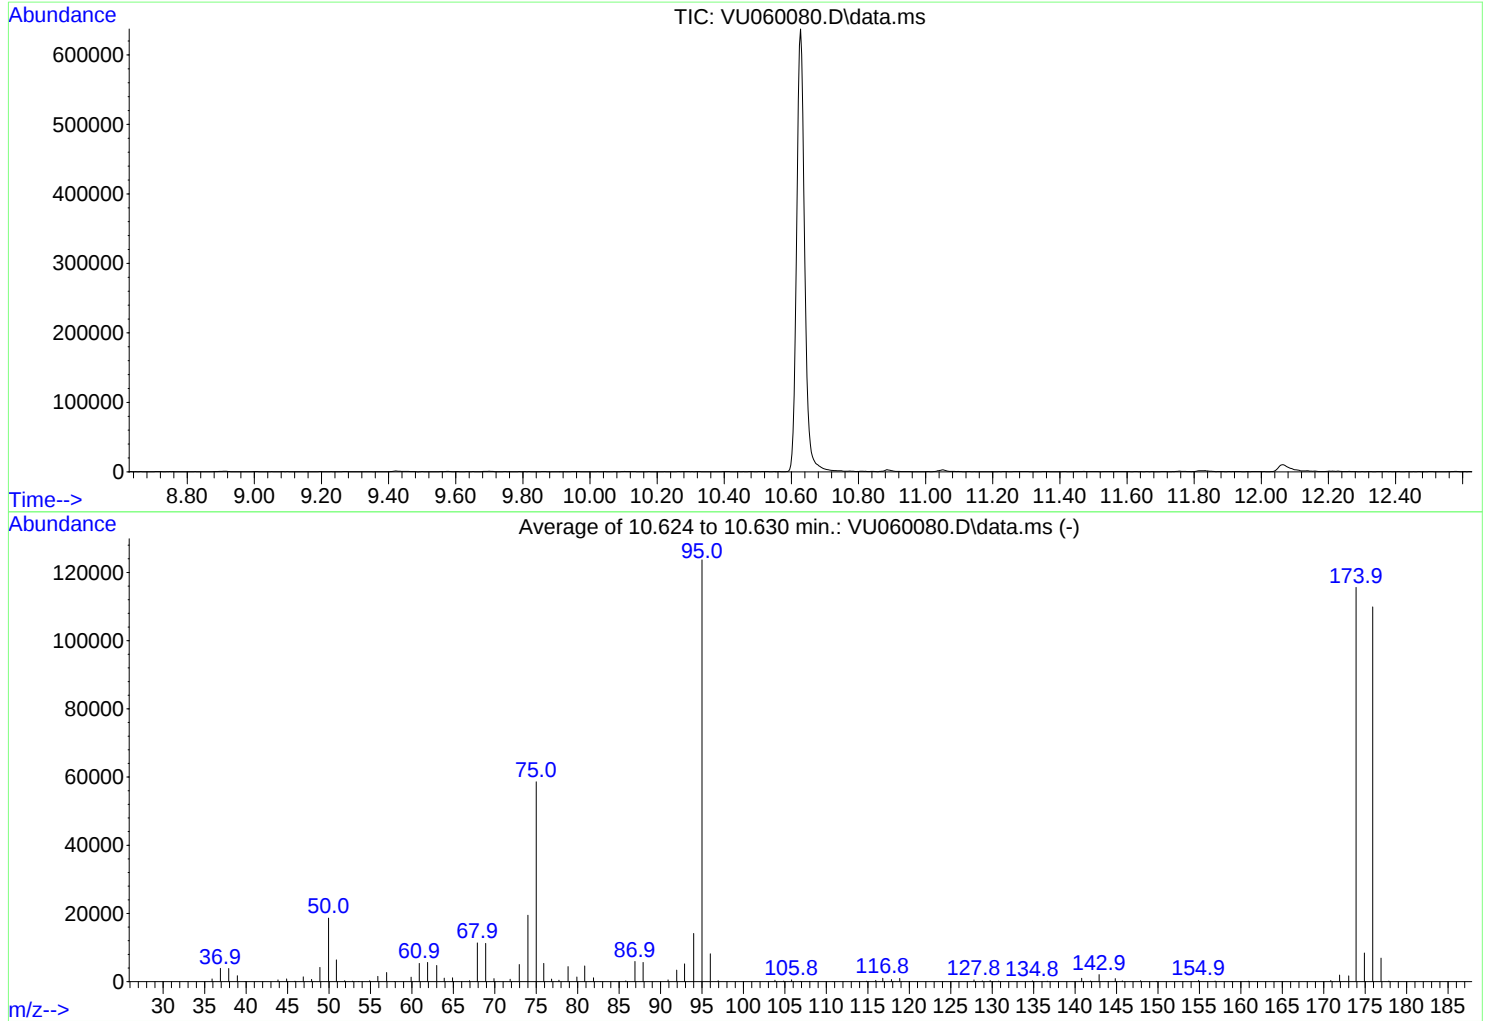

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	18637	PASS
75	95	30	80	47.4	58608	PASS
95	95	100	100	100.0	123699	PASS
96	95	5	9	6.6	8167	PASS
173	174	0.00	2	1.5	1683	PASS
174	95	50	120	93.5	115613	PASS
175	174	5	9	7.3	8392	PASS
176	174	95	101	95.1	109901	PASS
177	176	5	9	6.3	6893	PASS

m/z	Abundance
39.90	140.0
43.90	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
35.90	873.0
36.90	3956.0
37.90	3886.0
38.90	1706.0
40.00	182.0
43.90	808.0
44.90	836.0
45.90	148.0
46.90	1474.0
47.90	598.0
48.90	4159.0
49.90	18928.0
50.90	6597.0
51.90	304.0
52.80	119.0
53.60	103.0
54.90	281.0
55.90	1513.0
57.00	2675.0
59.90	1376.0
60.90	5316.0
61.90	5636.0
63.00	4745.0
63.90	1046.0
64.90	1180.0
67.00	249.0
67.90	11666.0
68.90	11320.0
69.90	794.0
71.80	691.0
73.00	4878.0
74.00	19504.0
75.00	58408.0
75.90	5342.0
76.90	772.0
77.80	421.0
78.90	4673.0
79.90	1346.0
80.80	4699.0
81.90	1086.0
85.80	243.0
86.90	6094.0
87.90	5598.0
90.90	495.0
92.00	3479.0
92.90	5274.0
94.00	14379.0
95.00	123816.0
96.00	8456.0
96.90	336.0
103.90	404.0
104.80	184.0
105.80	530.0
106.90	114.0
114.80	106.0
116.00	356.0
116.80	986.0
117.90	574.0
118.90	907.0
127.80	483.0
128.80	278.0
129.70	371.0
130.80	184.0
134.80	210.0
136.60	148.0
140.80	1027.0
141.90	167.0
142.90	2136.0
144.90	935.0
145.70	187.0
147.90	355.0
149.80	164.0
154.90	405.0
156.80	203.0
160.90	179.0
170.90	348.0
171.90	1866.0
173.00	1545.0
173.90	112992.0
174.90	8376.0
175.90	107288.0
176.90	6816.0
177.80	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
35.90	831.0
36.90	3989.0
37.90	3975.0
38.90	1766.0
39.90	171.0
43.80	748.0
44.90	808.0
45.90	165.0
46.90	1438.0
47.90	661.0
48.90	4349.0
49.90	19216.0
50.90	6599.0
51.90	303.0
52.90	170.0
54.90	271.0
55.90	1609.0
56.90	2720.0
57.90	104.0
59.90	1330.0
60.90	5541.0
61.90	5776.0
63.00	4903.0
63.90	1087.0
64.90	1174.0
66.00	106.0
67.00	289.0
67.90	11718.0
68.90	11565.0
69.90	900.0
71.90	754.0
72.90	5187.0
74.00	20144.0
75.00	60456.0
75.90	5513.0
76.90	756.0
77.70	439.0
78.90	4537.0
79.90	1399.0
80.90	4678.0
81.90	1150.0
85.80	270.0
86.90	5987.0
87.90	5939.0
90.90	522.0
92.00	3444.0
92.90	5402.0
94.00	14664.0
95.00	128144.0
96.00	8526.0
97.00	307.0
103.80	411.0
104.90	200.0
105.80	558.0
106.80	124.0
108.00	121.0
110.80	109.0
114.80	124.0
115.90	351.0
116.80	1031.0
117.90	637.0
118.80	970.0
127.80	535.0
128.80	260.0
129.70	354.0
130.80	184.0
134.90	224.0
136.70	162.0
140.80	1024.0
141.90	202.0
142.90	2165.0
144.90	911.0
145.70	250.0
147.90	317.0
149.80	126.0
154.90	400.0
156.90	183.0
160.90	169.0
170.80	325.0
171.90	2025.0
173.00	1723.0
173.90	119160.0
174.90	8622.0
175.90	113624.0
176.90	7029.0
177.80	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
35.90	661.0
36.90	3700.0
37.90	3732.0
39.00	1685.0
39.90	170.0
43.80	684.0
44.90	723.0
45.90	161.0
46.90	1272.0
47.90	667.0
48.90	4039.0
50.00	17768.0
50.90	5923.0
51.90	300.0
52.90	166.0
54.90	277.0
55.90	1510.0
56.90	2662.0
57.90	100.0
59.90	1170.0
60.90	5264.0
61.90	5464.0
63.00	4569.0
63.90	963.0
64.90	1072.0
66.00	106.0
66.90	311.0
67.90	10737.0
68.90	10728.0
69.90	924.0
71.90	708.0
72.90	5061.0
74.00	18832.0
75.00	56960.0
75.90	5202.0
76.80	791.0
77.80	439.0
78.80	4083.0
79.90	1304.0
80.90	4377.0
81.90	1095.0
82.80	110.0
85.80	260.0
86.90	5648.0
87.90	5393.0
90.90	506.0
91.90	3201.0
92.90	4943.0
94.00	13304.0
95.00	119136.0
96.00	7519.0
97.00	251.0
103.70	436.0
104.90	228.0
105.80	521.0
106.80	106.0
108.00	133.0
114.90	151.0
115.90	364.0
116.80	988.0
117.80	578.0
118.90	936.0
127.80	531.0
128.80	238.0
129.80	306.0
130.80	169.0
134.90	237.0
136.70	182.0
140.80	951.0
141.80	210.0
142.90	1922.0
144.00	102.0
144.80	855.0
145.70	253.0
147.90	247.0
154.90	384.0
157.00	180.0
158.90	120.0
160.90	117.0
170.80	284.0
171.90	1933.0
173.00	1780.0
173.90	114688.0
174.90	8177.0
175.90	108792.0
176.90	6833.0
177.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176