

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060195.D
 Acq On : 26 Jul 2024 01:02
 Operator : MD/SY
 Sample : VU0725WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 26 04:35:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 26 04:34:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	210949	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	217747	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	83385	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	80089	59.131	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	118.260%
7) Chloroethane-d5	1.907	69	65337	57.351	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.700%
11) 1,1-Dichloroethene-d2	2.560	63	93017	38.657	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.320%
21) 2-Butanone-d5	4.624	46	100002	106.241	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.240%
24) Chloroform-d	5.052	84	128577	49.021	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.040%
26) 1,2-Dichloroethane-d4	5.695	65	80589	51.675	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.340%
32) Benzene-d6	5.717	84	263799	47.311	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.620%
36) 1,2-Dichloropropane-d6	6.682	67	89537	51.884	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.760%
41) Toluene-d8	7.891	98	215274	40.598	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	8.177	79	33204	41.118	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.240%
47) 2-Hexanone-d5	8.631	63	57016	78.395	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.400%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	126307	47.685	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.380%
66) 1,2-Dichlorobenzene-d4	12.190	152	74450	48.588	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.180%
Target Compounds						
37) 1,2-Dichloropropane	6.685	63	8657	5.349	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060195.D
Acq On : 26 Jul 2024 01:02
Operator : MD/SY
Sample : VU0725WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jul 26 04:35:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 04:34:35 2024
Response via : Initial Calibration

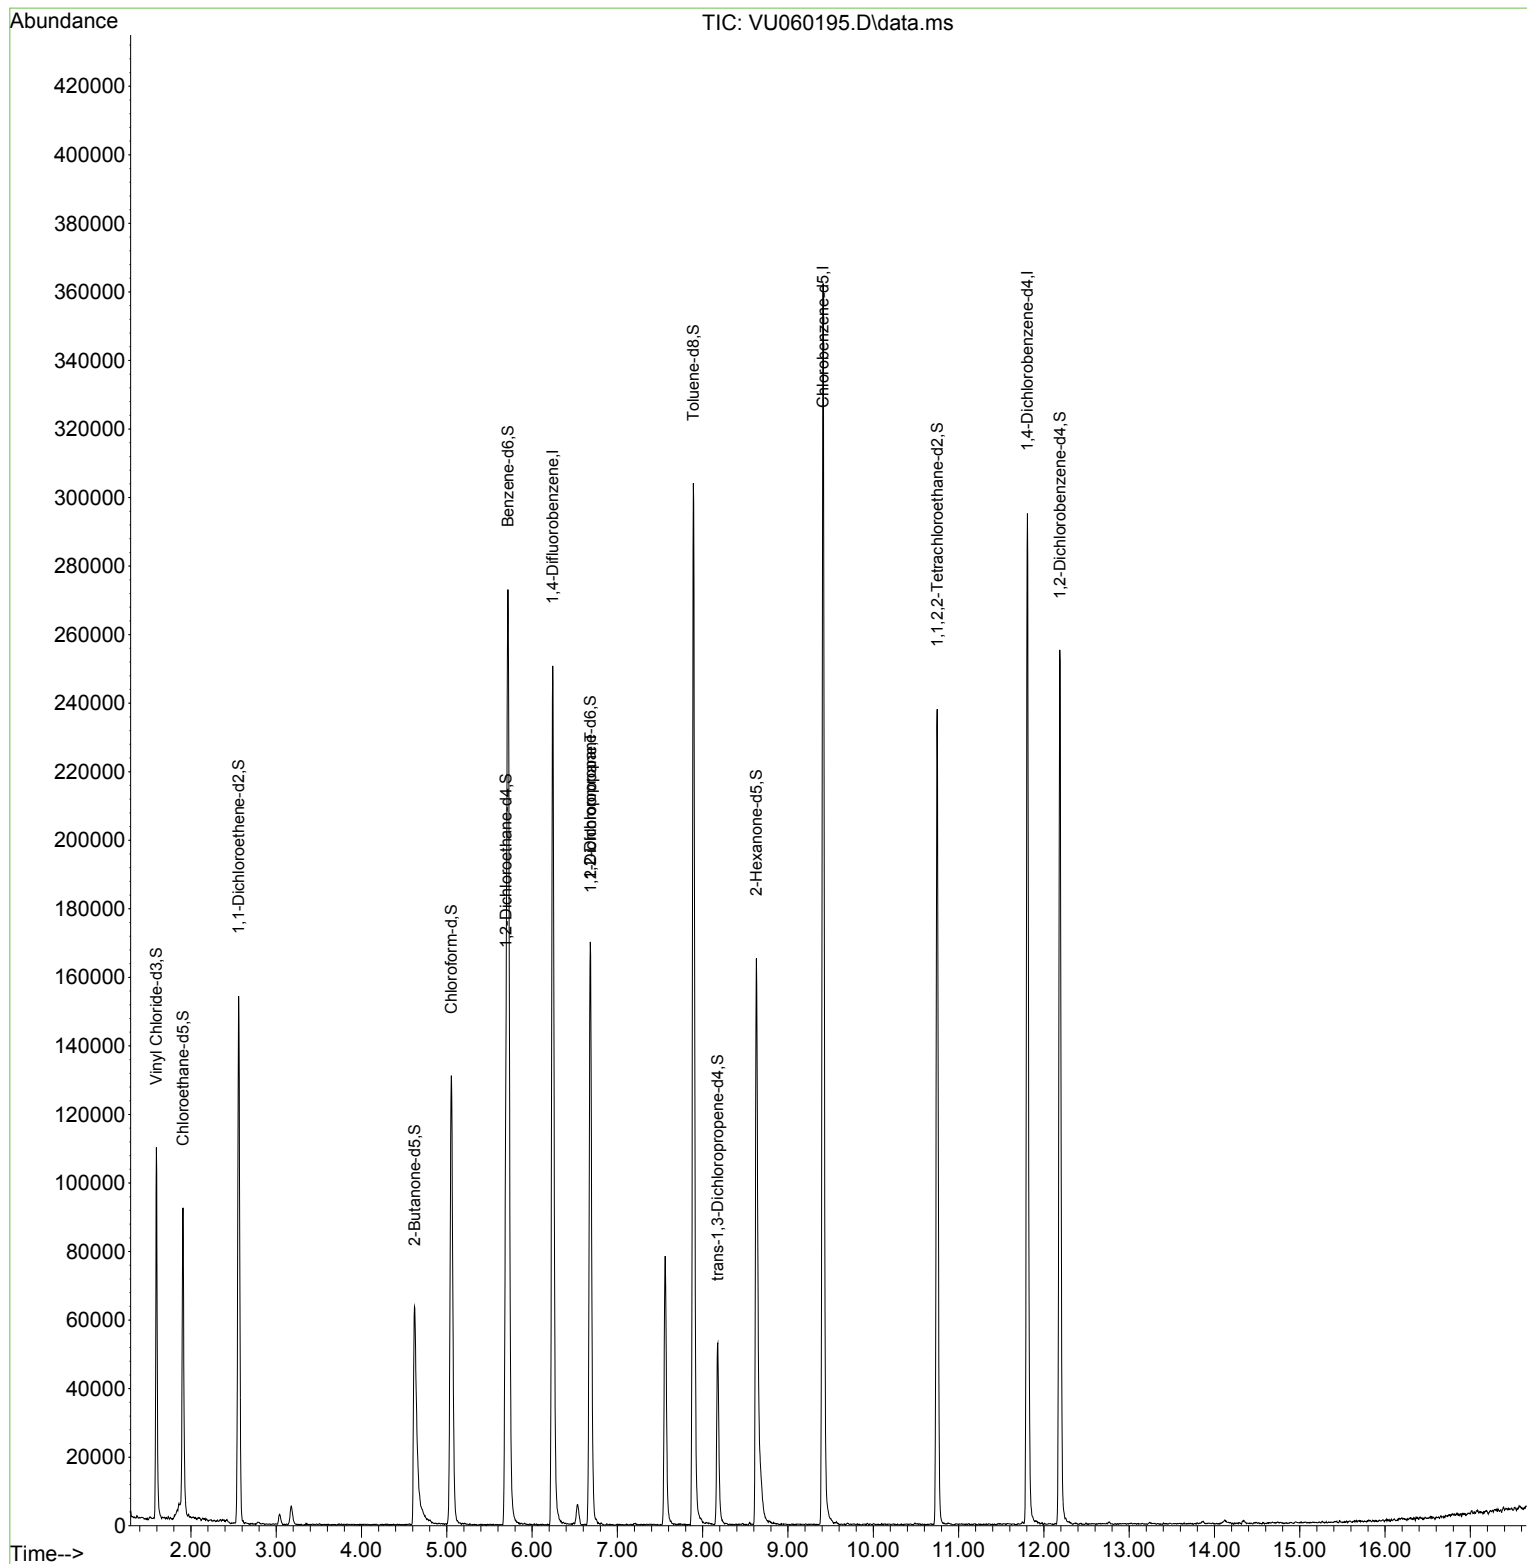

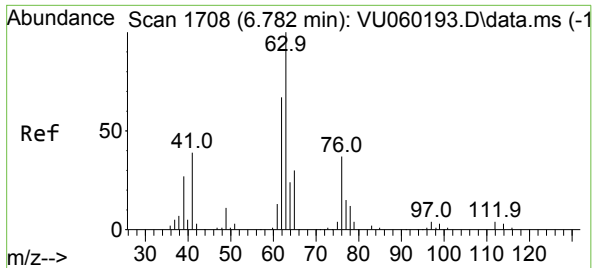

#37
1,2-Dichloropropane
Concen: 5.349 ug/L
RT: 6.685 min Scan# 1
Delta R.T. -0.097 min
Lab File: VU060195.D
Acq: 26 Jul 2024 01:02

Instrument :
MSVOA_U
ClientSampleId :

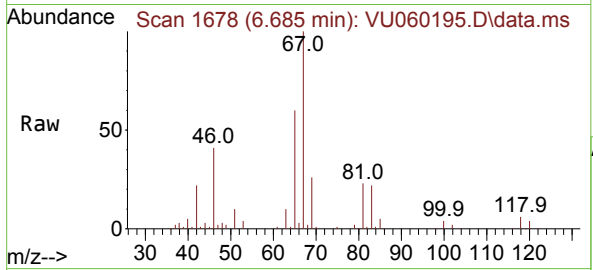

Tgt Ion: 63 Resp: 8657
Ion Ratio Lower Upper
63 100
112 0.0 3.0 4.6#

