

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060171.D
 Acq On : 25 Jul 2024 15:07
 Operator : MD/SY
 Sample : VU0725WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rBV	124623	148094	16.83%	2.228%
2	1.818	151	164	179	rVB9	6386	19238	2.19%	0.289%
3	1.904	182	191	212	rVB	92147	131872	14.98%	1.984%
4	2.319	317	320	322	rBV2	741	534	0.06%	0.008%
5	2.560	383	395	413	rBV	181447	298365	33.90%	4.488%
6	2.785	459	465	475	rVB2	663	965	0.11%	0.015%
7	3.043	536	545	556	rVB	2935	5435	0.62%	0.082%
8	3.171	580	585	594	rBV3	621	952	0.11%	0.014%
9	3.226	599	602	606	rVB2	284	271	0.03%	0.004%
10	3.599	714	718	724	rBV	193	208	0.02%	0.003%
11	4.007	842	845	850	rBV2	238	219	0.02%	0.003%
12	4.129	881	883	891	rVB2	253	287	0.03%	0.004%
13	4.210	902	908	911	rVV2	194	222	0.03%	0.003%
14	4.300	930	936	938	rBV2	342	393	0.04%	0.006%
15	4.425	970	975	980	rBV2	278	354	0.04%	0.005%
16	4.486	988	994	999	rBV2	334	472	0.05%	0.007%
17	4.570	1017	1020	1022	rBV2	306	181	0.02%	0.003%
18	4.618	1026	1035	1074	rBV	78462	209355	23.79%	3.149%
19	4.956	1138	1140	1144	rVB	458	223	0.03%	0.003%
20	5.055	1154	1171	1193	rBV	155586	345554	39.26%	5.198%
21	5.213	1218	1220	1224	rVB2	400	247	0.03%	0.004%
22	5.271	1234	1238	1240	rBV	249	200	0.02%	0.003%
23	5.403	1274	1279	1282	rBV	274	251	0.03%	0.004%
24	5.550	1321	1325	1327	rBV2	280	245	0.03%	0.004%
25	5.612	1341	1344	1348	rBV	235	214	0.02%	0.003%
26	5.718	1357	1377	1404	rBV2	325119	880193	100.00%	13.240%
27	6.007	1462	1467	1468	rBV2	366	201	0.02%	0.003%
28	6.078	1487	1489	1492	rVB2	374	212	0.02%	0.003%
29	6.155	1509	1513	1518	rVB2	241	284	0.03%	0.004%
30	6.187	1518	1523	1526	rBV2	166	214	0.02%	0.003%
31	6.242	1527	1540	1568	rBV	282152	551882	62.70%	8.302%
32	6.396	1586	1588	1595	rVB3	343	246	0.03%	0.004%
33	6.528	1620	1629	1645	rVB6	3968	7724	0.88%	0.116%
34	6.589	1645	1648	1653	rBV	222	243	0.03%	0.004%
35	6.682	1664	1677	1707	rVV	202653	399198	45.35%	6.005%
36	6.798	1710	1713	1716	rVV	543	417	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060171.D
 Acq On : 25 Jul 2024 15:07
 Operator : MD/SY
 Sample : VU0725WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.846	1724	1728	1732	rVB3	251	210	0.02%	0.003%
38	6.920	1747	1751	1754	rVV2	249	264	0.03%	0.004%
39	7.004	1772	1777	1782	rBV2	249	239	0.03%	0.004%
40	7.033	1782	1786	1791	rBV2	266	252	0.03%	0.004%
41	7.084	1799	1802	1807	rBV2	255	238	0.03%	0.004%
42	7.200	1833	1838	1840	rBV2	570	451	0.05%	0.007%
43	7.261	1854	1857	1862	rBV	229	187	0.02%	0.003%
44	7.287	1862	1865	1868	rBV	378	290	0.03%	0.004%
45	7.370	1888	1891	1899	rVB2	267	282	0.03%	0.004%
46	7.409	1899	1903	1906	rBV2	223	208	0.02%	0.003%
47	7.560	1939	1950	1969	rBV	99094	180072	20.46%	2.709%
48	7.891	2038	2053	2074	rBV	370828	657447	74.69%	9.890%
49	8.174	2131	2141	2163	rBV	68378	120177	13.65%	1.808%
50	8.306	2177	2182	2184	rVB3	298	279	0.03%	0.004%
51	8.332	2185	2190	2191	rBV2	271	201	0.02%	0.003%
52	8.409	2207	2214	2215	rBV	413	383	0.04%	0.006%
53	8.460	2226	2230	2239	rVB4	423	684	0.08%	0.010%
54	8.547	2253	2257	2258	rBV	448	291	0.03%	0.004%
55	8.631	2272	2283	2322	rBV2	210849	421353	47.87%	6.338%
56	8.898	2363	2366	2371	rVB3	347	284	0.03%	0.004%
57	8.923	2371	2374	2377	rBV	286	228	0.03%	0.003%
58	9.158	2442	2447	2452	rBV2	252	346	0.04%	0.005%
59	9.322	2495	2498	2503	rBV2	186	195	0.02%	0.003%
60	9.412	2512	2526	2552	rBV	410340	694601	78.91%	10.449%
61	9.701	2613	2616	2618	rVB2	353	226	0.03%	0.003%
62	9.766	2632	2636	2640	rBV2	226	295	0.03%	0.004%
63	9.910	2677	2681	2684	rBV2	238	239	0.03%	0.004%
64	9.991	2701	2706	2710	rBV	269	286	0.03%	0.004%
65	10.132	2747	2750	2753	rVB2	378	220	0.02%	0.003%
66	10.152	2753	2756	2763	rBV2	325	436	0.05%	0.007%
67	10.235	2778	2782	2786	rBV	314	326	0.04%	0.005%
68	10.335	2808	2813	2814	rBV	286	232	0.03%	0.003%
69	10.460	2849	2852	2854	rBV	303	256	0.03%	0.004%
70	10.576	2883	2888	2890	rBV2	313	284	0.03%	0.004%
71	10.647	2905	2910	2918	rBV3	529	666	0.08%	0.010%
72	10.750	2930	2942	2963	rVV	279394	454042	51.58%	6.830%
73	10.881	2978	2983	2990	rBV3	728	797	0.09%	0.012%
74	10.968	3006	3010	3015	rBV2	314	348	0.04%	0.005%
75	11.036	3025	3031	3035	rBV2	277	413	0.05%	0.006%
76	11.434	3149	3155	3156	rBV	277	284	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060171.D
 Acq On : 25 Jul 2024 15:07
 Operator : MD/SY
 Sample : VU0725WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.518	3179	3181	3191	rVB2	313	453	0.05%	0.007%
78	11.615	3208	3211	3217	rVB2	282	267	0.03%	0.004%
79	11.660	3219	3225	3230	rVB	330	483	0.05%	0.007%
80	11.692	3231	3235	3237	rBV	309	273	0.03%	0.004%
81	11.807	3259	3271	3298	rBV	334905	559389	63.55%	8.415%
82	12.187	3377	3389	3416	rBV	319960	535984	60.89%	8.063%
83	12.457	3468	3473	3475	rBV	334	299	0.03%	0.004%
84	12.708	3549	3551	3554	rBV	266	216	0.02%	0.003%
85	12.766	3563	3569	3573	rBV	875	914	0.10%	0.014%
86	12.811	3579	3583	3586	rBV2	388	379	0.04%	0.006%
87	12.872	3599	3602	3606	rBV2	244	231	0.03%	0.003%
88	12.994	3637	3640	3643	rBV2	363	241	0.03%	0.004%
89	13.241	3714	3717	3722	rBV	541	486	0.06%	0.007%
90	13.524	3800	3805	3810	rBV2	358	430	0.05%	0.006%
91	13.868	3909	3912	3918	rVB3	586	575	0.07%	0.009%
92	14.261	4031	4034	4037	rBV2	312	269	0.03%	0.004%
93	14.335	4054	4057	4058	rBV	348	213	0.02%	0.003%
94	14.344	4058	4060	4068	rVB4	772	682	0.08%	0.010%
95	14.479	4099	4102	4104	rBV2	250	189	0.02%	0.003%
96	14.602	4137	4140	4143	rBV	423	272	0.03%	0.004%
97	15.007	4260	4266	4267	rBV2	452	491	0.06%	0.007%
98	15.929	4550	4553	4555	rBV3	634	467	0.05%	0.007%
99	16.052	4588	4591	4592	rBV	643	328	0.04%	0.005%
100	16.129	4612	4615	4619	rBV3	744	645	0.07%	0.010%




Sum of corrected areas: 6647853

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060171.D
Acq On : 25 Jul 2024 15:07
Operator : MD/SY
Sample : VU0725WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

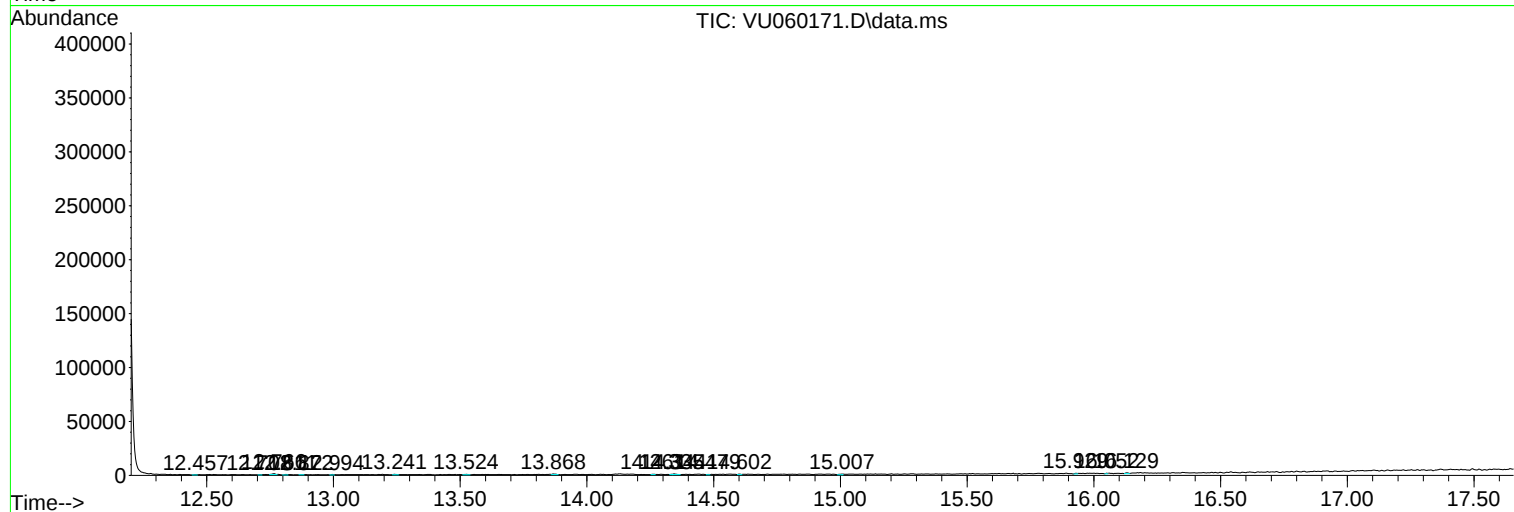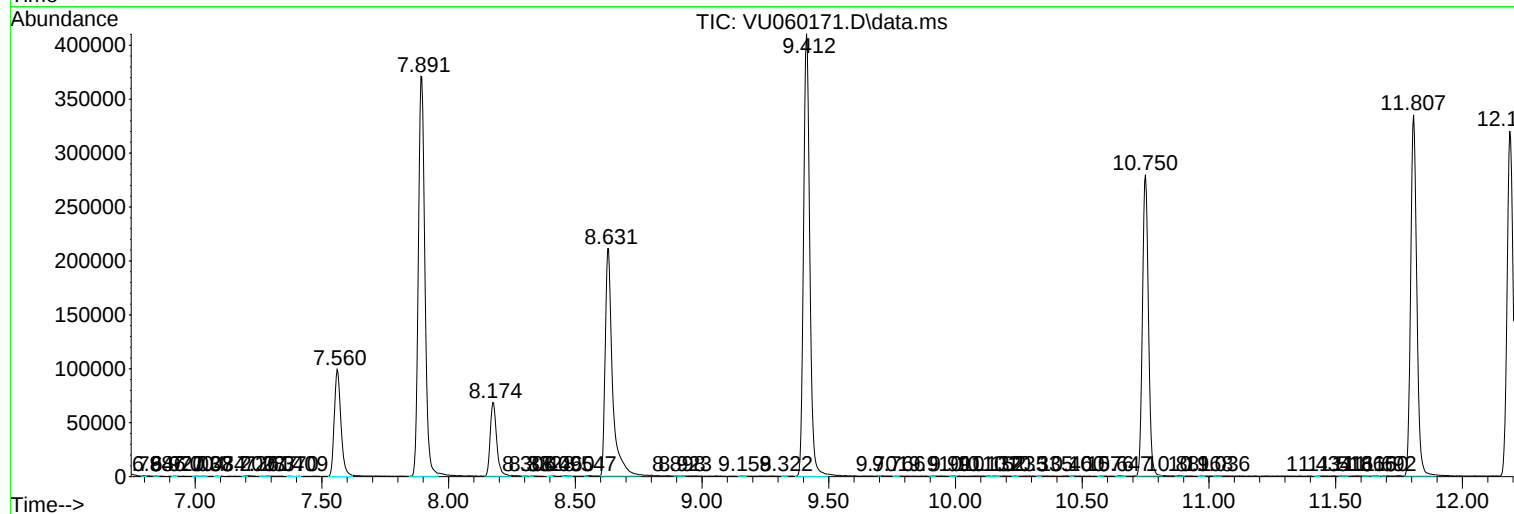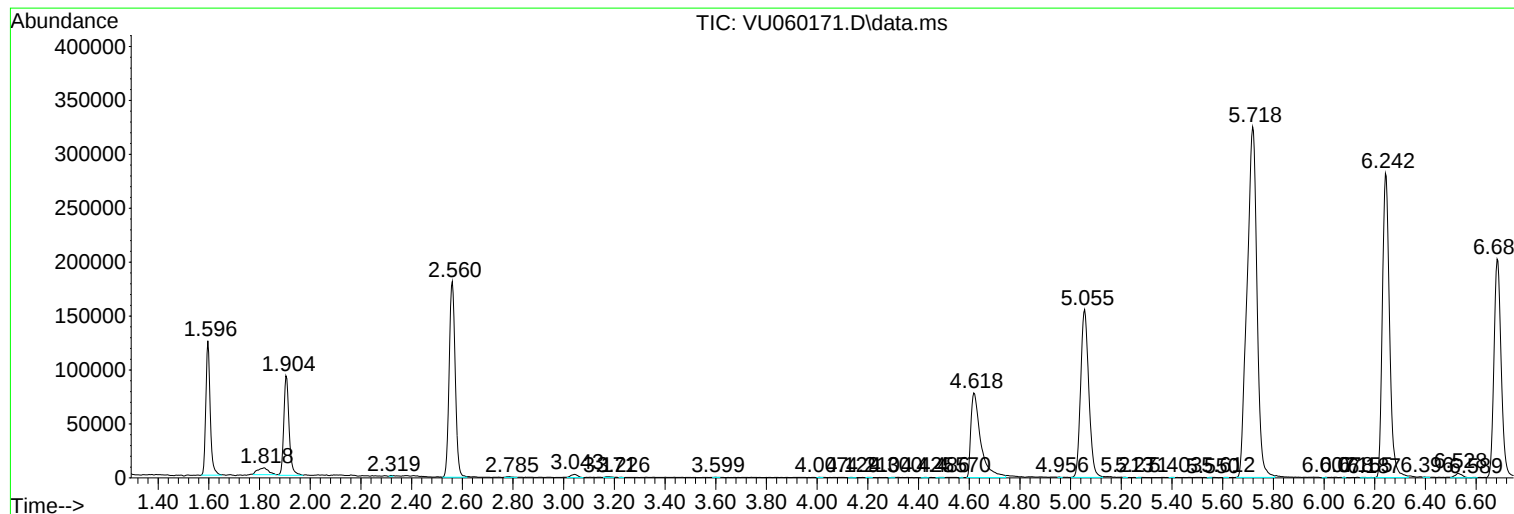

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060171.D
Acq On : 25 Jul 2024 15:07
Operator : MD/SY
Sample : VU0725WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060171.D
Acq On : 25 Jul 2024 15:07
Operator : MD/SY
Sample : VU0725WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------