

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060172.D
 Acq On : 25 Jul 2024 15:33
 Operator : MD/SY
 Sample : P3334-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rBV	98125	117630	17.52%	2.180%
2	1.904	182	191	212	rVB	70780	101163	15.07%	1.875%
3	2.557	382	394	414	rBV	141578	229866	34.24%	4.260%
4	2.756	454	456	459	rBV2	264	178	0.03%	0.003%
5	2.785	460	465	474	rVB4	634	982	0.15%	0.018%
6	3.039	533	544	559	rBV2	12754	25123	3.74%	0.466%
7	3.178	576	587	604	rVB2	2783	6597	0.98%	0.122%
8	3.621	721	725	731	rBV2	137	177	0.03%	0.003%
9	3.885	804	807	812	rVB2	243	228	0.03%	0.004%
10	3.923	816	819	826	rBV	179	208	0.03%	0.004%
11	4.460	983	986	992	rVB2	177	220	0.03%	0.004%
12	4.496	992	997	999	rBV	167	179	0.03%	0.003%
13	4.618	1025	1035	1064	rBV	61475	160940	23.98%	2.983%
14	4.991	1148	1151	1154	rBV2	223	181	0.03%	0.003%
15	5.055	1155	1171	1194	rVV	120522	266416	39.69%	4.938%
16	5.296	1242	1246	1251	rBV2	404	346	0.05%	0.006%
17	5.338	1255	1259	1268	rVB2	329	345	0.05%	0.006%
18	5.409	1277	1281	1285	rVB2	235	198	0.03%	0.004%
19	5.583	1333	1335	1342	rVB	302	349	0.05%	0.006%
20	5.618	1342	1346	1350	rBV2	361	416	0.06%	0.008%
21	5.718	1357	1377	1407	rBV2	247425	671260	100.00%	12.441%
22	5.866	1419	1423	1426	rBV2	466	347	0.05%	0.006%
23	5.927	1438	1442	1446	rVB2	434	393	0.06%	0.007%
24	6.042	1475	1478	1482	rVB	379	278	0.04%	0.005%
25	6.091	1490	1493	1500	rVB2	219	242	0.04%	0.004%
26	6.126	1500	1504	1507	rBV	358	304	0.05%	0.006%
27	6.171	1514	1518	1522	rVB2	318	256	0.04%	0.005%
28	6.242	1527	1540	1570	rBV	256831	506059	75.39%	9.379%
29	6.483	1611	1615	1618	rBV2	227	178	0.03%	0.003%
30	6.531	1622	1630	1641	rVV6	3325	6112	0.91%	0.113%
31	6.605	1650	1653	1656	rBV	319	227	0.03%	0.004%
32	6.682	1665	1677	1696	rBV	153595	301653	44.94%	5.591%
33	6.894	1740	1743	1749	rBV	306	385	0.06%	0.007%
34	6.946	1755	1759	1763	rVB	335	276	0.04%	0.005%
35	7.084	1800	1802	1806	rVB2	266	184	0.03%	0.003%
36	7.110	1806	1810	1814	rVB2	242	203	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060172.D
 Acq On : 25 Jul 2024 15:33
 Operator : MD/SY
 Sample : P3334-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.145	1817	1821	1825	rBV2	261	294	0.04%	0.005%
38	7.219	1839	1844	1846	rBV2	277	279	0.04%	0.005%
39	7.251	1852	1854	1860	rBV	308	291	0.04%	0.005%
40	7.296	1864	1868	1872	rBV2	276	338	0.05%	0.006%
41	7.390	1892	1897	1900	rBV2	236	237	0.04%	0.004%
42	7.560	1939	1950	1967	rBV	75928	135316	20.16%	2.508%
43	7.894	2041	2054	2076	rBV	276906	492370	73.35%	9.125%
44	8.100	2113	2118	2122	rBV4	323	399	0.06%	0.007%
45	8.174	2131	2141	2169	rBV2	50052	89252	13.30%	1.654%
46	8.335	2188	2191	2194	rBV	266	202	0.03%	0.004%
47	8.457	2226	2229	2232	rBV3	475	354	0.05%	0.007%
48	8.496	2238	2241	2244	rBV	248	184	0.03%	0.003%
49	8.515	2244	2247	2251	rVB	236	173	0.03%	0.003%
50	8.563	2258	2262	2265	rVB	399	327	0.05%	0.006%
51	8.589	2265	2270	2272	rBV	261	244	0.04%	0.005%
52	8.627	2272	2282	2322	rBV	157492	321198	47.85%	5.953%
53	8.881	2358	2361	2364	rBV	360	253	0.04%	0.005%
54	9.161	2444	2448	2450	rVB2	205	177	0.03%	0.003%
55	9.177	2450	2453	2458	rBV2	263	282	0.04%	0.005%
56	9.287	2480	2487	2491	rBV2	180	278	0.04%	0.005%
57	9.316	2492	2496	2503	rVB2	333	379	0.06%	0.007%
58	9.412	2513	2526	2556	rBV	377879	644347	95.99%	11.942%
59	9.570	2572	2575	2583	rBV3	312	310	0.05%	0.006%
60	10.033	2716	2719	2721	rBV	250	173	0.03%	0.003%
61	10.103	2738	2741	2745	rVB2	250	203	0.03%	0.004%
62	10.132	2745	2750	2755	rVB2	272	331	0.05%	0.006%
63	10.457	2848	2851	2855	rVB2	224	194	0.03%	0.004%
64	10.486	2855	2860	2864	rBV3	391	481	0.07%	0.009%
65	10.602	2890	2896	2898	rBV	237	286	0.04%	0.005%
66	10.750	2930	2942	2960	rBV	217408	354232	52.77%	6.565%
67	10.888	2980	2985	2988	rVV2	383	395	0.06%	0.007%
68	10.904	2988	2990	2994	rVB2	352	205	0.03%	0.004%
69	11.161	3067	3070	3075	rVB2	242	214	0.03%	0.004%
70	11.193	3075	3080	3082	rBV2	268	250	0.04%	0.005%
71	11.451	3155	3160	3165	rBV2	292	342	0.05%	0.006%
72	11.476	3165	3168	3174	rVV3	442	467	0.07%	0.009%
73	11.505	3175	3177	3186	rVB2	380	319	0.05%	0.006%
74	11.557	3186	3193	3196	rBV2	342	444	0.07%	0.008%
75	11.643	3216	3220	3224	rVB2	256	222	0.03%	0.004%
76	11.682	3229	3232	3234	rBV	322	251	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060172.D
 Acq On : 25 Jul 2024 15:33
 Operator : MD/SY
 Sample : P3334-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.807	3259	3271	3297	rBV	310578	526003	78.36%	9.749%
78	11.952	3313	3316	3322	rBV2	393	429	0.06%	0.008%
79	12.004	3328	3332	3335	rBV3	557	624	0.09%	0.012%
80	12.058	3344	3349	3352	rBV2	254	291	0.04%	0.005%
81	12.187	3377	3389	3411	rBV	243367	414349	61.73%	7.679%
82	12.444	3465	3469	3475	rVB	455	546	0.08%	0.010%
83	12.483	3476	3481	3483	rBV2	345	323	0.05%	0.006%
84	12.605	3514	3519	3520	rBV2	314	311	0.05%	0.006%
85	12.743	3557	3562	3564	rBV2	431	432	0.06%	0.008%
86	12.759	3564	3567	3568	rBV2	367	237	0.04%	0.004%
87	12.991	3634	3639	3642	rBV	448	471	0.07%	0.009%
88	13.431	3769	3776	3780	rBV2	412	636	0.09%	0.012%
89	13.630	3835	3838	3840	rBV	244	205	0.03%	0.004%
90	13.676	3849	3852	3857	rVB2	286	205	0.03%	0.004%
91	13.865	3908	3911	3913	rBV	550	303	0.05%	0.006%
92	13.981	3944	3947	3950	rBV2	269	233	0.03%	0.004%
93	14.132	3985	3994	3997	rBV3	662	1130	0.17%	0.021%
94	14.232	4023	4025	4029	rVB2	390	246	0.04%	0.005%
95	14.396	4073	4076	4077	rBV2	272	178	0.03%	0.003%
96	14.409	4077	4080	4083	rVV2	426	323	0.05%	0.006%
97	14.798	4197	4201	4204	rBV2	692	474	0.07%	0.009%
98	14.962	4249	4252	4257	rBV2	373	366	0.05%	0.007%
99	15.666	4470	4471	4477	rBV3	510	365	0.05%	0.007%
100	15.926	4550	4552	4557	rVB2	668	403	0.06%	0.007%




Sum of corrected areas: 5395675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060172.D
Acq On : 25 Jul 2024 15:33
Operator : MD/SY
Sample : P3334-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

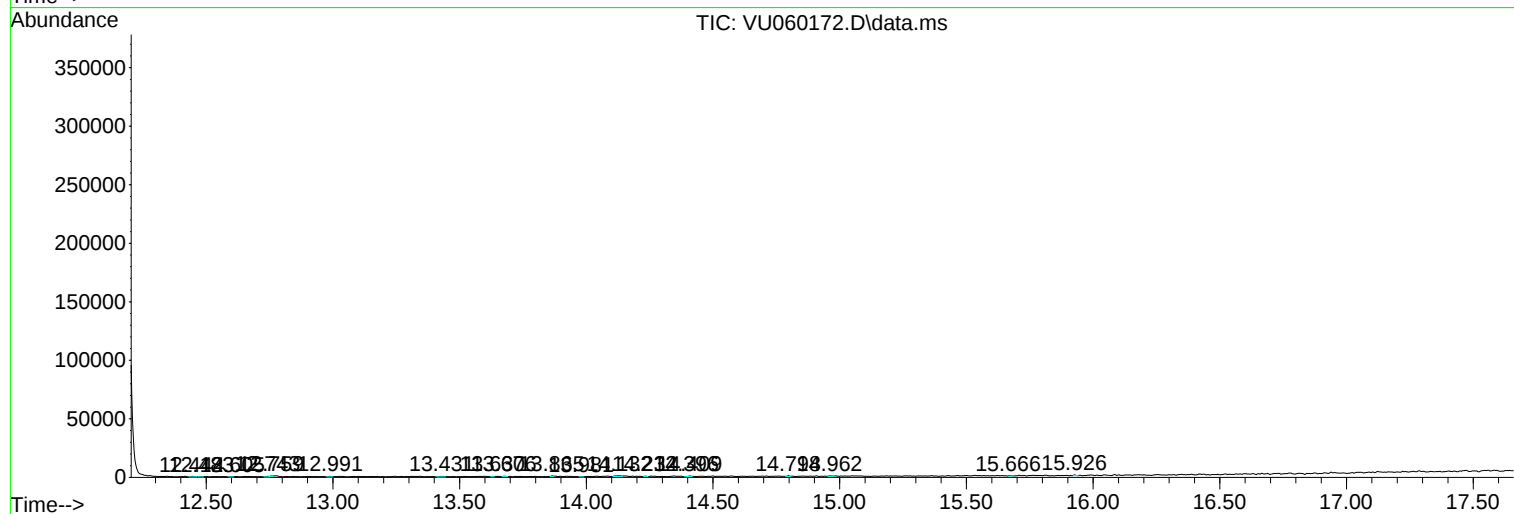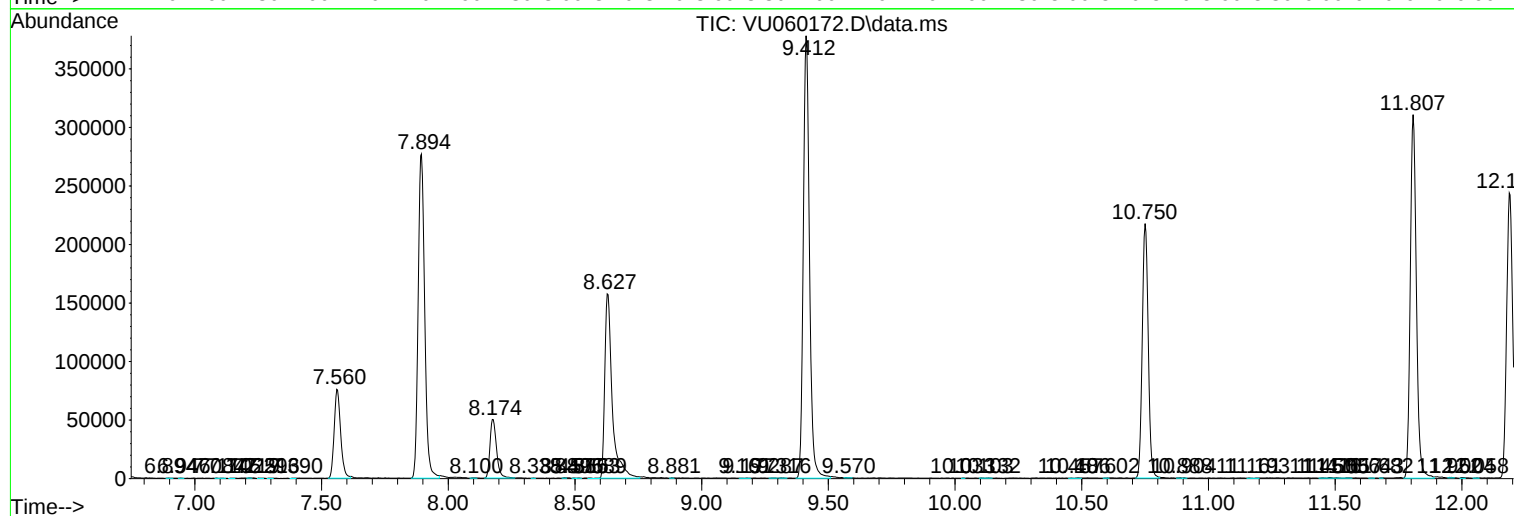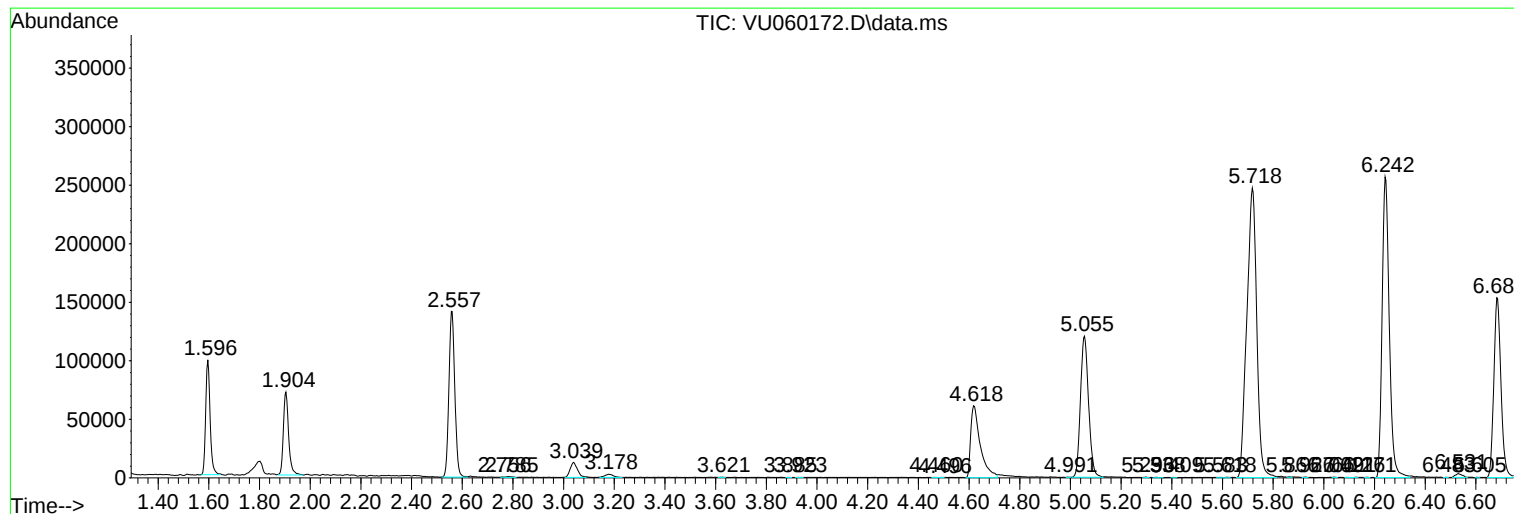

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060172.D
Acq On : 25 Jul 2024 15:33
Operator : MD/SY
Sample : P3334-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060172.D
Acq On : 25 Jul 2024 15:33
Operator : MD/SY
Sample : P3334-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------