

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060173.D
 Acq On : 25 Jul 2024 15:57
 Operator : MD/SY
 Sample : P3327-31 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	110	rBV	97811	116355	17.19%	2.164%
2	1.904	183	191	209	rVB	70425	98454	14.55%	1.831%
3	2.238	293	295	298	rBV2	684	276	0.04%	0.005%
4	2.560	383	395	411	rBV	142596	229624	33.93%	4.270%
5	2.682	431	433	438	rBV2	323	230	0.03%	0.004%
6	3.039	532	544	560	rBV2	12262	25354	3.75%	0.472%
7	3.177	579	587	589	rBV3	877	1076	0.16%	0.020%
8	3.573	705	710	715	rVB	314	362	0.05%	0.007%
9	3.611	719	722	725	rBV2	299	230	0.03%	0.004%
10	3.711	748	753	757	rBV	300	369	0.05%	0.007%
11	3.865	791	801	810	rBV2	916	1827	0.27%	0.034%
12	4.004	838	844	847	rBV2	271	343	0.05%	0.006%
13	4.299	934	936	942	rVB2	338	278	0.04%	0.005%
14	4.357	952	954	959	rVB2	361	300	0.04%	0.006%
15	4.389	959	964	966	rBV	229	237	0.04%	0.004%
16	4.525	1003	1006	1009	rVB	241	189	0.03%	0.004%
17	4.621	1026	1036	1077	rBV	62626	201546	29.78%	3.748%
18	5.055	1156	1171	1194	rBV2	118347	265071	39.16%	4.930%
19	5.222	1219	1223	1225	rBV2	302	260	0.04%	0.005%
20	5.463	1294	1298	1305	rVB2	260	268	0.04%	0.005%
21	5.534	1314	1320	1324	rBV2	324	360	0.05%	0.007%
22	5.637	1349	1352	1356	rBV	297	263	0.04%	0.005%
23	5.717	1357	1377	1406	rBV2	249658	676819	100.00%	12.587%
24	6.055	1476	1482	1485	rVB2	221	201	0.03%	0.004%
25	6.242	1528	1540	1576	rBV	257452	500116	73.89%	9.301%
26	6.534	1620	1631	1644	rVV8	7255	15268	2.26%	0.284%
27	6.611	1651	1655	1659	rBV2	431	320	0.05%	0.006%
28	6.682	1663	1677	1706	rVV	156057	306501	45.29%	5.700%
29	6.804	1710	1715	1716	rBV2	515	369	0.05%	0.007%
30	6.894	1739	1743	1748	rVB	323	353	0.05%	0.007%
31	6.920	1748	1751	1754	rBV2	247	185	0.03%	0.003%
32	6.946	1754	1759	1763	rVB2	240	245	0.04%	0.005%
33	6.968	1763	1766	1769	rBV2	276	208	0.03%	0.004%
34	7.020	1778	1782	1785	rVV2	287	188	0.03%	0.003%
35	7.196	1830	1837	1840	rBV2	364	368	0.05%	0.007%
36	7.364	1886	1889	1893	rBV	204	196	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060173.D
 Acq On : 25 Jul 2024 15:57
 Operator : MD/SY
 Sample : P3327-31 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.425	1904	1908	1911	rBV2	192	191	0.03%	0.004%
38	7.467	1916	1921	1925	rBV	245	293	0.04%	0.005%
39	7.560	1939	1950	1971	rVV	74727	133631	19.74%	2.485%
40	7.659	1978	1981	1986	rBV3	266	267	0.04%	0.005%
41	7.717	1996	1999	2002	rBV	456	405	0.06%	0.008%
42	7.894	2041	2054	2072	rBV	272225	484248	71.55%	9.006%
43	8.177	2131	2142	2161	rBV	50751	88747	13.11%	1.650%
44	8.280	2172	2174	2178	rVB	409	201	0.03%	0.004%
45	8.402	2209	2212	2220	rVB2	356	398	0.06%	0.007%
46	8.447	2220	2226	2227	rBV	277	235	0.03%	0.004%
47	8.630	2272	2283	2321	rBV2	159550	327435	48.38%	6.089%
48	8.852	2349	2352	2356	rVB3	418	310	0.05%	0.006%
49	8.994	2392	2396	2398	rBV	391	317	0.05%	0.006%
50	9.087	2419	2425	2428	rBV2	214	276	0.04%	0.005%
51	9.177	2448	2453	2459	rVB2	282	421	0.06%	0.008%
52	9.222	2465	2467	2476	rVB2	287	311	0.05%	0.006%
53	9.412	2514	2526	2550	rBV	367885	627349	92.69%	11.667%
54	9.608	2584	2587	2592	rBV2	269	194	0.03%	0.004%
55	9.836	2653	2658	2661	rBV	252	273	0.04%	0.005%
56	9.978	2696	2702	2706	rBV2	252	370	0.05%	0.007%
57	10.023	2710	2716	2720	rBV2	341	376	0.06%	0.007%
58	10.061	2722	2728	2732	rBV2	234	295	0.04%	0.005%
59	10.302	2796	2803	2807	rBV2	265	379	0.06%	0.007%
60	10.537	2871	2876	2879	rBV2	228	221	0.03%	0.004%
61	10.698	2922	2926	2928	rBV2	241	191	0.03%	0.004%
62	10.749	2929	2942	2960	rVV	222037	355413	52.51%	6.610%
63	10.891	2981	2986	2993	rBV3	495	640	0.09%	0.012%
64	11.023	3024	3027	3033	rVV2	236	297	0.04%	0.006%
65	11.206	3080	3084	3087	rBV2	244	255	0.04%	0.005%
66	11.238	3091	3094	3098	rBV2	293	237	0.04%	0.004%
67	11.454	3156	3161	3164	rBV2	285	283	0.04%	0.005%
68	11.666	3224	3227	3233	rBV	255	263	0.04%	0.005%
69	11.695	3233	3236	3242	rVB2	227	249	0.04%	0.005%
70	11.730	3242	3247	3249	rBV2	306	293	0.04%	0.005%
71	11.756	3249	3255	3258	rVB2	445	334	0.05%	0.006%
72	11.807	3258	3271	3291	rBV	300044	498320	73.63%	9.267%
73	12.068	3349	3352	3355	rVB	294	204	0.03%	0.004%
74	12.122	3365	3369	3372	rBV2	299	292	0.04%	0.005%
75	12.187	3377	3389	3416	rBV	234803	399445	59.02%	7.429%
76	12.627	3521	3526	3528	rBV	230	200	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060173.D
 Acq On : 25 Jul 2024 15:57
 Operator : MD/SY
 Sample : P3327-31 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.765	3562	3569	3571	rBV4	669	764	0.11%	0.014%
78	12.810	3579	3583	3587	rBV2	338	274	0.04%	0.005%
79	12.926	3615	3619	3624	rVB2	327	307	0.05%	0.006%
80	13.090	3665	3670	3677	rVV2	334	479	0.07%	0.009%
81	13.138	3678	3685	3689	rBV2	377	518	0.08%	0.010%
82	13.219	3706	3710	3714	rBV	247	239	0.04%	0.004%
83	13.322	3740	3742	3745	rBV	252	189	0.03%	0.004%
84	13.376	3757	3759	3764	rBV2	220	232	0.03%	0.004%
85	13.560	3812	3816	3818	rBV	260	230	0.03%	0.004%
86	13.743	3868	3873	3877	rBV2	410	354	0.05%	0.007%
87	13.830	3896	3900	3902	rBV	400	317	0.05%	0.006%
88	13.871	3910	3913	3916	rBV2	575	374	0.06%	0.007%
89	14.109	3983	3987	3988	rBV2	434	293	0.04%	0.005%
90	14.283	4034	4041	4044	rBV2	296	438	0.06%	0.008%
91	14.344	4058	4060	4064	rVB2	557	357	0.05%	0.007%
92	14.386	4069	4073	4077	rVB2	272	248	0.04%	0.005%
93	14.424	4081	4085	4087	rBV2	641	517	0.08%	0.010%
94	14.569	4126	4130	4135	rBV2	600	676	0.10%	0.013%
95	14.894	4229	4231	4235	rBV3	344	248	0.04%	0.005%
96	15.161	4311	4314	4316	rBV	483	294	0.04%	0.005%
97	15.264	4344	4346	4348	rBV2	373	185	0.03%	0.003%
98	15.383	4381	4383	4385	rBV	578	263	0.04%	0.005%
99	15.527	4426	4428	4430	rBV	511	268	0.04%	0.005%
100	15.855	4527	4530	4532	rBV2	596	375	0.06%	0.007%




Sum of corrected areas: 5377107

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060173.D
Acq On : 25 Jul 2024 15:57
Operator : MD/SY
Sample : P3327-31 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

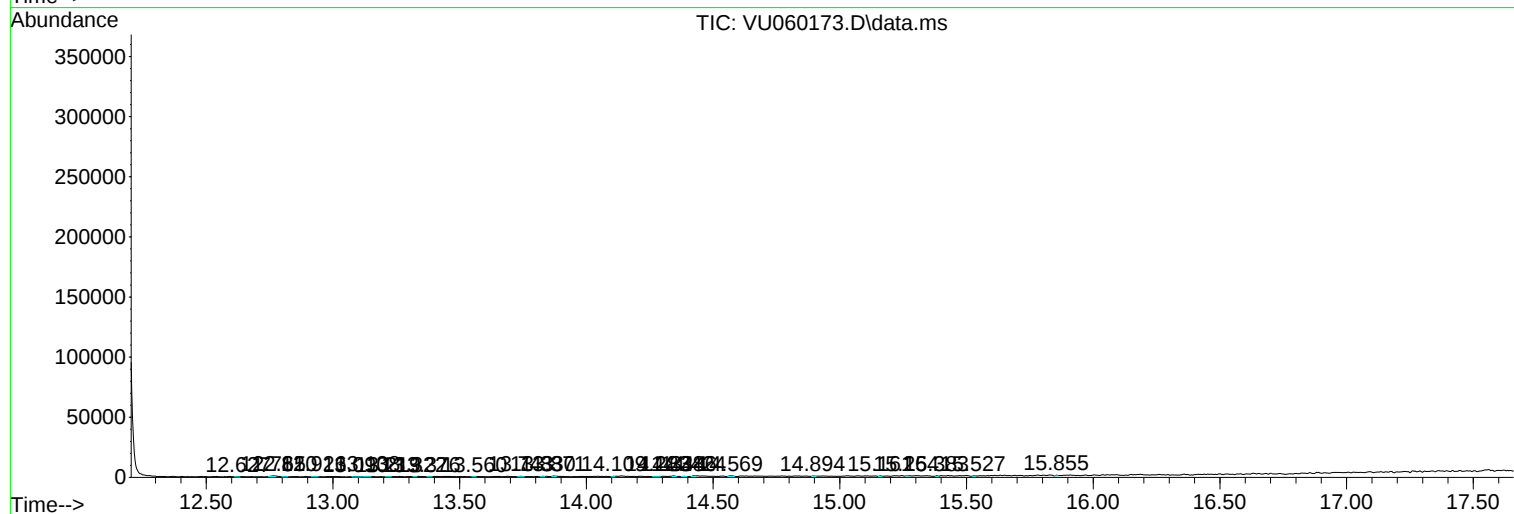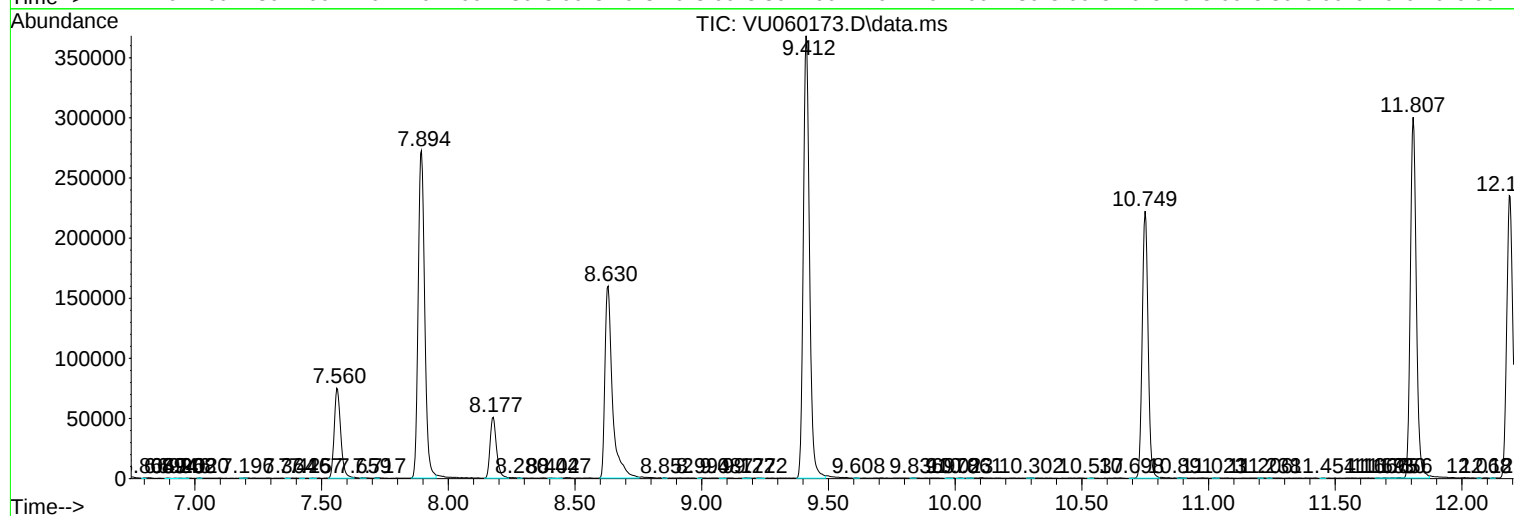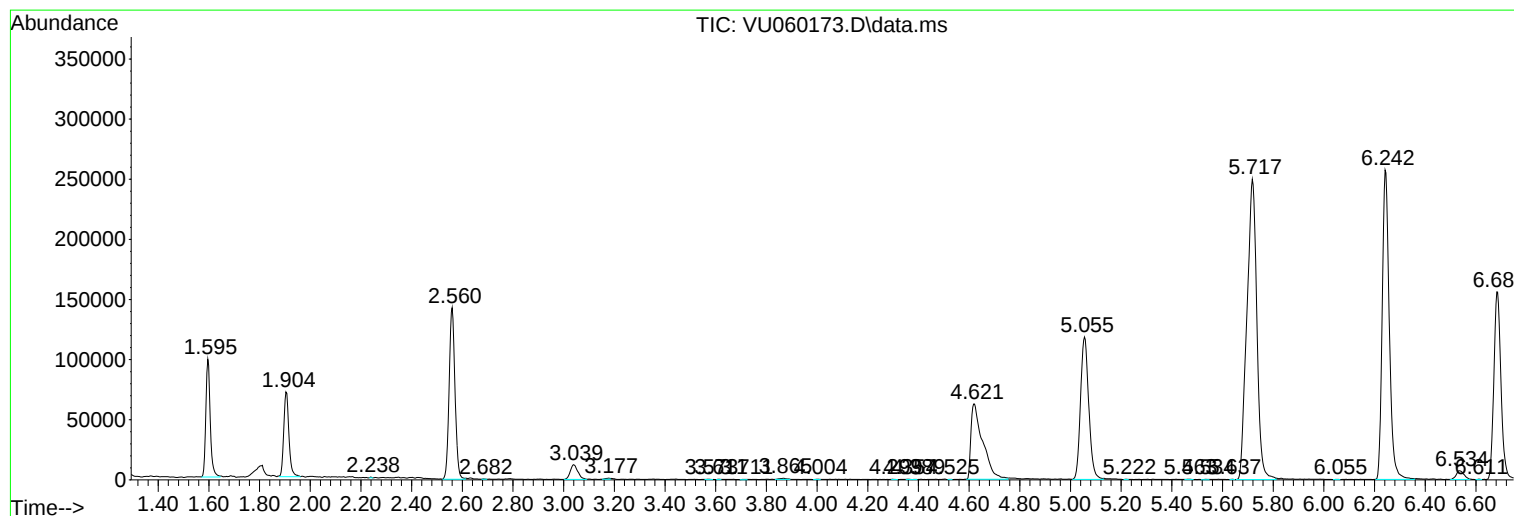

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060173.D
Acq On : 25 Jul 2024 15:57
Operator : MD/SY
Sample : P3327-31 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060173.D
Acq On : 25 Jul 2024 15:57
Operator : MD/SY
Sample : P3327-31 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------