

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060174.D
 Acq On : 25 Jul 2024 16:19
 Operator : MD/SY
 Sample : P3260-07DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	115	rVB	102764	123478	17.10%	2.042%
2	1.904	182	191	210	rVB	75828	106919	14.80%	1.768%
3	2.560	383	395	411	rBV	148465	243172	33.67%	4.021%
4	2.782	458	464	467	rBV2	440	580	0.08%	0.010%
5	2.956	515	518	521	rBV	255	216	0.03%	0.004%
6	3.042	534	545	560	rVB2	5917	11734	1.62%	0.194%
7	3.177	574	587	609	rVB2	9560	21863	3.03%	0.362%
8	3.267	609	615	618	rVB	215	229	0.03%	0.004%
9	3.483	677	682	685	rBV2	313	317	0.04%	0.005%
10	3.547	699	702	705	rVB	269	202	0.03%	0.003%
11	3.628	724	727	730	rBV	240	191	0.03%	0.003%
12	3.824	784	788	790	rBV2	314	242	0.03%	0.004%
13	3.962	824	831	835	rBV	293	432	0.06%	0.007%
14	4.097	865	873	876	rVB2	274	400	0.06%	0.007%
15	4.248	917	920	923	rBV2	261	187	0.03%	0.003%
16	4.621	1023	1036	1066	rBV	69493	188407	26.09%	3.115%
17	4.972	1141	1145	1150	rBV3	268	260	0.04%	0.004%
18	5.055	1153	1171	1200	rBV	125998	284611	39.41%	4.706%
19	5.187	1209	1212	1216	rVB2	536	438	0.06%	0.007%
20	5.210	1216	1219	1222	rBV2	355	227	0.03%	0.004%
21	5.255	1231	1233	1237	rVB2	298	264	0.04%	0.004%
22	5.290	1242	1244	1250	rVV2	385	297	0.04%	0.005%
23	5.370	1268	1269	1273	rVB	340	178	0.02%	0.003%
24	5.438	1286	1290	1299	rBV2	190	214	0.03%	0.004%
25	5.534	1314	1320	1322	rBV2	223	253	0.04%	0.004%
26	5.647	1352	1355	1358	rBV	278	200	0.03%	0.003%
27	5.718	1358	1377	1404	rBV2	266125	722236	100.00%	11.943%
28	5.965	1451	1454	1455	rBV	358	181	0.03%	0.003%
29	6.036	1471	1476	1480	rVB2	392	359	0.05%	0.006%
30	6.126	1501	1504	1507	rVB	301	210	0.03%	0.003%
31	6.242	1528	1540	1567	rBV	264775	511535	70.83%	8.459%
32	6.438	1598	1601	1604	rBV3	233	167	0.02%	0.003%
33	6.457	1604	1607	1612	rVB3	240	256	0.04%	0.004%
34	6.534	1621	1631	1644	rVB5	6473	12612	1.75%	0.209%
35	6.589	1644	1648	1653	rVB2	283	227	0.03%	0.004%
36	6.682	1664	1677	1698	rBV	167145	327519	45.35%	5.416%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060174.D
 Acq On : 25 Jul 2024 16:19
 Operator : MD/SY
 Sample : P3260-07DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.862	1728	1733	1734	rBV2	297	214	0.03%	0.004%
38	7.039	1784	1788	1791	rVB	212	160	0.02%	0.003%
39	7.084	1798	1802	1805	rVB	224	182	0.03%	0.003%
40	7.103	1805	1808	1810	rBV2	257	181	0.03%	0.003%
41	7.200	1831	1838	1840	rBV2	499	377	0.05%	0.006%
42	7.335	1873	1880	1882	rBV2	221	257	0.04%	0.004%
43	7.412	1901	1904	1907	rBV	309	235	0.03%	0.004%
44	7.502	1926	1932	1935	rBV	233	262	0.04%	0.004%
45	7.560	1939	1950	1973	rBV2	80141	145469	20.14%	2.405%
46	7.656	1978	1980	1983	rVB2	452	248	0.03%	0.004%
47	7.717	1993	1999	2006	rVB4	517	864	0.12%	0.014%
48	7.746	2006	2008	2010	rBV	297	172	0.02%	0.003%
49	7.785	2016	2020	2022	rBV	321	255	0.04%	0.004%
50	7.891	2041	2053	2076	rBV	297905	526085	72.84%	8.699%
51	8.116	2119	2123	2127	rVB2	368	317	0.04%	0.005%
52	8.177	2128	2142	2164	rBV	56251	98591	13.65%	1.630%
53	8.457	2225	2229	2230	rBV2	230	179	0.02%	0.003%
54	8.502	2238	2243	2245	rBV	258	252	0.03%	0.004%
55	8.547	2245	2257	2273	rVV	222058	376094	52.07%	6.219%
56	8.627	2273	2282	2321	rVB2	175071	357032	49.43%	5.904%
57	8.836	2342	2347	2350	rBV3	595	427	0.06%	0.007%
58	8.968	2386	2388	2392	rVB2	217	160	0.02%	0.003%
59	9.081	2416	2423	2426	rBV2	677	679	0.09%	0.011%
60	9.412	2511	2526	2559	rBV	388358	656791	90.94%	10.860%
61	9.569	2572	2575	2580	rVB3	612	563	0.08%	0.009%
62	9.698	2612	2615	2618	rVB2	287	194	0.03%	0.003%
63	9.746	2624	2630	2632	rBV2	235	229	0.03%	0.004%
64	9.823	2650	2654	2656	rBV	226	160	0.02%	0.003%
65	9.862	2663	2666	2668	rBV	224	160	0.02%	0.003%
66	10.023	2712	2716	2718	rBV	235	174	0.02%	0.003%
67	10.061	2726	2728	2731	rBV	238	162	0.02%	0.003%
68	10.328	2808	2811	2814	rBV2	215	176	0.02%	0.003%
69	10.373	2822	2825	2828	rBV	377	264	0.04%	0.004%
70	10.486	2857	2860	2862	rBV	273	201	0.03%	0.003%
71	10.749	2929	2942	2962	rBV	233392	381240	52.79%	6.304%
72	10.856	2971	2975	2977	rBV2	195	164	0.02%	0.003%
73	10.888	2980	2985	2993	rVB4	615	871	0.12%	0.014%
74	10.926	2994	2997	3001	rBV2	204	203	0.03%	0.003%
75	10.965	3006	3009	3018	rVB2	378	482	0.07%	0.008%
76	11.020	3022	3026	3028	rBV	234	203	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060174.D
 Acq On : 25 Jul 2024 16:19
 Operator : MD/SY
 Sample : P3260-07DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.071	3037	3042	3045	rBV	254	291	0.04%	0.005%
78	11.126	3053	3059	3062	rBV2	237	274	0.04%	0.005%
79	11.328	3119	3122	3129	rBV2	435	536	0.07%	0.009%
80	11.367	3129	3134	3138	rBV2	231	317	0.04%	0.005%
81	11.434	3147	3155	3159	rBV	358	526	0.07%	0.009%
82	11.499	3171	3175	3179	rBV2	359	281	0.04%	0.005%
83	11.807	3257	3271	3302	rBV	308229	507455	70.26%	8.391%
84	12.048	3343	3346	3350	rVB2	243	213	0.03%	0.004%
85	12.187	3377	3389	3413	rBV	251870	421630	58.38%	6.972%
86	12.338	3433	3436	3438	rBV2	683	352	0.05%	0.006%
87	12.454	3468	3472	3477	rBV2	256	259	0.04%	0.004%
88	12.531	3486	3496	3500	rBV2	413	684	0.09%	0.011%
89	12.550	3500	3502	3506	rVV	280	203	0.03%	0.003%
90	12.711	3549	3552	3555	rBV2	322	208	0.03%	0.003%
91	12.756	3562	3566	3567	rBV	568	402	0.06%	0.007%
92	13.354	3750	3752	3755	rVB2	318	176	0.02%	0.003%
93	13.370	3755	3757	3759	rBV2	250	174	0.02%	0.003%
94	13.473	3786	3789	3792	rBV	216	159	0.02%	0.003%
95	13.563	3814	3817	3820	rBV	231	166	0.02%	0.003%
96	13.907	3922	3924	3927	rVB2	337	199	0.03%	0.003%
97	14.052	3965	3969	3971	rBV	255	192	0.03%	0.003%
98	14.392	4072	4075	4082	rVB3	589	512	0.07%	0.008%
99	14.907	4232	4235	4238	rBV2	449	336	0.05%	0.006%
100	15.055	4278	4281	4283	rBV	346	238	0.03%	0.004%




Sum of corrected areas: 6047525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060174.D
Acq On : 25 Jul 2024 16:19
Operator : MD/SY
Sample : P3260-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

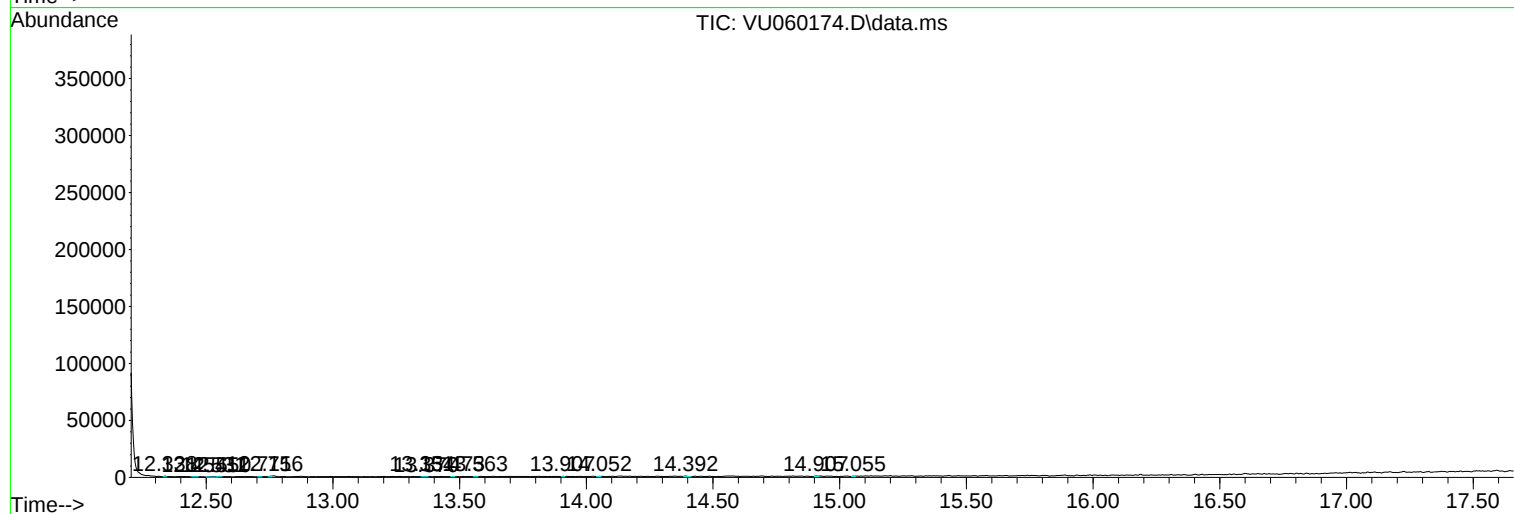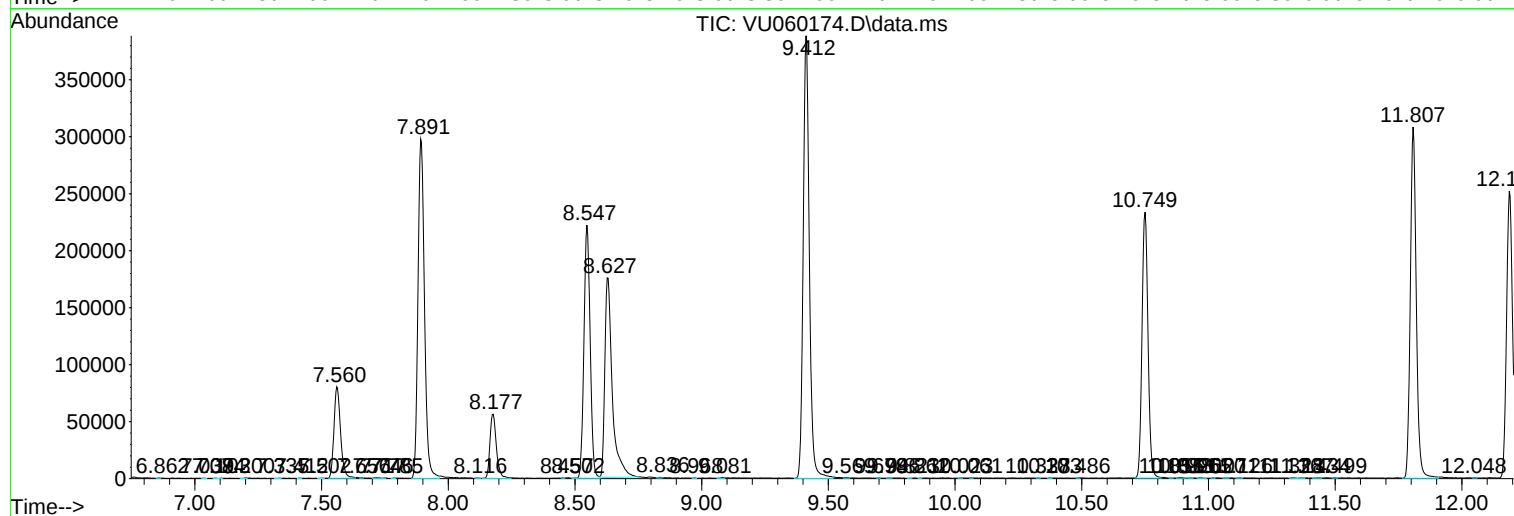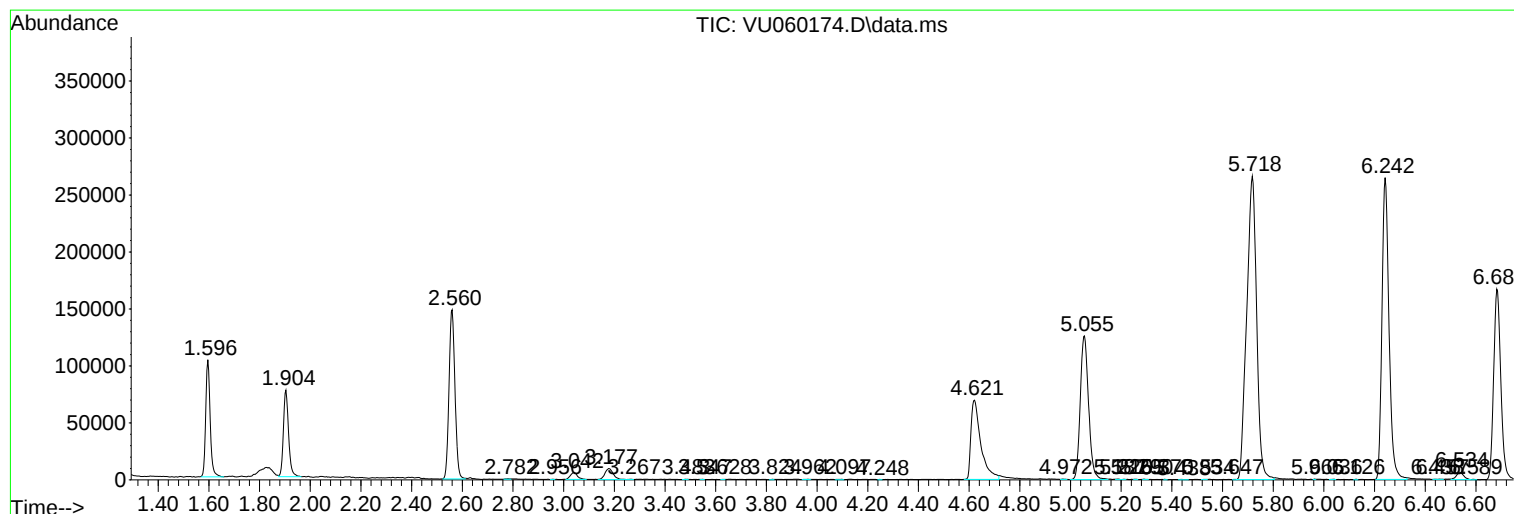

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060174.D
Acq On : 25 Jul 2024 16:19
Operator : MD/SY
Sample : P3260-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060174.D
Acq On : 25 Jul 2024 16:19
Operator : MD/SY
Sample : P3260-07DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------