

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060175.D
 Acq On : 25 Jul 2024 16:43
 Operator : MD/SY
 Sample : P3260-09DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	117	rVB	96604	128509	16.82%	2.005%
2	1.894	182	188	211	rVB	86431	166314	21.77%	2.595%
3	2.554	381	393	412	rBV	159019	259908	34.02%	4.056%
4	2.721	442	445	449	rVB	507	426	0.06%	0.007%
5	2.827	475	478	487	rVB	266	344	0.05%	0.005%
6	3.039	533	544	558	rVB3	6396	13436	1.76%	0.210%
7	3.177	570	587	605	rBV	13305	31259	4.09%	0.488%
8	3.306	624	627	631	rBV2	266	194	0.03%	0.003%
9	3.335	631	636	637	rBV	241	203	0.03%	0.003%
10	3.656	733	736	743	rVB2	262	221	0.03%	0.003%
11	3.689	743	746	749	rBV2	235	192	0.03%	0.003%
12	4.055	856	860	863	rBV2	251	253	0.03%	0.004%
13	4.296	932	935	943	rVB	324	311	0.04%	0.005%
14	4.332	943	946	953	rVB2	305	397	0.05%	0.006%
15	4.386	959	963	967	rVB2	231	228	0.03%	0.004%
16	4.544	1009	1012	1018	rVB2	283	298	0.04%	0.005%
17	4.624	1026	1037	1085	rBV	69179	200220	26.21%	3.124%
18	4.853	1104	1108	1112	rBV4	396	345	0.05%	0.005%
19	4.898	1120	1122	1126	rBV	356	223	0.03%	0.003%
20	5.052	1155	1170	1191	rBV	132001	296864	38.86%	4.632%
21	5.283	1236	1242	1248	rBV3	368	501	0.07%	0.008%
22	5.328	1253	1256	1265	rVB2	263	399	0.05%	0.006%
23	5.380	1265	1272	1273	rBV2	221	259	0.03%	0.004%
24	5.576	1330	1333	1340	rVV2	192	262	0.03%	0.004%
25	5.714	1358	1376	1404	rBV2	285775	764022	100.00%	11.922%
26	5.872	1423	1425	1431	rVB2	413	288	0.04%	0.004%
27	5.920	1436	1440	1445	rBV3	163	196	0.03%	0.003%
28	5.981	1454	1459	1460	rBV2	329	245	0.03%	0.004%
29	6.151	1508	1512	1518	rVB2	315	306	0.04%	0.005%
30	6.184	1518	1522	1527	rVB2	192	235	0.03%	0.004%
31	6.242	1527	1540	1571	rBV	267621	526406	68.90%	8.214%
32	6.406	1586	1591	1594	rVB3	380	296	0.04%	0.005%
33	6.431	1594	1599	1603	rBV2	554	549	0.07%	0.009%
34	6.483	1612	1615	1621	rBV2	444	485	0.06%	0.008%
35	6.537	1621	1632	1645	rVB2	6021	13105	1.72%	0.204%
36	6.589	1645	1648	1650	rBV3	532	441	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060175.D
 Acq On : 25 Jul 2024 16:43
 Operator : MD/SY
 Sample : P3260-09DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.682	1664	1677	1696	rBV	175636	345061	45.16%	5.384%
38	7.020	1778	1782	1785	rBV2	240	196	0.03%	0.003%
39	7.042	1785	1789	1792	rVV2	307	277	0.04%	0.004%
40	7.145	1815	1821	1823	rBV2	324	349	0.05%	0.005%
41	7.264	1851	1858	1860	rBV	226	227	0.03%	0.004%
42	7.309	1869	1872	1878	rVB2	157	181	0.02%	0.003%
43	7.428	1907	1909	1915	rBV2	179	185	0.02%	0.003%
44	7.508	1931	1934	1939	rVB2	232	201	0.03%	0.003%
45	7.560	1939	1950	1973	rBV2	84983	153440	20.08%	2.394%
46	7.672	1982	1985	1988	rBV	343	301	0.04%	0.005%
47	7.714	1993	1998	2003	rBV3	465	578	0.08%	0.009%
48	7.782	2015	2019	2022	rBV	181	196	0.03%	0.003%
49	7.891	2041	2053	2078	rBV	320003	558541	73.11%	8.716%
50	8.174	2128	2141	2162	rBV	58240	102078	13.36%	1.593%
51	8.547	2243	2257	2273	rBV2	218281	371663	48.65%	5.799%
52	8.634	2274	2284	2326	rVB	189106	397559	52.04%	6.204%
53	8.839	2345	2348	2352	rVB2	294	184	0.02%	0.003%
54	8.859	2352	2354	2361	rVB3	265	252	0.03%	0.004%
55	9.074	2419	2421	2425	rVV2	246	195	0.03%	0.003%
56	9.167	2446	2450	2459	rVV2	254	300	0.04%	0.005%
57	9.354	2502	2508	2509	rBV2	249	249	0.03%	0.004%
58	9.412	2514	2526	2554	rBV	387778	658051	86.13%	10.268%
59	9.701	2611	2616	2620	rBV2	339	363	0.05%	0.006%
60	9.862	2661	2666	2668	rBV2	198	186	0.02%	0.003%
61	9.955	2691	2695	2696	rBV	253	185	0.02%	0.003%
62	10.039	2717	2721	2725	rBV2	365	433	0.06%	0.007%
63	10.454	2846	2850	2856	rBV	152	210	0.03%	0.003%
64	10.553	2877	2881	2884	rBV2	331	263	0.03%	0.004%
65	10.656	2910	2913	2917	rVB2	254	210	0.03%	0.003%
66	10.749	2930	2942	2959	rBV	257520	417496	54.64%	6.515%
67	10.946	2999	3003	3006	rBV2	222	207	0.03%	0.003%
68	11.093	3046	3049	3052	rBV	259	206	0.03%	0.003%
69	11.238	3091	3094	3097	rBV	240	212	0.03%	0.003%
70	11.386	3136	3140	3148	rVB2	275	400	0.05%	0.006%
71	11.425	3149	3152	3158	rBV2	218	271	0.04%	0.004%
72	11.515	3177	3180	3185	rVB2	251	233	0.03%	0.004%
73	11.544	3185	3189	3191	rBV2	271	226	0.03%	0.004%
74	11.807	3259	3271	3294	rBV	322961	524807	68.69%	8.189%
75	11.958	3314	3318	3320	rBV2	363	316	0.04%	0.005%
76	12.013	3332	3335	3339	rVB2	332	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060175.D
 Acq On : 25 Jul 2024 16:43
 Operator : MD/SY
 Sample : P3260-09DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.036	3340	3342	3350	rVB3	436	394	0.05%	0.006%
78	12.077	3351	3355	3357	rBV	255	190	0.02%	0.003%
79	12.135	3370	3373	3377	rBV2	211	194	0.03%	0.003%
80	12.190	3377	3390	3413	rBV	276555	455571	59.63%	7.109%
81	12.344	3436	3438	3441	rBV3	385	210	0.03%	0.003%
82	12.370	3443	3446	3450	rBV3	363	321	0.04%	0.005%
83	12.601	3515	3518	3522	rBV	287	199	0.03%	0.003%
84	12.646	3531	3532	3541	rBV2	331	423	0.06%	0.007%
85	12.762	3563	3568	3571	rBV2	663	764	0.10%	0.012%
86	12.904	3610	3612	3618	rVB2	318	273	0.04%	0.004%
87	13.254	3717	3721	3723	rBV	441	405	0.05%	0.006%
88	13.473	3786	3789	3793	rVB	412	304	0.04%	0.005%
89	13.515	3794	3802	3804	rBV2	422	597	0.08%	0.009%
90	14.306	4046	4048	4052	rBV2	238	206	0.03%	0.003%
91	14.495	4105	4107	4110	rBV	383	241	0.03%	0.004%
92	14.756	4185	4188	4191	rVB3	403	248	0.03%	0.004%
93	14.775	4191	4194	4195	rBV	307	213	0.03%	0.003%
94	14.932	4241	4243	4247	rVB	600	357	0.05%	0.006%
95	14.958	4248	4251	4252	rBV	307	180	0.02%	0.003%
96	15.174	4315	4318	4323	rBV4	481	503	0.07%	0.008%
97	15.209	4327	4329	4333	rVV2	626	415	0.05%	0.006%
98	15.232	4333	4336	4347	rVB3	597	934	0.12%	0.015%
99	15.434	4396	4399	4400	rBV	430	198	0.03%	0.003%
100	15.801	4511	4513	4515	rBV3	655	370	0.05%	0.006%




Sum of corrected areas: 6408590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060175.D
Acq On : 25 Jul 2024 16:43
Operator : MD/SY
Sample : P3260-09DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

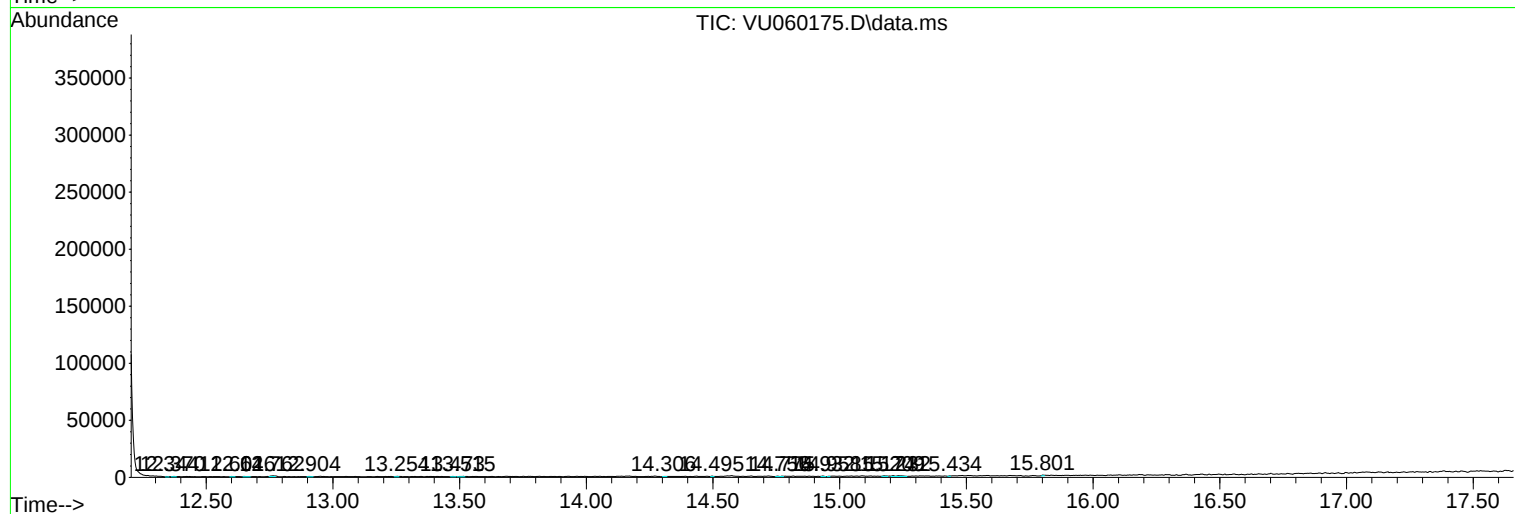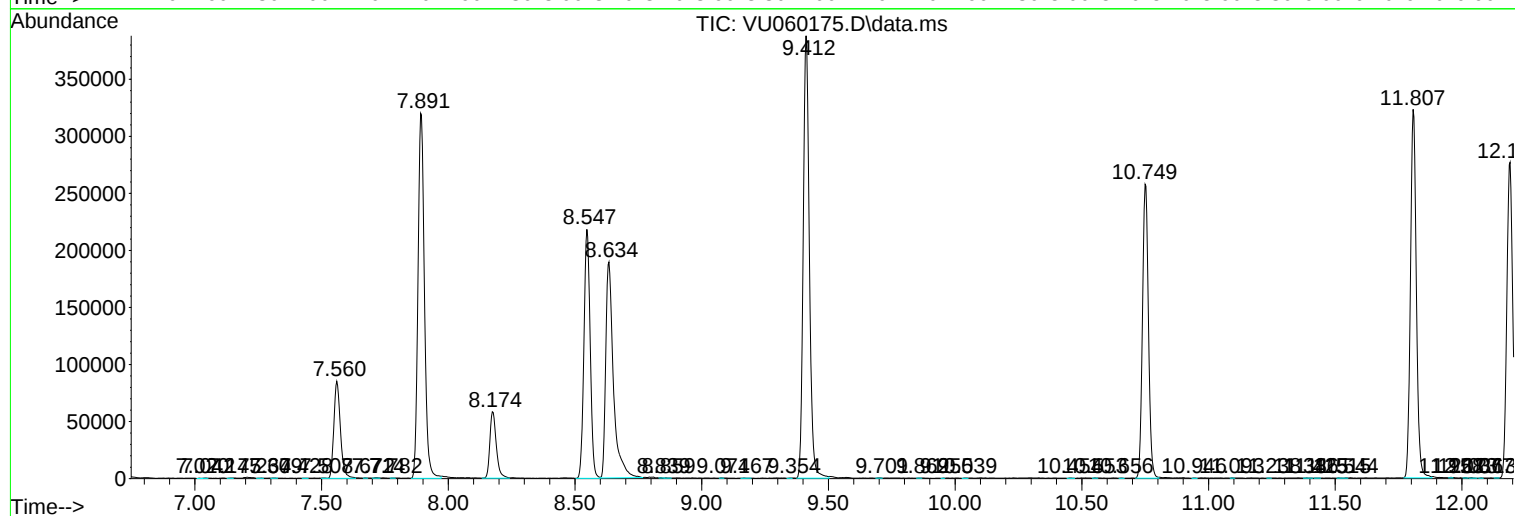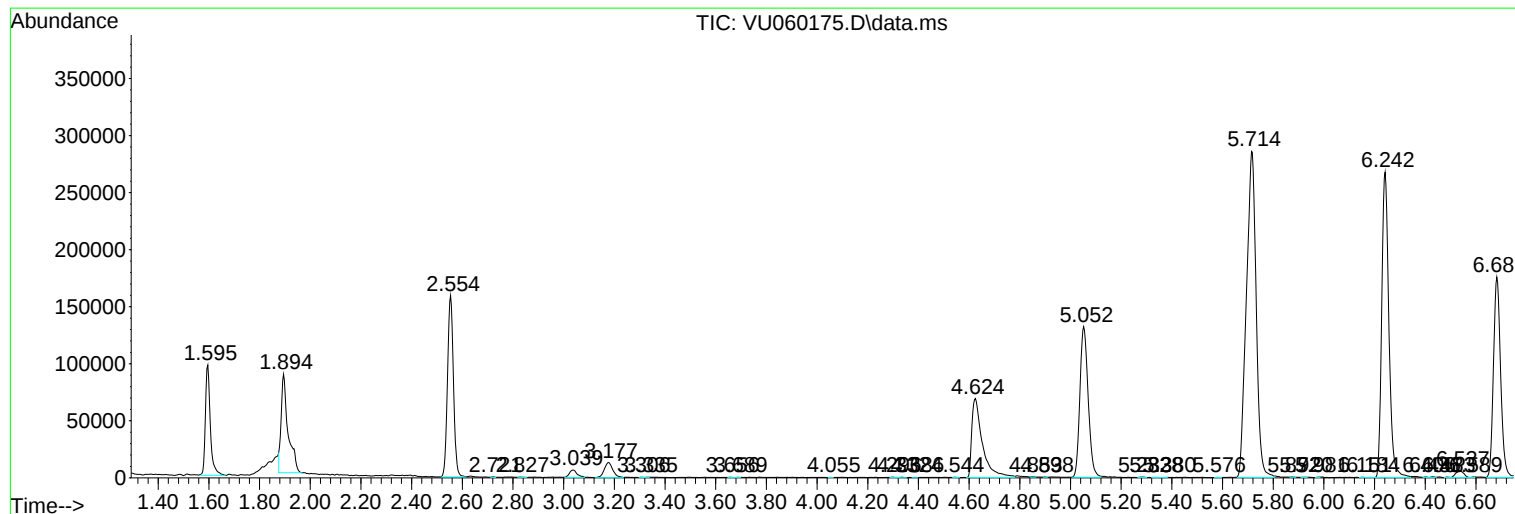

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060175.D
Acq On : 25 Jul 2024 16:43
Operator : MD/SY
Sample : P3260-09DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060175.D
Acq On : 25 Jul 2024 16:43
Operator : MD/SY
Sample : P3260-09DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------