

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060176.D
 Acq On : 25 Jul 2024 17:07
 Operator : MD/SY
 Sample : P3335-04 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	94743	111100	4.90%	1.446%
2	1.904	183	191	209	rVB	71225	98256	4.34%	1.279%
3	2.560	383	395	414	rBV	141987	230023	10.15%	2.994%
4	2.782	462	464	467	rBV2	430	253	0.01%	0.003%
5	2.930	507	510	514	rBV2	269	188	0.01%	0.002%
6	2.962	514	520	523	rBV2	279	379	0.02%	0.005%
7	2.997	527	531	534	rVV	462	378	0.02%	0.005%
8	3.039	534	544	556	rVB3	4040	7876	0.35%	0.103%
9	3.178	574	587	601	rBV2	8521	18923	0.84%	0.246%
10	3.354	640	642	643	rBV	216	68	0.00%	0.001%
11	3.637	727	730	734	rVB	323	216	0.01%	0.003%
12	3.663	734	738	741	rBV	269	269	0.01%	0.004%
13	3.772	770	772	776	rVB	189	153	0.01%	0.002%
14	3.814	780	785	794	rVB2	289	512	0.02%	0.007%
15	3.859	794	799	802	rBV	318	365	0.02%	0.005%
16	3.933	817	822	825	rBV2	204	204	0.01%	0.003%
17	4.023	848	850	853	rBV	103	61	0.00%	0.001%
18	4.042	853	856	860	rBV2	189	190	0.01%	0.002%
19	4.132	883	884	886	rBV2	97	55	0.00%	0.001%
20	4.255	919	922	927	rBV	235	239	0.01%	0.003%
21	4.277	927	929	930	rBV	108	62	0.00%	0.001%
22	4.457	982	985	987	rBV	234	192	0.01%	0.002%
23	4.499	992	998	1003	rBV	184	287	0.01%	0.004%
24	4.618	1023	1035	1072	rBV	67611	195629	8.63%	2.547%
25	4.927	1127	1131	1133	rBV3	258	244	0.01%	0.003%
26	5.055	1156	1171	1193	rBV	118287	265949	11.74%	3.462%
27	5.290	1242	1244	1246	rBV	155	43	0.00%	0.001%
28	5.306	1246	1249	1253	rBV2	173	166	0.01%	0.002%
29	5.361	1264	1266	1269	rBV	241	146	0.01%	0.002%
30	5.422	1283	1285	1287	rBV	114	79	0.00%	0.001%
31	5.467	1297	1299	1301	rBV2	178	101	0.00%	0.001%
32	5.509	1306	1312	1314	rBV2	266	229	0.01%	0.003%
33	5.615	1343	1345	1347	rBV	182	117	0.01%	0.002%
34	5.634	1348	1351	1353	rBV	231	141	0.01%	0.002%
35	5.718	1357	1377	1400	rBV2	245937	675093	29.79%	8.788%
36	5.891	1428	1431	1434	rBV3	263	252	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060176.D
 Acq On : 25 Jul 2024 17:07
 Operator : MD/SY
 Sample : P3335-04 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.994	1461	1463	1464	rBV3	106	58	0.00%	0.001%
38	6.052	1478	1481	1486	rBV2	278	259	0.01%	0.003%
39	6.181	1515	1521	1524	rBV2	222	281	0.01%	0.004%
40	6.242	1528	1540	1563	rBV	255514	496728	21.92%	6.466%
41	6.534	1616	1631	1657	rBV	1203882	2266122	100.00%	29.500%
42	6.682	1667	1677	1709	rVB	159954	317812	14.02%	4.137%
43	6.865	1731	1734	1735	rBV	336	146	0.01%	0.002%
44	6.943	1753	1758	1761	rVB2	310	333	0.01%	0.004%
45	6.962	1761	1764	1766	rBV2	165	116	0.01%	0.002%
46	7.020	1780	1782	1785	rBV2	323	197	0.01%	0.003%
47	7.055	1791	1793	1795	rBV	153	40	0.00%	0.001%
48	7.087	1799	1803	1810	rBV2	301	361	0.02%	0.005%
49	7.123	1810	1814	1817	rBV2	382	346	0.02%	0.005%
50	7.206	1832	1840	1843	rBV3	544	725	0.03%	0.009%
51	7.316	1869	1874	1876	rBV2	269	230	0.01%	0.003%
52	7.328	1876	1878	1879	rBV2	257	111	0.00%	0.001%
53	7.386	1889	1896	1900	rBV2	272	369	0.02%	0.005%
54	7.419	1902	1906	1909	rBV2	204	189	0.01%	0.002%
55	7.512	1932	1935	1937	rBV2	297	235	0.01%	0.003%
56	7.560	1939	1950	1971	rVV2	78110	140583	6.20%	1.830%
57	7.891	2042	2053	2080	rBV	282807	503792	22.23%	6.558%
58	8.174	2131	2141	2168	rBV2	50852	90431	3.99%	1.177%
59	8.312	2182	2184	2187	rBV2	205	106	0.00%	0.001%
60	8.370	2198	2202	2208	rVB3	383	401	0.02%	0.005%
61	8.441	2219	2224	2226	rBV	261	257	0.01%	0.003%
62	8.550	2249	2258	2268	rVB3	8555	13700	0.60%	0.178%
63	8.627	2272	2282	2322	rBV2	164902	335805	14.82%	4.371%
64	8.885	2359	2362	2365	rVB	458	266	0.01%	0.003%
65	8.939	2376	2379	2381	rBV2	348	180	0.01%	0.002%
66	9.033	2399	2408	2412	rBV2	233	412	0.02%	0.005%
67	9.052	2412	2414	2420	rVV2	425	312	0.01%	0.004%
68	9.078	2420	2422	2424	rBV2	181	63	0.00%	0.001%
69	9.142	2438	2442	2447	rBV2	258	312	0.01%	0.004%
70	9.312	2493	2495	2498	rBV	219	148	0.01%	0.002%
71	9.412	2513	2526	2555	rBV	370433	631948	27.89%	8.226%
72	9.644	2592	2598	2599	rBV2	337	296	0.01%	0.004%
73	9.692	2608	2613	2619	rBV3	386	460	0.02%	0.006%
74	9.901	2674	2678	2682	rBV	147	191	0.01%	0.002%
75	9.949	2691	2693	2697	rVB2	201	121	0.01%	0.002%
76	10.058	2721	2727	2729	rBV	346	351	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060176.D
 Acq On : 25 Jul 2024 17:07
 Operator : MD/SY
 Sample : P3335-04 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.139	2750	2752	2754	rBV2	155	74	0.00%	0.001%
78	10.267	2782	2792	2797	rBV2	323	531	0.02%	0.007%
79	10.290	2797	2799	2803	rVB2	234	174	0.01%	0.002%
80	10.309	2803	2805	2807	rBV	107	44	0.00%	0.001%
81	10.322	2807	2809	2814	rBV2	223	198	0.01%	0.003%
82	10.354	2817	2819	2821	rBV2	245	139	0.01%	0.002%
83	10.470	2853	2855	2856	rBV2	174	76	0.00%	0.001%
84	10.518	2868	2870	2874	rBV	206	115	0.01%	0.001%
85	10.608	2891	2898	2900	rBV2	247	299	0.01%	0.004%
86	10.708	2926	2929	2930	rBV	187	81	0.00%	0.001%
87	10.750	2930	2942	2962	rVV	223191	358459	15.82%	4.666%
88	10.852	2972	2974	2978	rBV	152	67	0.00%	0.001%
89	10.875	2979	2981	2983	rBV	391	263	0.01%	0.003%
90	10.962	3004	3008	3011	rBV2	352	368	0.02%	0.005%
91	10.997	3017	3019	3021	rBV2	239	136	0.01%	0.002%
92	11.197	3075	3081	3084	rBV2	280	324	0.01%	0.004%
93	11.245	3093	3096	3102	rBV	227	222	0.01%	0.003%
94	11.303	3109	3114	3116	rBV	220	203	0.01%	0.003%
95	11.354	3128	3130	3132	rBV	209	75	0.00%	0.001%
96	11.370	3132	3135	3137	rBV2	213	120	0.01%	0.002%
97	11.663	3223	3226	3232	rVB2	299	293	0.01%	0.004%
98	11.807	3260	3271	3297	rBV	309540	503260	22.21%	6.551%
99	12.190	3378	3390	3411	rBV	236539	402764	17.77%	5.243%
100	12.868	3596	3601	3603	rBV2	363	359	0.02%	0.005%




Sum of corrected areas: 7681875

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060176.D
Acq On : 25 Jul 2024 17:07
Operator : MD/SY
Sample : P3335-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

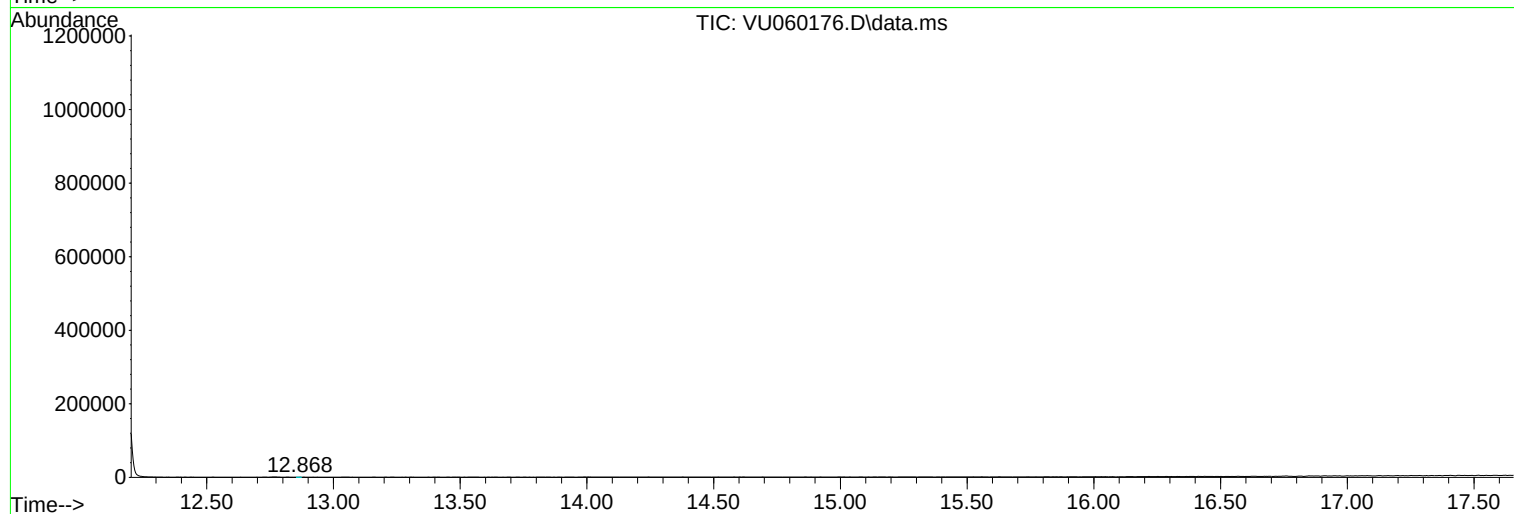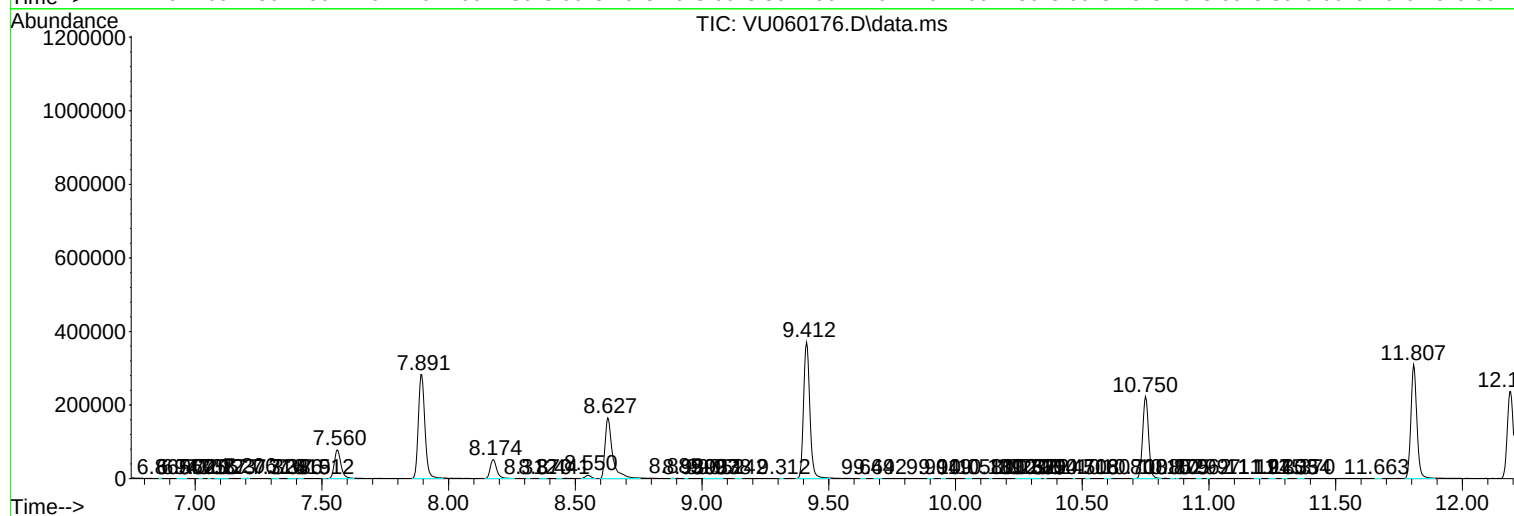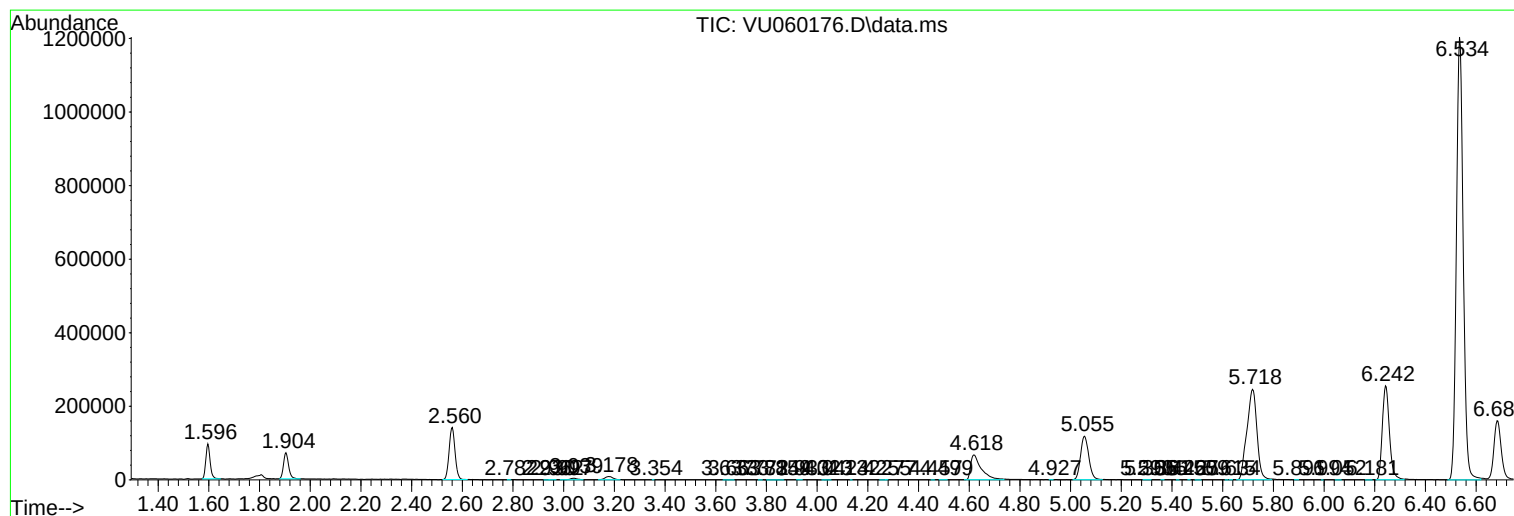

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060176.D
Acq On : 25 Jul 2024 17:07
Operator : MD/SY
Sample : P3335-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060176.D
Acq On : 25 Jul 2024 17:07
Operator : MD/SY
Sample : P3335-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------