

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060178.D
 Acq On : 25 Jul 2024 17:55
 Operator : MD/SY
 Sample : P3335-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	117	rBV	100210	120271	13.29%	1.831%
2	1.904	184	191	211	rVB	82094	118580	13.10%	1.805%
3	2.560	382	395	413	rBV	144708	236165	26.09%	3.595%
4	2.628	414	416	420	rVB3	481	351	0.04%	0.005%
5	2.779	459	463	465	rBV	519	333	0.04%	0.005%
6	2.795	465	468	471	rVB2	642	408	0.05%	0.006%
7	3.042	534	545	560	rVB2	4660	9487	1.05%	0.144%
8	3.177	575	587	602	rBV2	5537	12382	1.37%	0.189%
9	3.287	618	621	629	rBV2	155	187	0.02%	0.003%
10	3.345	634	639	640	rBV	321	255	0.03%	0.004%
11	3.747	761	764	768	rBV2	210	183	0.02%	0.003%
12	3.808	776	783	787	rBV2	396	539	0.06%	0.008%
13	4.190	897	902	907	rVB2	184	200	0.02%	0.003%
14	4.444	977	981	989	rBV2	266	370	0.04%	0.006%
15	4.486	992	994	999	rBV2	176	201	0.02%	0.003%
16	4.579	1017	1023	1025	rBV2	293	389	0.04%	0.006%
17	4.624	1025	1037	1083	rBV4	67416	247139	27.31%	3.762%
18	5.055	1156	1171	1197	rBV	125179	275747	30.47%	4.198%
19	5.229	1222	1225	1228	rVB3	293	197	0.02%	0.003%
20	5.264	1231	1236	1238	rBV2	408	413	0.05%	0.006%
21	5.335	1255	1258	1265	rVB	238	229	0.03%	0.003%
22	5.396	1274	1277	1282	rVB2	351	296	0.03%	0.005%
23	5.435	1286	1289	1293	rVV	290	203	0.02%	0.003%
24	5.470	1295	1300	1304	rBV2	210	225	0.02%	0.003%
25	5.560	1323	1328	1330	rBV	272	272	0.03%	0.004%
26	5.595	1335	1339	1342	rBV2	308	267	0.03%	0.004%
27	5.718	1357	1377	1411	rBV2	257679	702246	77.59%	10.691%
28	5.891	1427	1431	1433	rBV2	321	246	0.03%	0.004%
29	5.981	1454	1459	1464	rBV3	305	394	0.04%	0.006%
30	6.055	1480	1482	1485	rBV	304	180	0.02%	0.003%
31	6.139	1505	1508	1513	rBV2	259	299	0.03%	0.005%
32	6.242	1528	1540	1567	rVV	257461	503709	55.65%	7.668%
33	6.534	1618	1631	1665	rBV	475978	905090	100.00%	13.779%
34	6.685	1665	1678	1698	rVB	163704	321028	35.47%	4.887%
35	6.808	1714	1716	1720	rVV	434	335	0.04%	0.005%
36	6.885	1738	1740	1745	rBV	167	181	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060178.D
 Acq On : 25 Jul 2024 17:55
 Operator : MD/SY
 Sample : P3335-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.007	1774	1778	1783	rVB2	220	239	0.03%	0.004%
38	7.036	1783	1787	1790	rBV2	276	263	0.03%	0.004%
39	7.119	1810	1813	1817	rVB	249	202	0.02%	0.003%
40	7.216	1838	1843	1844	rBV	310	211	0.02%	0.003%
41	7.280	1859	1863	1867	rVB	334	339	0.04%	0.005%
42	7.309	1867	1872	1875	rBV2	253	250	0.03%	0.004%
43	7.422	1903	1907	1911	rVB2	257	266	0.03%	0.004%
44	7.447	1911	1915	1919	rBV2	230	245	0.03%	0.004%
45	7.505	1929	1933	1935	rBV2	210	179	0.02%	0.003%
46	7.560	1939	1950	1971	rBV	77851	141205	15.60%	2.150%
47	7.717	1995	1999	2007	rVB5	601	649	0.07%	0.010%
48	7.811	2025	2028	2032	rVB2	307	205	0.02%	0.003%
49	7.894	2040	2054	2073	rBV	293053	517641	57.19%	7.881%
50	8.177	2130	2142	2159	rBV	52773	93474	10.33%	1.423%
51	8.425	2216	2219	2227	rVB3	407	461	0.05%	0.007%
52	8.467	2227	2232	2236	rBV2	485	544	0.06%	0.008%
53	8.550	2247	2258	2272	rBV2	38145	64106	7.08%	0.976%
54	8.631	2272	2283	2315	rBV2	170601	350690	38.75%	5.339%
55	9.094	2423	2427	2432	rVB2	265	264	0.03%	0.004%
56	9.123	2432	2436	2442	rVB2	211	230	0.03%	0.004%
57	9.180	2451	2454	2458	rVV	245	191	0.02%	0.003%
58	9.312	2492	2495	2497	rBV2	255	196	0.02%	0.003%
59	9.412	2513	2526	2551	rBV	374776	639636	70.67%	9.738%
60	9.862	2663	2666	2672	rBV2	281	312	0.03%	0.005%
61	9.913	2679	2682	2686	rBV2	224	230	0.03%	0.004%
62	10.081	2731	2734	2738	rVB2	332	279	0.03%	0.004%
63	10.106	2738	2742	2745	rBV2	262	246	0.03%	0.004%
64	10.203	2768	2772	2775	rVB2	269	209	0.02%	0.003%
65	10.296	2797	2801	2803	rBV	266	208	0.02%	0.003%
66	10.425	2836	2841	2843	rBV2	324	311	0.03%	0.005%
67	10.457	2848	2851	2857	rBV2	253	340	0.04%	0.005%
68	10.512	2866	2868	2873	rVB2	227	216	0.02%	0.003%
69	10.544	2874	2878	2881	rBV2	348	301	0.03%	0.005%
70	10.569	2881	2886	2889	rVV2	337	370	0.04%	0.006%
71	10.598	2892	2895	2898	rVB2	242	183	0.02%	0.003%
72	10.749	2927	2942	2968	rBV	234329	378025	41.77%	5.755%
73	11.081	3042	3045	3047	rVV	282	206	0.02%	0.003%
74	11.113	3051	3055	3057	rBV2	299	232	0.03%	0.004%
75	11.293	3107	3111	3114	rBV2	332	269	0.03%	0.004%
76	11.360	3128	3132	3135	rBV	296	244	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060178.D
 Acq On : 25 Jul 2024 17:55
 Operator : MD/SY
 Sample : P3335-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.383	3135	3139	3141	rVV	292	182	0.02%	0.003%
78	11.441	3147	3157	3161	rVB	261	402	0.04%	0.006%
79	11.675	3228	3230	3237	rVB2	377	368	0.04%	0.006%
80	11.714	3237	3242	3246	rBV2	346	419	0.05%	0.006%
81	11.753	3252	3254	3256	rBV2	363	215	0.02%	0.003%
82	11.807	3259	3271	3295	rVV	302060	497621	54.98%	7.576%
83	12.187	3377	3389	3411	rBV	240200	411119	45.42%	6.259%
84	12.486	3479	3482	3485	rBV	382	212	0.02%	0.003%
85	12.714	3547	3553	3556	rVB	373	428	0.05%	0.007%
86	12.743	3556	3562	3563	rBV2	318	332	0.04%	0.005%
87	13.026	3645	3650	3655	rBV	277	351	0.04%	0.005%
88	13.280	3726	3729	3731	rBV	256	187	0.02%	0.003%
89	13.987	3946	3949	3951	rBV2	350	243	0.03%	0.004%
90	14.074	3972	3976	3979	rBV2	499	420	0.05%	0.006%
91	14.145	3994	3998	3999	rBV2	266	195	0.02%	0.003%
92	14.206	4011	4017	4022	rBV2	501	635	0.07%	0.010%
93	14.392	4072	4075	4076	rBV	401	220	0.02%	0.003%
94	14.457	4093	4095	4098	rVB2	396	183	0.02%	0.003%
95	14.479	4099	4102	4108	rVB2	418	456	0.05%	0.007%
96	14.511	4108	4112	4113	rBV2	446	316	0.03%	0.005%
97	14.791	4196	4199	4201	rBV2	415	258	0.03%	0.004%
98	15.138	4303	4307	4310	rBV2	349	308	0.03%	0.005%
99	15.386	4382	4384	4387	rBV2	420	250	0.03%	0.004%
100	15.518	4422	4425	4427	rBV3	521	364	0.04%	0.006%




Sum of corrected areas: 6568548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060178.D
Acq On : 25 Jul 2024 17:55
Operator : MD/SY
Sample : P3335-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

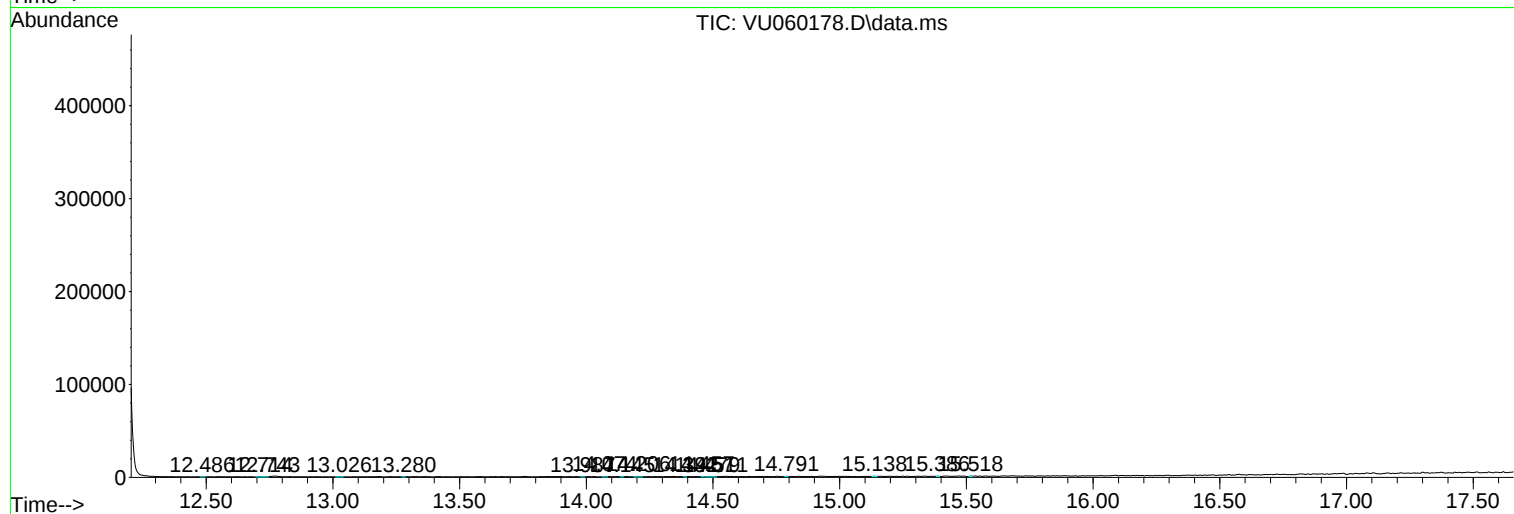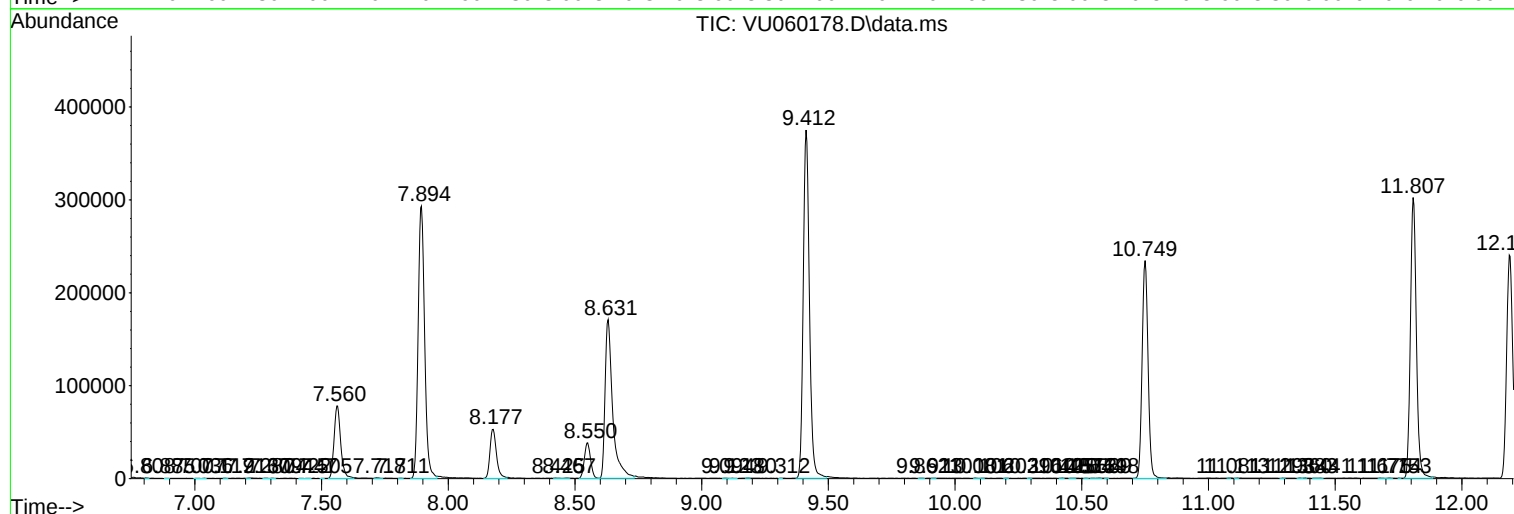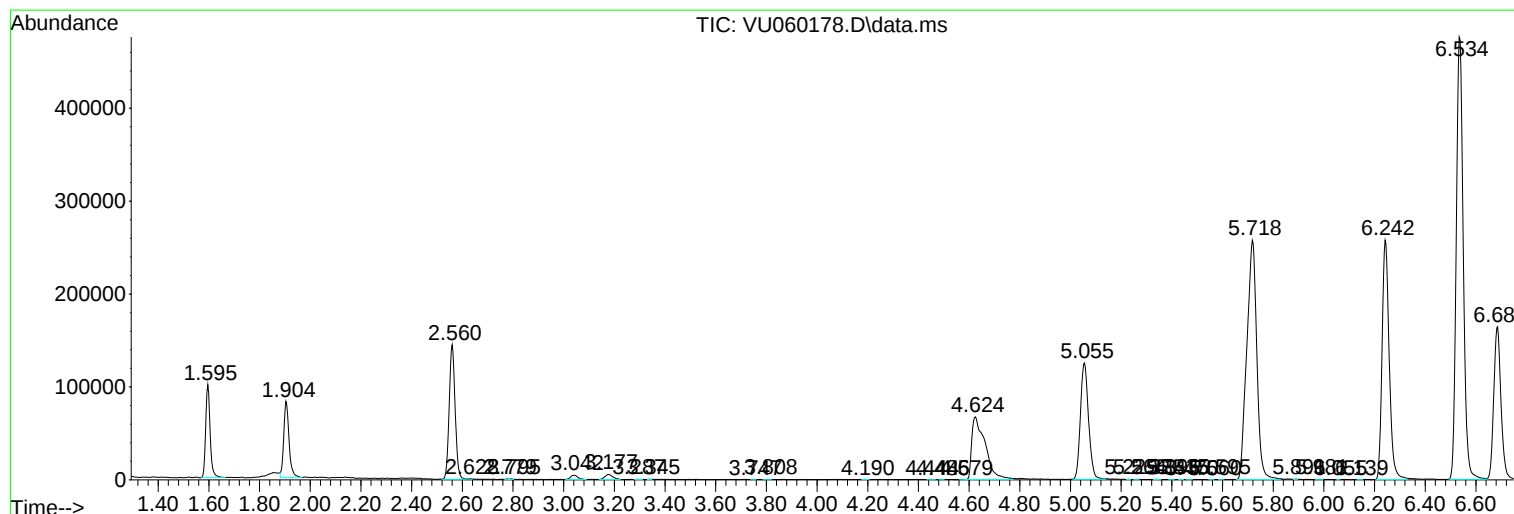

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060178.D
Acq On : 25 Jul 2024 17:55
Operator : MD/SY
Sample : P3335-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060178.D
Acq On : 25 Jul 2024 17:55
Operator : MD/SY
Sample : P3335-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------