

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060179.D
 Acq On : 25 Jul 2024 18:19
 Operator : MD/SY
 Sample : P3335-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rBV	96458	114359	16.91%	2.061%
2	1.727	131	136	143	rVB	5953	6338	0.94%	0.114%
3	1.904	184	191	208	rVB	74715	105835	15.65%	1.907%
4	2.197	279	282	285	rVB3	824	498	0.07%	0.009%
5	2.213	285	287	290	rVV2	548	322	0.05%	0.006%
6	2.229	290	292	295	rVB2	598	251	0.04%	0.005%
7	2.560	382	395	410	rBV	137590	224176	33.15%	4.039%
8	2.637	411	419	429	rVB2	3541	6052	0.89%	0.109%
9	2.727	441	447	450	rBV2	447	493	0.07%	0.009%
10	3.039	536	544	554	rBV3	2128	4161	0.62%	0.075%
11	3.181	575	588	596	rBV2	4194	9124	1.35%	0.164%
12	3.232	601	604	609	rVB	497	475	0.07%	0.009%
13	3.264	609	614	618	rBV2	201	264	0.04%	0.005%
14	3.351	629	641	656	rBV3	14134	29035	4.29%	0.523%
15	3.470	674	678	683	rVB	302	311	0.05%	0.006%
16	3.499	683	687	692	rBV	261	328	0.05%	0.006%
17	3.888	799	808	810	rBV2	217	320	0.05%	0.006%
18	3.969	829	833	837	rBV2	237	250	0.04%	0.005%
19	4.020	845	849	856	rBV2	298	464	0.07%	0.008%
20	4.071	861	865	870	rVB2	280	250	0.04%	0.005%
21	4.155	887	891	894	rBV2	342	302	0.04%	0.005%
22	4.245	914	919	923	rVB	291	236	0.03%	0.004%
23	4.268	923	926	930	rBV2	298	233	0.03%	0.004%
24	4.338	944	948	953	rVB2	239	274	0.04%	0.005%
25	4.367	953	957	959	rBV	265	240	0.04%	0.004%
26	4.473	986	990	992	rBV	343	264	0.04%	0.005%
27	4.621	1025	1036	1068	rBV	74459	217127	32.10%	3.912%
28	5.055	1154	1171	1194	rBV	119363	262071	38.75%	4.722%
29	5.306	1245	1249	1259	rVV2	381	395	0.06%	0.007%
30	5.358	1259	1265	1273	rVB2	291	457	0.07%	0.008%
31	5.403	1273	1279	1282	rBV2	461	455	0.07%	0.008%
32	5.419	1282	1284	1288	rVV2	293	254	0.04%	0.005%
33	5.473	1298	1301	1309	rBV2	190	258	0.04%	0.005%
34	5.615	1338	1345	1348	rBV2	217	282	0.04%	0.005%
35	5.718	1356	1377	1410	rBV2	243775	676324	100.00%	12.186%
36	5.891	1429	1431	1439	rVB3	299	282	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060179.D
 Acq On : 25 Jul 2024 18:19
 Operator : MD/SY
 Sample : P3335-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.923	1439	1441	1445	rVB3	492	382	0.06%	0.007%
38	6.017	1467	1470	1475	rBV3	395	410	0.06%	0.007%
39	6.081	1486	1490	1494	rVB2	338	304	0.04%	0.005%
40	6.120	1494	1502	1508	rBV2	270	489	0.07%	0.009%
41	6.177	1515	1520	1526	rVB2	381	498	0.07%	0.009%
42	6.242	1527	1540	1561	rBV	261294	506966	74.96%	9.135%
43	6.538	1620	1632	1650	rBV6	21054	41774	6.18%	0.753%
44	6.682	1664	1677	1696	rBV2	152204	301128	44.52%	5.426%
45	6.991	1768	1773	1779	rVB2	379	529	0.08%	0.010%
46	7.058	1790	1794	1800	rVV2	264	394	0.06%	0.007%
47	7.094	1801	1805	1813	rVB	192	236	0.03%	0.004%
48	7.206	1834	1840	1842	rBV2	424	415	0.06%	0.007%
49	7.274	1857	1861	1863	rBV2	355	317	0.05%	0.006%
50	7.357	1883	1887	1892	rBV	209	253	0.04%	0.005%
51	7.560	1939	1950	1971	rBV2	71594	131788	19.49%	2.375%
52	7.714	1994	1998	2005	rVB4	438	516	0.08%	0.009%
53	7.795	2014	2023	2026	rBV4	1502	1743	0.26%	0.031%
54	7.891	2041	2053	2073	rBV	267138	474808	70.20%	8.555%
55	8.100	2115	2118	2122	rVB2	469	347	0.05%	0.006%
56	8.174	2131	2141	2162	rVV2	48865	86475	12.79%	1.558%
57	8.377	2198	2204	2207	rBV2	258	240	0.04%	0.004%
58	8.470	2223	2233	2235	rBV3	2113	2415	0.36%	0.044%
59	8.550	2249	2258	2265	rBV5	1852	3093	0.46%	0.056%
60	8.631	2272	2283	2314	rBV2	207209	421866	62.38%	7.601%
61	9.303	2486	2492	2495	rBV2	200	234	0.03%	0.004%
62	9.412	2514	2526	2553	rBV	380691	645755	95.48%	11.635%
63	9.570	2567	2575	2579	rBV4	1754	2076	0.31%	0.037%
64	9.698	2608	2615	2628	rVV4	1656	2960	0.44%	0.053%
65	10.103	2732	2741	2742	rBV2	986	1082	0.16%	0.019%
66	10.232	2776	2781	2785	rBV	307	300	0.04%	0.005%
67	10.418	2833	2839	2845	rBV2	360	441	0.07%	0.008%
68	10.463	2847	2853	2855	rBV2	256	293	0.04%	0.005%
69	10.518	2865	2870	2875	rVV2	191	261	0.04%	0.005%
70	10.705	2922	2928	2930	rBV2	320	308	0.05%	0.006%
71	10.750	2930	2942	2961	rVV	222383	360252	53.27%	6.491%
72	10.888	2977	2985	2993	rVB2	1826	2671	0.39%	0.048%
73	11.110	3050	3054	3060	rBV3	388	458	0.07%	0.008%
74	11.235	3090	3093	3100	rBV	330	317	0.05%	0.006%
75	11.695	3230	3236	3240	rBV2	347	488	0.07%	0.009%
76	11.807	3259	3271	3293	rVV	299694	491747	72.71%	8.860%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060179.D
 Acq On : 25 Jul 2024 18:19
 Operator : MD/SY
 Sample : P3335-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.068	3346	3352	3363	rBV6	2362	4812	0.71%	0.087%
78	12.187	3377	3389	3416	rBV	231254	385149	56.95%	6.940%
79	12.470	3474	3477	3481	rBV	282	302	0.04%	0.005%
80	12.688	3538	3545	3548	rBV2	344	428	0.06%	0.008%
81	12.733	3554	3559	3562	rBV2	310	328	0.05%	0.006%
82	12.769	3564	3570	3576	rVB4	960	1347	0.20%	0.024%
83	12.949	3620	3626	3632	rVB2	707	815	0.12%	0.015%
84	13.151	3685	3689	3693	rBV3	353	415	0.06%	0.007%
85	13.290	3728	3732	3734	rBV	319	245	0.04%	0.004%
86	13.505	3794	3799	3802	rVB2	432	340	0.05%	0.006%
87	13.528	3802	3806	3809	rBV2	339	340	0.05%	0.006%
88	13.643	3839	3842	3847	rVB2	332	245	0.04%	0.004%
89	13.679	3847	3853	3858	rBV2	384	534	0.08%	0.010%
90	13.872	3909	3913	3917	rBV	338	338	0.05%	0.006%
91	14.241	4023	4028	4033	rBV	329	471	0.07%	0.008%
92	14.473	4097	4100	4107	rVB2	486	635	0.09%	0.011%
93	14.512	4109	4112	4116	rBV	436	416	0.06%	0.007%
94	14.534	4117	4119	4125	rVV3	313	262	0.04%	0.005%
95	15.200	4323	4326	4331	rVB2	467	371	0.05%	0.007%
96	15.740	4491	4494	4496	rBV2	499	316	0.05%	0.006%
97	15.849	4526	4528	4532	rBV4	803	635	0.09%	0.011%
98	16.331	4676	4678	4681	rBV3	787	425	0.06%	0.008%
99	16.347	4681	4683	4686	rVV3	690	335	0.05%	0.006%
100	16.402	4697	4700	4701	rBV3	990	592	0.09%	0.011%




Sum of corrected areas: 5549885

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060179.D
Acq On : 25 Jul 2024 18:19
Operator : MD/SY
Sample : P3335-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

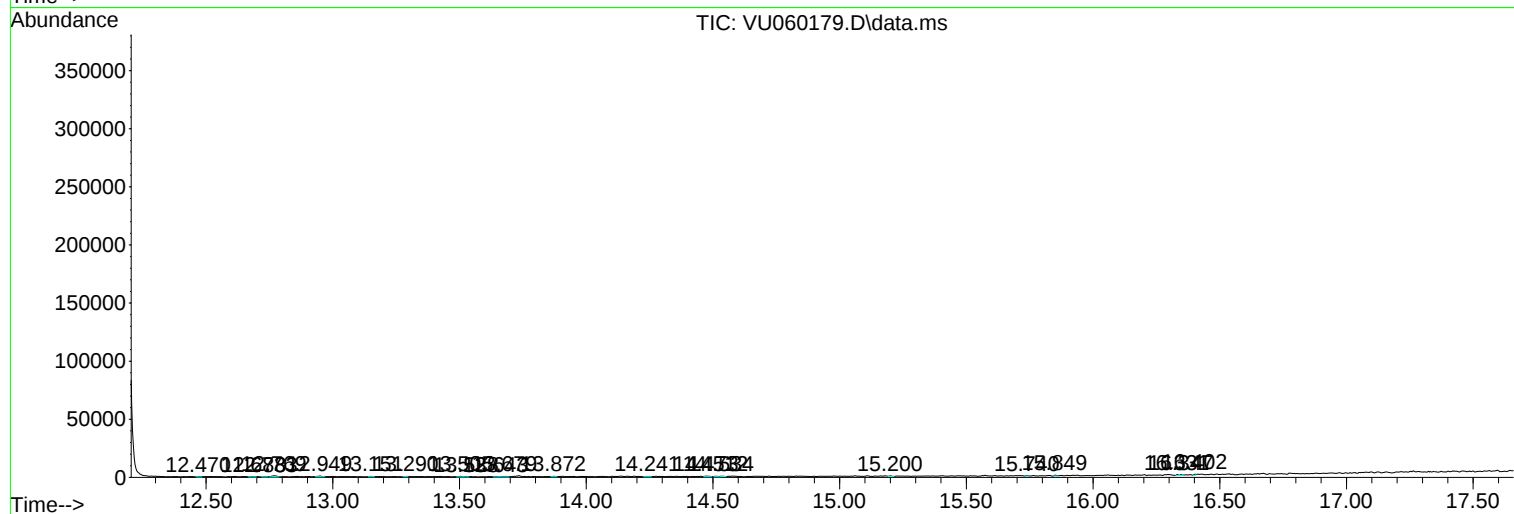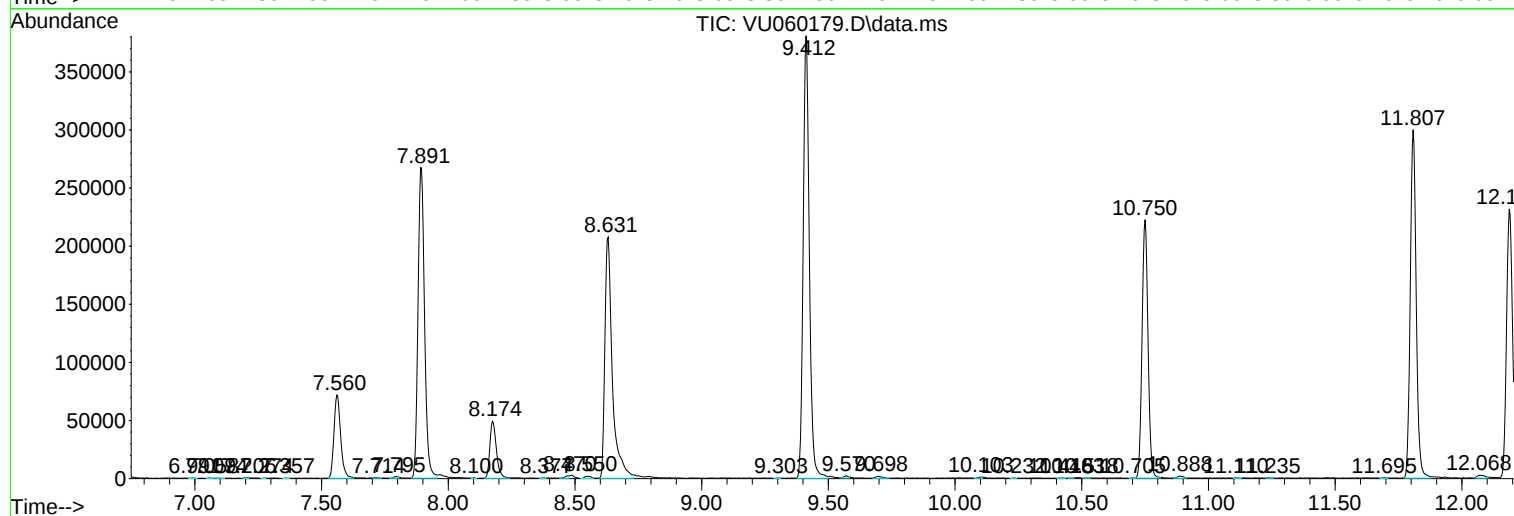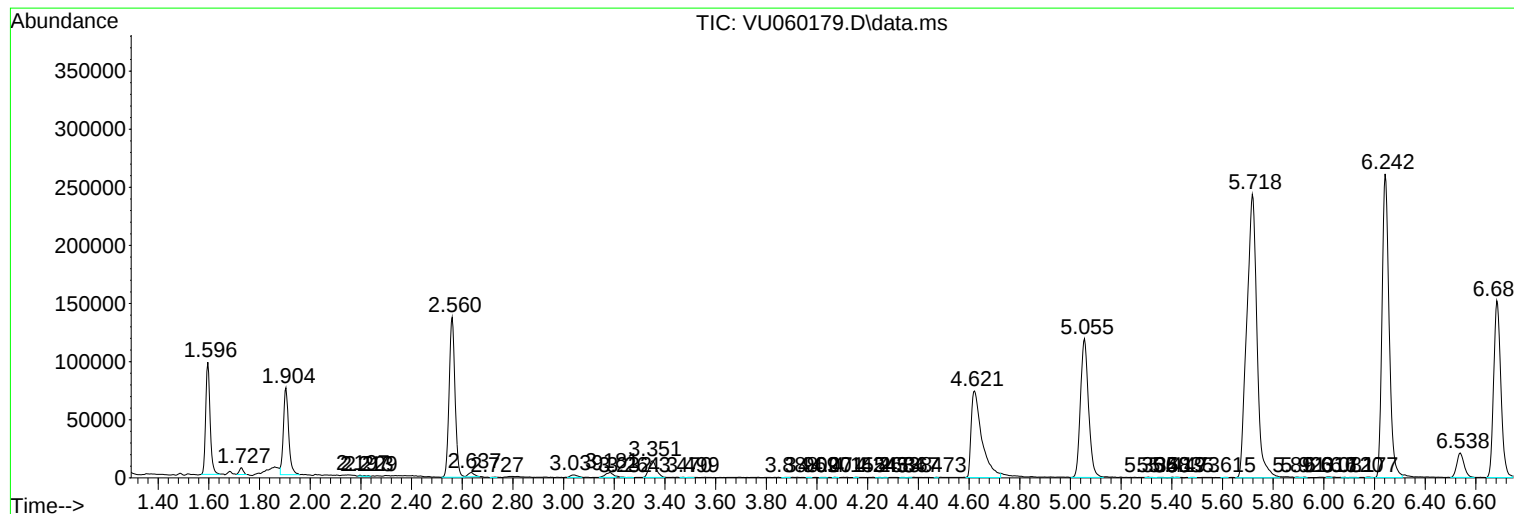

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060179.D
Acq On : 25 Jul 2024 18:19
Operator : MD/SY
Sample : P3335-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060179.D
Acq On : 25 Jul 2024 18:19
Operator : MD/SY
Sample : P3335-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------