

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060180.D
 Acq On : 25 Jul 2024 18:43
 Operator : MD/SY
 Sample : P3335-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rBV	96425	114223	16.60%	2.046%
2	1.682	117	122	128	rBV	3359	4294	0.62%	0.077%
3	1.727	130	136	146	rVB	17450	21507	3.13%	0.385%
4	1.904	184	191	213	rVB	73224	103942	15.11%	1.862%
5	2.560	384	395	408	rBV	137137	223972	32.56%	4.012%
6	2.628	411	416	431	rVB3	5465	9024	1.31%	0.162%
7	2.792	451	467	474	rBV3	4454	10628	1.54%	0.190%
8	2.911	501	504	508	rBV4	255	260	0.04%	0.005%
9	2.959	512	519	521	rBV	357	429	0.06%	0.008%
10	3.039	536	544	558	rBV3	2473	4914	0.71%	0.088%
11	3.177	573	587	604	rBV2	7186	16898	2.46%	0.303%
12	3.293	617	623	627	rBV2	319	283	0.04%	0.005%
13	3.351	630	641	660	rBV2	15665	30967	4.50%	0.555%
14	3.676	738	742	746	rBV2	260	268	0.04%	0.005%
15	4.197	897	904	906	rBV	198	264	0.04%	0.005%
16	4.444	977	981	984	rBV2	252	240	0.03%	0.004%
17	4.538	1007	1010	1015	rVB2	264	263	0.04%	0.005%
18	4.621	1023	1036	1073	rBV	74952	222928	32.40%	3.993%
19	5.055	1155	1171	1195	rBV2	118519	264868	38.50%	4.744%
20	5.184	1208	1211	1213	rBV2	294	218	0.03%	0.004%
21	5.325	1249	1255	1260	rVB3	239	334	0.05%	0.006%
22	5.470	1297	1300	1304	rVB	348	290	0.04%	0.005%
23	5.502	1304	1310	1312	rBV2	281	291	0.04%	0.005%
24	5.570	1329	1331	1339	rVB2	243	261	0.04%	0.005%
25	5.621	1342	1347	1353	rBV	276	229	0.03%	0.004%
26	5.718	1358	1377	1415	rBV2	246525	687954	100.00%	12.323%
27	6.020	1465	1471	1478	rVV3	695	870	0.13%	0.016%
28	6.058	1480	1483	1489	rVB2	354	395	0.06%	0.007%
29	6.107	1495	1498	1504	rVB2	393	377	0.05%	0.007%
30	6.242	1527	1540	1565	rBV	248480	485280	70.54%	8.693%
31	6.441	1597	1602	1607	rBV3	353	340	0.05%	0.006%
32	6.496	1613	1619	1622	rBV3	447	594	0.09%	0.011%
33	6.537	1622	1632	1648	rVV5	15393	31666	4.60%	0.567%
34	6.682	1663	1677	1706	rBV	154261	309789	45.03%	5.549%
35	6.910	1745	1748	1752	rBV	401	290	0.04%	0.005%
36	6.994	1769	1774	1777	rBV	257	268	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060180.D
 Acq On : 25 Jul 2024 18:43
 Operator : MD/SY
 Sample : P3335-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.171	1826	1829	1832	rVV	296	207	0.03%	0.004%
38	7.209	1839	1841	1849	rVB2	558	626	0.09%	0.011%
39	7.502	1928	1932	1934	rBV	304	249	0.04%	0.004%
40	7.563	1938	1951	1971	rBV	71632	132517	19.26%	2.374%
41	7.705	1990	1995	1996	rBV	296	224	0.03%	0.004%
42	7.801	2013	2025	2037	rBV5	1764	3248	0.47%	0.058%
43	7.894	2040	2054	2077	rBV	269754	484294	70.40%	8.675%
44	8.074	2108	2110	2115	rVB2	430	330	0.05%	0.006%
45	8.103	2115	2119	2121	rBV2	414	257	0.04%	0.005%
46	8.174	2131	2141	2163	rBV	49636	87071	12.66%	1.560%
47	8.251	2163	2165	2168	rVV3	416	287	0.04%	0.005%
48	8.280	2171	2174	2178	rVB	476	412	0.06%	0.007%
49	8.470	2220	2233	2248	rBV5	3357	7441	1.08%	0.133%
50	8.547	2252	2257	2264	rVB5	1309	1789	0.26%	0.032%
51	8.631	2270	2283	2315	rBV2	205453	425499	61.85%	7.622%
52	8.907	2367	2369	2375	rBV2	270	311	0.05%	0.006%
53	9.007	2394	2400	2402	rVB2	295	288	0.04%	0.005%
54	9.029	2403	2407	2414	rBV2	197	265	0.04%	0.005%
55	9.232	2467	2470	2477	rVB2	257	264	0.04%	0.005%
56	9.325	2496	2499	2507	rBV2	245	269	0.04%	0.005%
57	9.412	2512	2526	2558	rBV	360584	619833	90.10%	11.103%
58	9.569	2567	2575	2582	rVV4	2104	2733	0.40%	0.049%
59	9.602	2582	2585	2592	rVB2	608	672	0.10%	0.012%
60	9.701	2607	2616	2626	rVB6	1715	3101	0.45%	0.056%
61	9.775	2634	2639	2643	rVB2	231	214	0.03%	0.004%
62	9.820	2648	2653	2656	rBV	230	215	0.03%	0.004%
63	10.100	2735	2740	2750	rVB4	1095	1613	0.23%	0.029%
64	10.235	2778	2782	2785	rBV2	326	329	0.05%	0.006%
65	10.331	2806	2812	2816	rVV2	360	328	0.05%	0.006%
66	10.479	2849	2858	2861	rBV2	640	612	0.09%	0.011%
67	10.515	2866	2869	2872	rBV2	280	230	0.03%	0.004%
68	10.631	2902	2905	2909	rVB2	374	317	0.05%	0.006%
69	10.656	2909	2913	2917	rVB	314	256	0.04%	0.005%
70	10.749	2929	2942	2961	rBV	226270	370320	53.83%	6.633%
71	10.852	2968	2974	2976	rBV2	313	293	0.04%	0.005%
72	10.888	2976	2985	2995	rVB4	3998	6133	0.89%	0.110%
73	10.978	3010	3013	3016	rVB2	279	220	0.03%	0.004%
74	11.032	3024	3030	3036	rVB2	260	337	0.05%	0.006%
75	11.190	3075	3079	3082	rBV	267	243	0.04%	0.004%
76	11.303	3110	3114	3118	rVB2	231	237	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060180.D
 Acq On : 25 Jul 2024 18:43
 Operator : MD/SY
 Sample : P3335-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.331	3118	3123	3129	rVB2	317	389	0.06%	0.007%
78	11.367	3130	3134	3138	rBV2	318	349	0.05%	0.006%
79	11.425	3148	3152	3155	rBV	278	255	0.04%	0.005%
80	11.550	3188	3191	3193	rBV2	278	218	0.03%	0.004%
81	11.592	3199	3204	3208	rBV2	236	257	0.04%	0.005%
82	11.717	3238	3243	3248	rBV2	650	884	0.13%	0.016%
83	11.756	3253	3255	3259	rVB	386	216	0.03%	0.004%
84	11.807	3259	3271	3295	rBV	288179	476482	69.26%	8.535%
85	12.071	3342	3353	3368	rBV6	3048	7823	1.14%	0.140%
86	12.190	3378	3390	3407	rBV	230405	384648	55.91%	6.890%
87	12.354	3438	3441	3445	rVB3	321	243	0.04%	0.004%
88	12.765	3561	3569	3576	rBV	1682	2342	0.34%	0.042%
89	12.846	3591	3594	3597	rBV	280	247	0.04%	0.004%
90	13.302	3732	3736	3739	rBV2	365	306	0.04%	0.005%
91	13.524	3801	3805	3809	rBV2	503	337	0.05%	0.006%
92	13.868	3909	3912	3919	rBV2	420	461	0.07%	0.008%
93	14.566	4126	4129	4135	rBV2	566	750	0.11%	0.013%
94	14.711	4171	4174	4177	rBV2	409	286	0.04%	0.005%
95	15.032	4272	4274	4279	rBV2	399	465	0.07%	0.008%
96	15.232	4332	4336	4338	rBV2	447	378	0.05%	0.007%
97	15.396	4384	4387	4391	rBV2	616	423	0.06%	0.008%
98	15.415	4391	4393	4395	rBV2	496	245	0.04%	0.004%
99	15.563	4435	4439	4446	rVB3	636	698	0.10%	0.013%
100	16.373	4689	4691	4692	rBV	638	309	0.04%	0.006%




Sum of corrected areas: 5582713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060180.D
Acq On : 25 Jul 2024 18:43
Operator : MD/SY
Sample : P3335-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

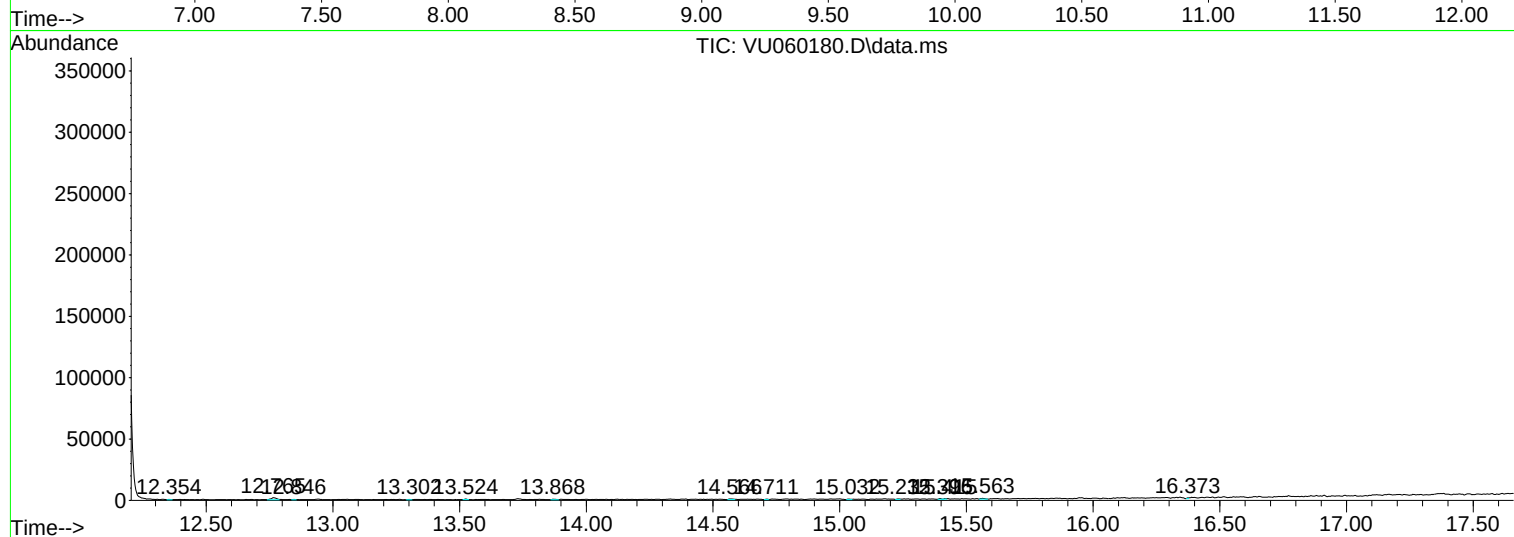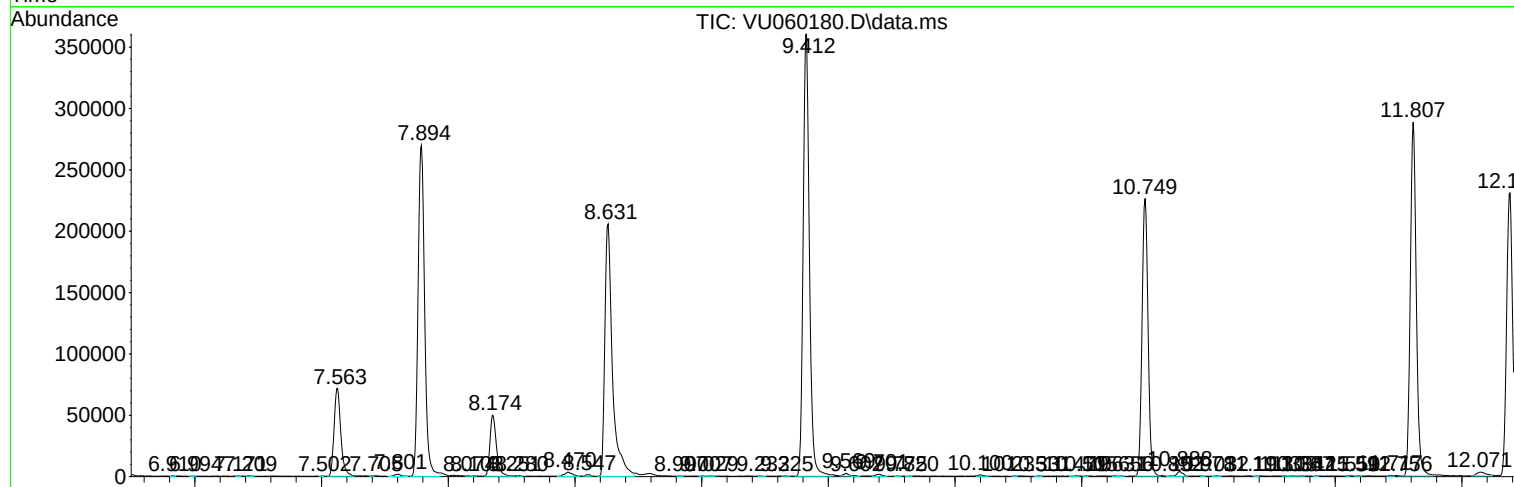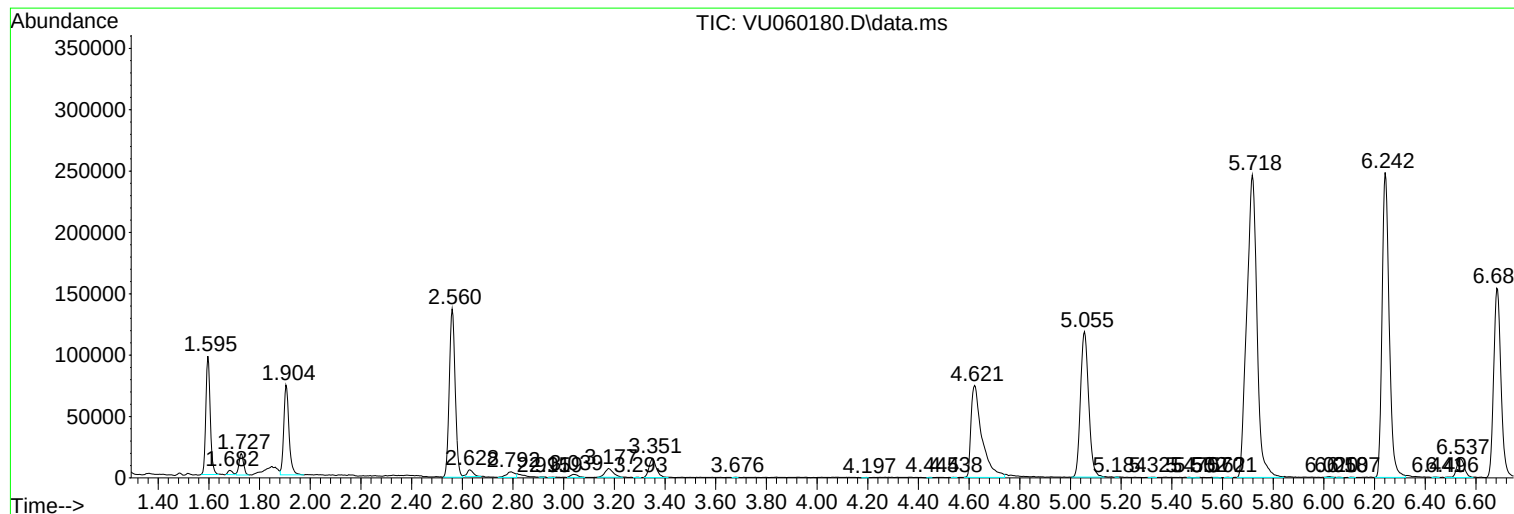

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060180.D
Acq On : 25 Jul 2024 18:43
Operator : MD/SY
Sample : P3335-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060180.D
Acq On : 25 Jul 2024 18:43
Operator : MD/SY
Sample : P3335-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------