

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060181.D
 Acq On : 25 Jul 2024 19:07
 Operator : MD/SY
 Sample : P3335-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	16	21	32	rVB3	7395	7909	1.19%	0.151%
2	1.595	87	95	109	rVB	98650	115857	17.42%	2.208%
3	1.682	117	122	131	rVB	5720	6349	0.95%	0.121%
4	1.904	184	191	209	rVB	72427	102878	15.47%	1.961%
5	2.560	382	395	408	rBV	137222	223094	33.55%	4.252%
6	2.628	408	416	433	rVB	8918	17147	2.58%	0.327%
7	2.788	452	466	488	rBV3	4739	16781	2.52%	0.320%
8	2.914	502	505	508	rVB2	342	240	0.04%	0.005%
9	2.955	515	518	525	rVB3	437	482	0.07%	0.009%
10	3.039	535	544	559	rVB6	2775	5860	0.88%	0.112%
11	3.177	577	587	602	rVB2	3431	7872	1.18%	0.150%
12	3.345	632	639	640	rBV2	1114	974	0.15%	0.019%
13	3.390	649	653	657	rVB2	292	277	0.04%	0.005%
14	3.531	688	697	699	rBV2	353	422	0.06%	0.008%
15	3.576	707	711	714	rBV3	491	368	0.06%	0.007%
16	3.923	813	819	828	rVB2	179	375	0.06%	0.007%
17	4.129	878	883	885	rBV2	249	246	0.04%	0.005%
18	4.177	891	898	902	rBV2	205	284	0.04%	0.005%
19	4.271	921	927	931	rVV2	199	228	0.03%	0.004%
20	4.457	978	985	987	rBV2	291	342	0.05%	0.007%
21	4.621	1026	1036	1068	rBV	61058	169824	25.54%	3.237%
22	5.055	1155	1171	1197	rBV	118213	264456	39.77%	5.040%
23	5.168	1203	1206	1211	rBV4	297	228	0.03%	0.004%
24	5.242	1227	1229	1233	rVB2	396	262	0.04%	0.005%
25	5.306	1246	1249	1253	rVV	320	234	0.04%	0.004%
26	5.332	1253	1257	1264	rVV2	232	273	0.04%	0.005%
27	5.576	1328	1333	1340	rBV2	461	608	0.09%	0.012%
28	5.618	1340	1346	1349	rBV2	243	236	0.04%	0.004%
29	5.717	1358	1377	1406	rBV2	242229	664949	100.00%	12.673%
30	5.978	1454	1458	1460	rBV2	380	283	0.04%	0.005%
31	6.113	1495	1500	1504	rBV2	235	242	0.04%	0.005%
32	6.242	1527	1540	1571	rBV	247368	488794	73.51%	9.316%
33	6.541	1619	1633	1645	rVV5	14918	29591	4.45%	0.564%
34	6.682	1662	1677	1712	rBV	153527	306352	46.07%	5.839%
35	6.807	1712	1716	1722	rVB3	549	479	0.07%	0.009%
36	6.862	1728	1733	1736	rBV2	235	216	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060181.D
 Acq On : 25 Jul 2024 19:07
 Operator : MD/SY
 Sample : P3335-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.910	1743	1748	1750	rBV	312	267	0.04%	0.005%
38	7.164	1823	1827	1829	rBV2	314	221	0.03%	0.004%
39	7.184	1829	1833	1834	rBV2	460	284	0.04%	0.005%
40	7.209	1838	1841	1845	rVB3	424	326	0.05%	0.006%
41	7.560	1939	1950	1971	rVV	71327	128716	19.36%	2.453%
42	7.708	1993	1996	1998	rBV2	353	251	0.04%	0.005%
43	7.785	2015	2020	2022	rBV2	290	304	0.05%	0.006%
44	7.798	2022	2024	2028	rVB3	356	237	0.04%	0.005%
45	7.891	2041	2053	2072	rBV	263408	466651	70.18%	8.894%
46	8.074	2106	2110	2116	rBV3	340	381	0.06%	0.007%
47	8.116	2121	2123	2127	rVB2	396	236	0.04%	0.004%
48	8.177	2128	2142	2158	rBV	48516	85682	12.89%	1.633%
49	8.415	2214	2216	2223	rVB2	269	244	0.04%	0.005%
50	8.467	2224	2232	2242	rVV2	1118	1682	0.25%	0.032%
51	8.540	2251	2255	2256	rBV2	1049	573	0.09%	0.011%
52	8.630	2272	2283	2322	rBV3	157489	330771	49.74%	6.304%
53	9.232	2466	2470	2473	rBV2	208	247	0.04%	0.005%
54	9.338	2498	2503	2506	rBV	245	254	0.04%	0.005%
55	9.412	2513	2526	2552	rBV	351628	597678	89.88%	11.391%
56	9.701	2608	2616	2624	rBV2	534	987	0.15%	0.019%
57	9.756	2628	2633	2637	rVB2	328	319	0.05%	0.006%
58	10.097	2736	2739	2741	rBV2	298	225	0.03%	0.004%
59	10.229	2777	2780	2786	rVB	260	235	0.04%	0.004%
60	10.470	2852	2855	2858	rVV2	258	207	0.03%	0.004%
61	10.534	2872	2875	2879	rVB2	276	230	0.03%	0.004%
62	10.611	2892	2899	2905	rBV2	354	620	0.09%	0.012%
63	10.749	2928	2942	2963	rBV	222543	358411	53.90%	6.831%
64	10.888	2979	2985	2995	rBV3	1416	1920	0.29%	0.037%
65	11.055	3034	3037	3040	rBV	388	276	0.04%	0.005%
66	11.081	3040	3045	3050	rVV2	205	263	0.04%	0.005%
67	11.209	3080	3085	3087	rBV2	296	284	0.04%	0.005%
68	11.238	3090	3094	3097	rBV	273	216	0.03%	0.004%
69	11.486	3166	3171	3172	rBV2	237	223	0.03%	0.004%
70	11.608	3205	3209	3213	rVB2	321	317	0.05%	0.006%
71	11.740	3244	3250	3254	rBV	405	511	0.08%	0.010%
72	11.807	3259	3271	3296	rBV	277401	452179	68.00%	8.618%
73	12.036	3338	3342	3347	rBV2	284	278	0.04%	0.005%
74	12.087	3355	3358	3365	rBV4	577	549	0.08%	0.010%
75	12.187	3373	3389	3413	rBV	217477	368945	55.48%	7.032%
76	12.318	3427	3430	3433	rBV2	432	348	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060181.D
 Acq On : 25 Jul 2024 19:07
 Operator : MD/SY
 Sample : P3335-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.351	3436	3440	3445	rVB2	360	326	0.05%	0.006%
78	12.431	3461	3465	3467	rBV2	409	367	0.06%	0.007%
79	12.470	3473	3477	3480	rBV	446	335	0.05%	0.006%
80	12.511	3485	3490	3495	rBV	399	466	0.07%	0.009%
81	12.765	3562	3569	3572	rBV2	1252	1627	0.24%	0.031%
82	12.804	3578	3581	3583	rBV2	319	244	0.04%	0.005%
83	13.154	3687	3690	3697	rBV	395	309	0.05%	0.006%
84	13.646	3839	3843	3848	rBV2	423	377	0.06%	0.007%
85	13.833	3898	3901	3905	rBV	305	277	0.04%	0.005%
86	13.884	3914	3917	3920	rVB2	447	268	0.04%	0.005%
87	13.904	3920	3923	3927	rBV	271	228	0.03%	0.004%
88	13.984	3945	3948	3951	rBV	374	295	0.04%	0.006%
89	14.013	3955	3957	3964	rVV2	351	333	0.05%	0.006%
90	14.453	4092	4094	4098	rBV	410	227	0.03%	0.004%
91	14.550	4121	4124	4126	rBV	342	267	0.04%	0.005%
92	14.775	4190	4194	4198	rBV2	369	347	0.05%	0.007%
93	14.945	4244	4247	4248	rBV	407	253	0.04%	0.005%
94	15.019	4267	4270	4275	rVB	499	454	0.07%	0.009%
95	15.045	4275	4278	4280	rBV2	305	224	0.03%	0.004%
96	15.080	4287	4289	4292	rVB	411	249	0.04%	0.005%
97	15.103	4292	4296	4299	rBV2	504	526	0.08%	0.010%
98	15.910	4545	4547	4548	rBV	670	251	0.04%	0.005%
99	16.354	4683	4685	4686	rBV2	636	301	0.05%	0.006%
100	16.389	4693	4696	4701	rBV4	1023	757	0.11%	0.014%




Sum of corrected areas: 5246868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060181.D
Acq On : 25 Jul 2024 19:07
Operator : MD/SY
Sample : P3335-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

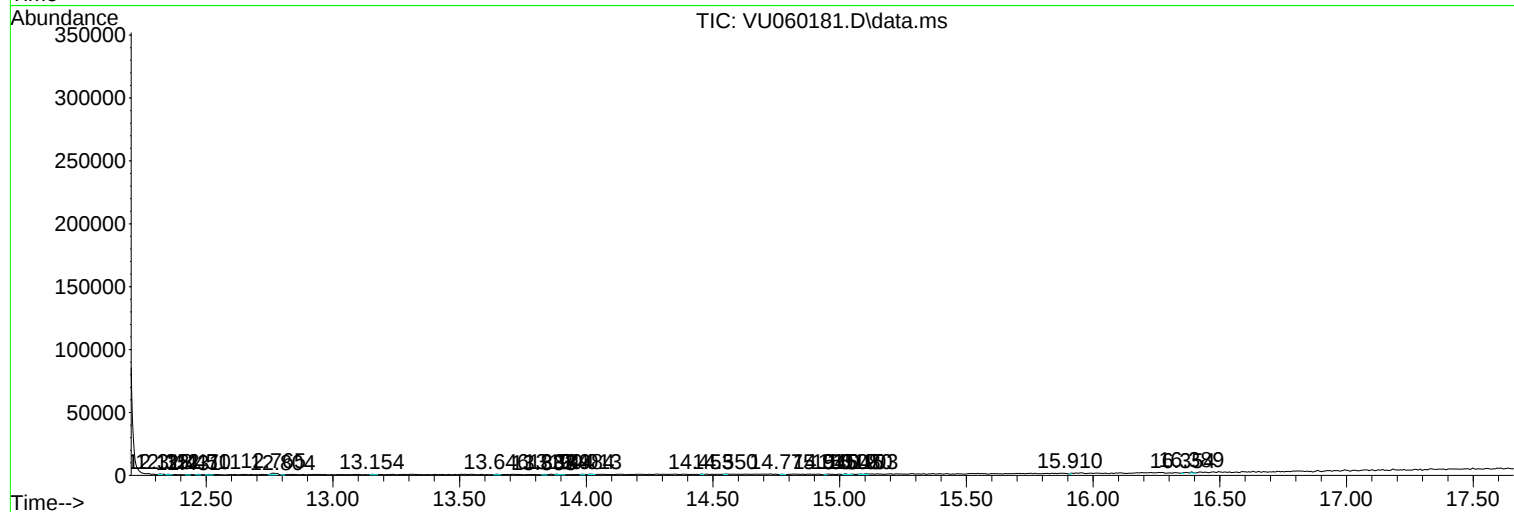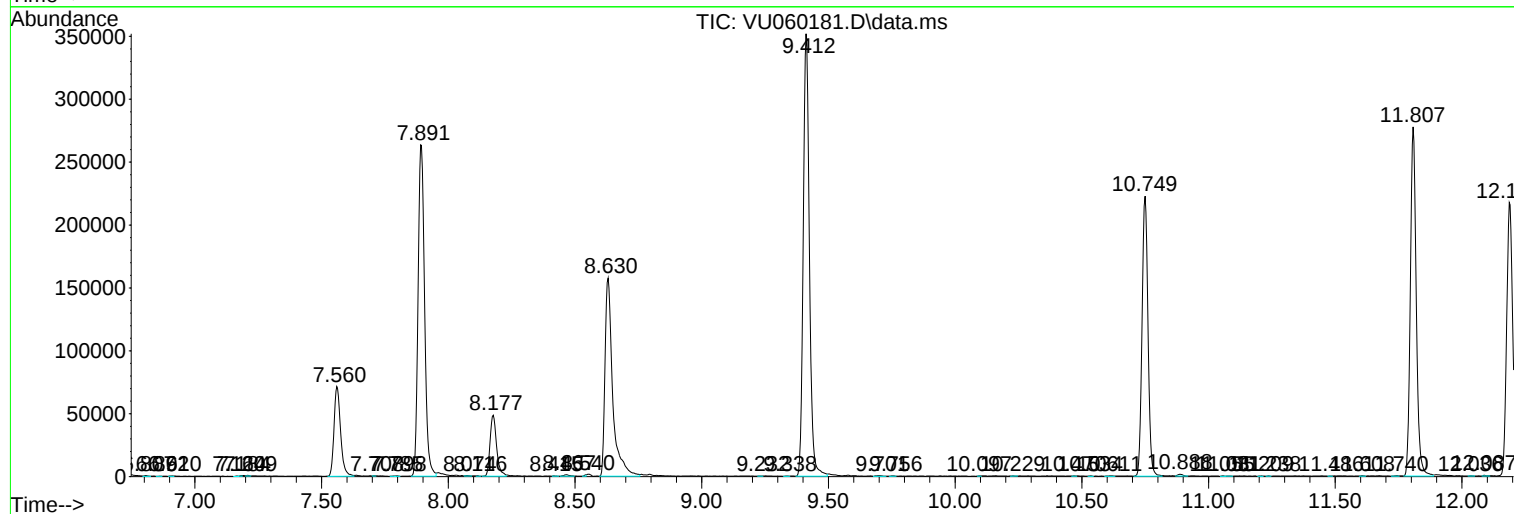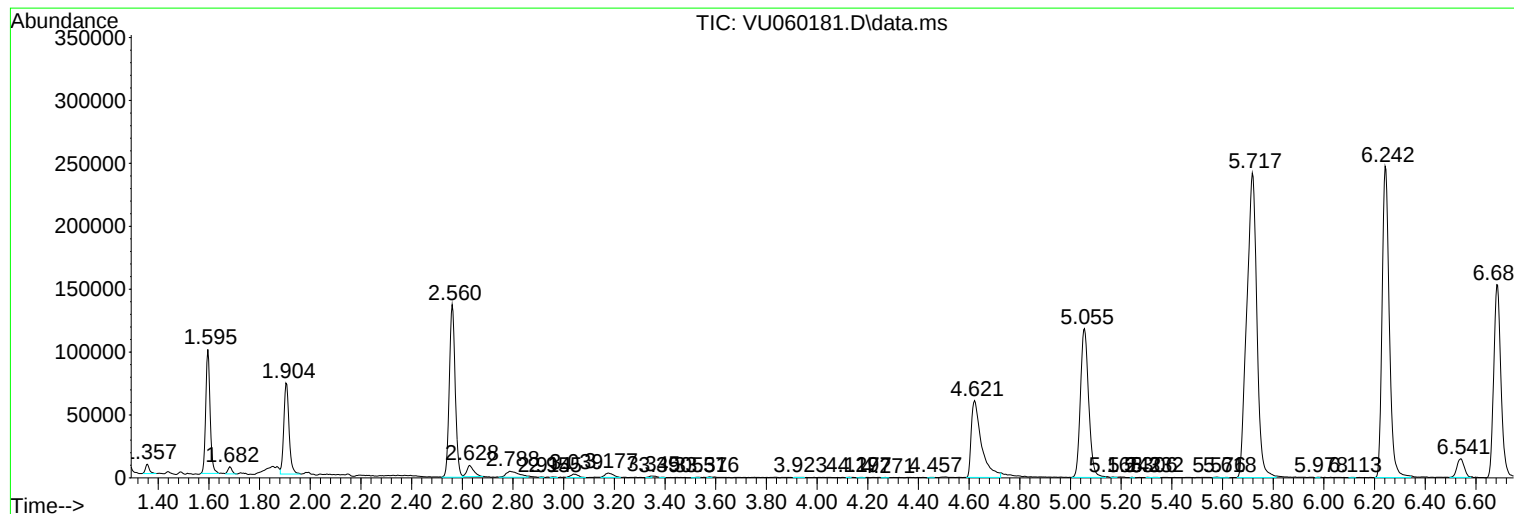

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060181.D
Acq On : 25 Jul 2024 19:07
Operator : MD/SY
Sample : P3335-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060181.D
Acq On : 25 Jul 2024 19:07
Operator : MD/SY
Sample : P3335-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------