

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060183.D
 Acq On : 25 Jul 2024 19:55
 Operator : MD/SY
 Sample : P3335-14 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rBV	96157	112478	7.21%	1.664%
2	1.904	184	191	209	rVB	75398	107518	6.90%	1.591%
3	2.560	383	395	411	rBV	137999	224995	14.43%	3.329%
4	2.776	458	462	463	rBV	328	237	0.02%	0.004%
5	2.846	478	484	491	rBV2	435	660	0.04%	0.010%
6	3.043	535	545	556	rVB	4282	7697	0.49%	0.114%
7	3.178	573	587	600	rBV	5043	11723	0.75%	0.173%
8	3.348	635	640	648	rBV4	636	1127	0.07%	0.017%
9	3.441	665	669	672	rBV	329	300	0.02%	0.004%
10	3.480	679	681	688	rBV	303	395	0.03%	0.006%
11	3.895	807	810	814	rVB2	336	246	0.02%	0.004%
12	3.997	837	842	844	rBV	220	214	0.01%	0.003%
13	4.017	844	848	853	rVB2	227	230	0.01%	0.003%
14	4.120	876	880	884	rBV2	196	238	0.02%	0.004%
15	4.219	908	911	915	rVB2	261	224	0.01%	0.003%
16	4.245	915	919	922	rBV2	305	279	0.02%	0.004%
17	4.290	926	933	939	rBV2	264	437	0.03%	0.006%
18	4.403	964	968	972	rBV	264	304	0.02%	0.004%
19	4.509	996	1001	1005	rVB2	206	224	0.01%	0.003%
20	4.624	1026	1037	1039	rBV	65902	95420	6.12%	1.412%
21	4.895	1118	1121	1124	rVV3	346	245	0.02%	0.004%
22	5.055	1155	1171	1193	rBV	117182	261977	16.80%	3.876%
23	5.319	1249	1253	1258	rVV2	235	276	0.02%	0.004%
24	5.358	1262	1265	1270	rVB2	435	368	0.02%	0.005%
25	5.390	1270	1275	1278	rBV2	275	255	0.02%	0.004%
26	5.438	1285	1290	1292	rBV	255	229	0.01%	0.003%
27	5.505	1307	1311	1316	rBV2	233	311	0.02%	0.005%
28	5.718	1353	1377	1413	rBV2	246690	671008	43.04%	9.927%
29	6.030	1471	1474	1476	rBV	374	265	0.02%	0.004%
30	6.084	1486	1491	1496	rBV2	272	342	0.02%	0.005%
31	6.242	1528	1540	1568	rBV	250323	484105	31.05%	7.162%
32	6.534	1617	1631	1660	rBV	819621	1559134	100.00%	23.067%
33	6.682	1665	1677	1700	rVB	156752	311101	19.95%	4.603%
34	6.811	1713	1717	1721	rVB3	595	493	0.03%	0.007%
35	7.100	1801	1807	1809	rBV2	305	350	0.02%	0.005%
36	7.200	1832	1838	1840	rBV3	322	339	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060183.D
 Acq On : 25 Jul 2024 19:55
 Operator : MD/SY
 Sample : P3335-14 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.216	1840	1843	1851	rVV2	540	551	0.04%	0.008%
38	7.357	1883	1887	1893	rBV2	290	240	0.02%	0.004%
39	7.502	1926	1932	1936	rVB2	251	297	0.02%	0.004%
40	7.560	1936	1950	1971	rBV	74510	135008	8.66%	1.997%
41	7.679	1985	1987	1991	rVB2	314	239	0.02%	0.004%
42	7.718	1996	1999	2004	rVB3	589	614	0.04%	0.009%
43	7.759	2009	2012	2015	rVB	354	219	0.01%	0.003%
44	7.891	2041	2053	2080	rBV	273543	488482	31.33%	7.227%
45	8.177	2131	2142	2163	rBV	49782	89913	5.77%	1.330%
46	8.293	2174	2178	2182	rBV3	365	361	0.02%	0.005%
47	8.399	2204	2211	2222	rVB5	1823	2768	0.18%	0.041%
48	8.509	2240	2245	2248	rVB	222	228	0.01%	0.003%
49	8.537	2248	2254	2255	rBV2	250	247	0.02%	0.004%
50	8.550	2255	2258	2263	rVB3	1003	742	0.05%	0.011%
51	8.631	2272	2283	2316	rBV2	159212	328327	21.06%	4.858%
52	8.914	2369	2371	2375	rVB2	398	218	0.01%	0.003%
53	9.412	2514	2526	2557	rVV	368188	618926	39.70%	9.157%
54	9.595	2580	2583	2588	rVV3	284	263	0.02%	0.004%
55	9.627	2589	2593	2597	rVB2	314	293	0.02%	0.004%
56	9.663	2600	2604	2608	rBV	272	272	0.02%	0.004%
57	9.737	2623	2627	2631	rBV2	293	262	0.02%	0.004%
58	9.959	2692	2696	2700	rVV	197	216	0.01%	0.003%
59	9.981	2700	2703	2706	rVV	344	249	0.02%	0.004%
60	10.039	2717	2721	2725	rBV2	387	343	0.02%	0.005%
61	10.123	2742	2747	2749	rBV	250	295	0.02%	0.004%
62	10.454	2846	2850	2857	rBV2	242	323	0.02%	0.005%
63	10.505	2863	2866	2871	rBV2	227	243	0.02%	0.004%
64	10.750	2929	2942	2963	rBV	221527	358503	22.99%	5.304%
65	10.849	2971	2973	2976	rVB3	403	212	0.01%	0.003%
66	10.878	2979	2982	2983	rBV2	400	233	0.01%	0.003%
67	10.959	3004	3007	3011	rVB	256	237	0.02%	0.004%
68	10.991	3011	3017	3020	rBV	261	269	0.02%	0.004%
69	11.225	3087	3090	3093	rBV	277	252	0.02%	0.004%
70	11.576	3196	3199	3202	rVB	368	207	0.01%	0.003%
71	11.807	3259	3271	3296	rBV	291130	475436	30.49%	7.034%
72	12.071	3350	3353	3358	rBV2	237	253	0.02%	0.004%
73	12.187	3377	3389	3413	rBV	227345	387466	24.85%	5.732%
74	12.344	3436	3438	3441	rVB2	498	250	0.02%	0.004%
75	12.444	3464	3469	3472	rBV2	347	338	0.02%	0.005%
76	12.614	3518	3522	3527	rVB	251	244	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060183.D
 Acq On : 25 Jul 2024 19:55
 Operator : MD/SY
 Sample : P3335-14 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.647	3529	3532	3535	rBV2	297	254	0.02%	0.004%
78	12.698	3542	3548	3550	rBV2	289	322	0.02%	0.005%
79	12.766	3563	3569	3577	rVB4	1213	2050	0.13%	0.030%
80	12.823	3584	3587	3589	rBV	358	213	0.01%	0.003%
81	13.084	3665	3668	3672	rBV2	214	211	0.01%	0.003%
82	13.219	3704	3710	3712	rBV2	344	402	0.03%	0.006%
83	13.296	3731	3734	3741	rVB2	280	314	0.02%	0.005%
84	13.540	3806	3810	3812	rBV	365	242	0.02%	0.004%
85	13.576	3816	3821	3823	rVB2	340	262	0.02%	0.004%
86	13.598	3823	3828	3831	rBV2	267	222	0.01%	0.003%
87	13.618	3831	3834	3839	rBV	242	212	0.01%	0.003%
88	13.798	3886	3890	3893	rBV	271	207	0.01%	0.003%
89	13.849	3904	3906	3913	rVB2	325	275	0.02%	0.004%
90	14.084	3977	3979	3987	rVB2	262	281	0.02%	0.004%
91	14.119	3987	3990	3995	rBV2	341	365	0.02%	0.005%
92	14.528	4114	4117	4118	rBV	393	236	0.02%	0.003%
93	14.582	4131	4134	4140	rVB4	462	464	0.03%	0.007%
94	14.778	4191	4195	4203	rBV2	408	595	0.04%	0.009%
95	14.839	4211	4214	4219	rVB2	473	390	0.03%	0.006%
96	15.219	4328	4332	4334	rBV2	448	392	0.03%	0.006%
97	15.235	4334	4337	4340	rVV3	555	428	0.03%	0.006%
98	15.293	4352	4355	4358	rBV	422	319	0.02%	0.005%
99	15.624	4454	4458	4460	rBV2	423	336	0.02%	0.005%
100	15.666	4467	4471	4472	rBV2	459	359	0.02%	0.005%




Sum of corrected areas: 6759134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060183.D
Acq On : 25 Jul 2024 19:55
Operator : MD/SY
Sample : P3335-14 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

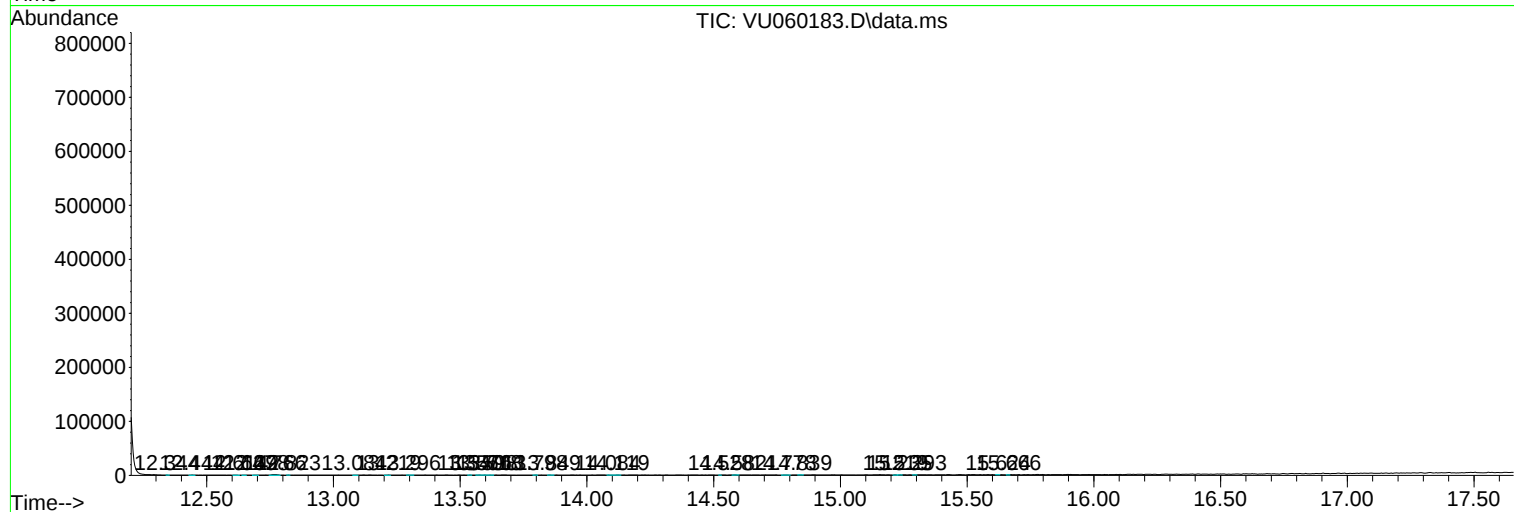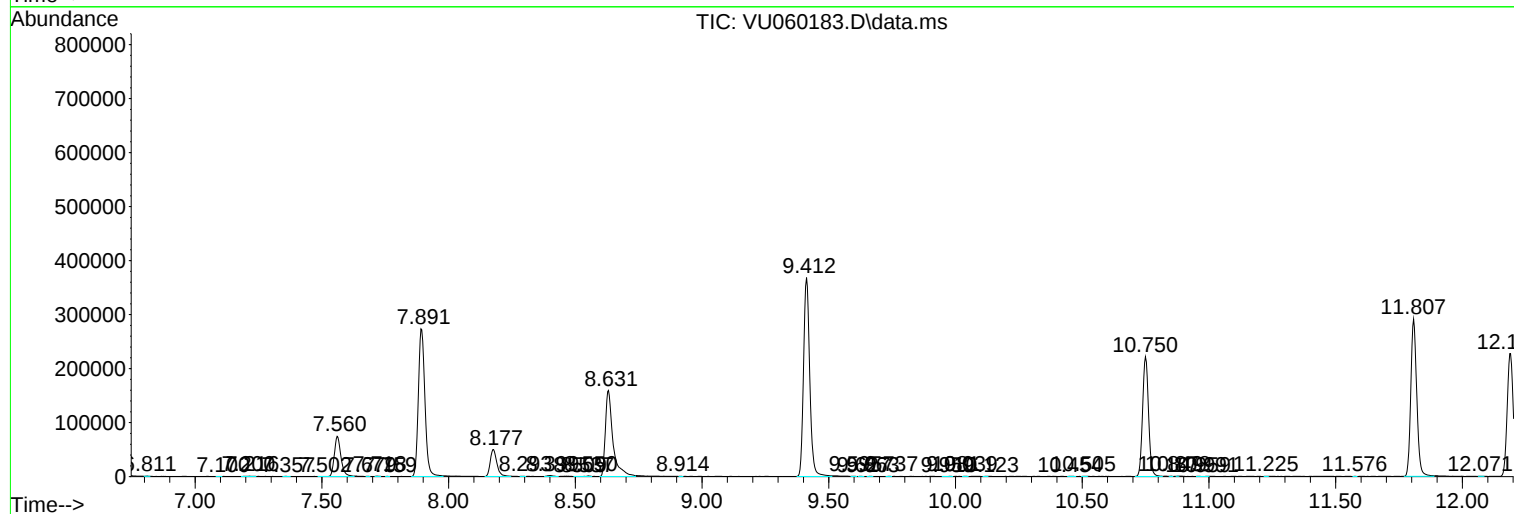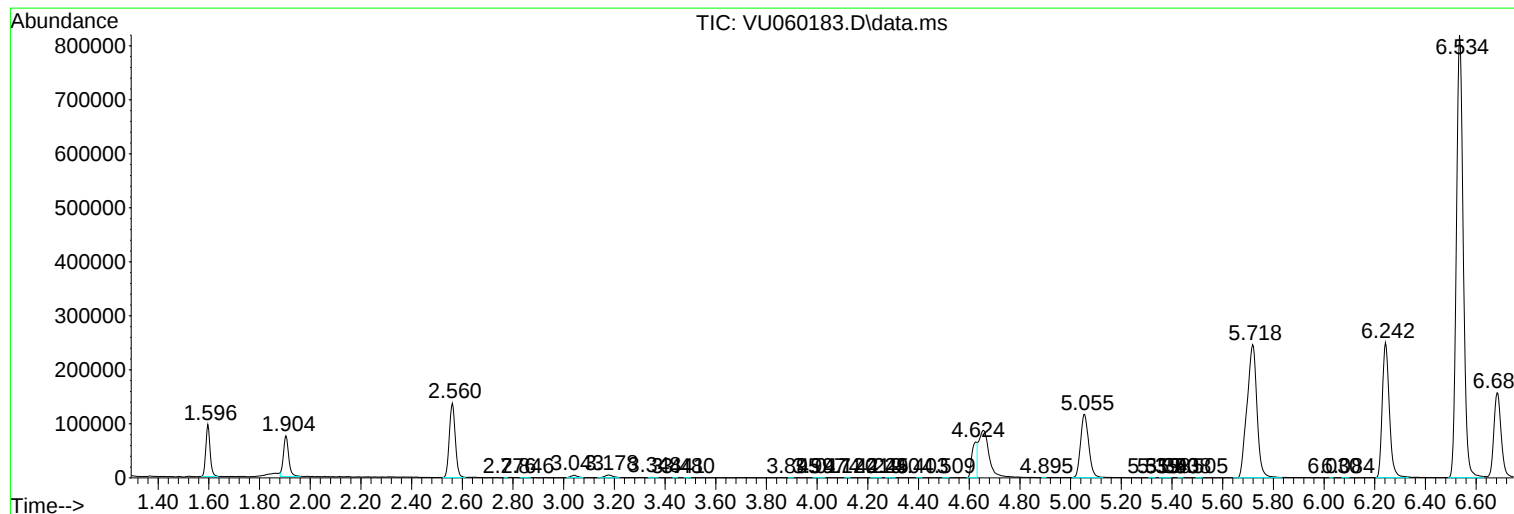

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060183.D
Acq On : 25 Jul 2024 19:55
Operator : MD/SY
Sample : P3335-14 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060183.D
Acq On : 25 Jul 2024 19:55
Operator : MD/SY
Sample : P3335-14 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------