

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060185.D
 Acq On : 25 Jul 2024 20:42
 Operator : MD/SY
 Sample : P3335-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	97109	111404	12.26%	1.749%
2	1.904	184	191	210	rVB	77115	109836	12.09%	1.724%
3	2.560	383	395	412	rBV	140747	236146	25.98%	3.707%
4	2.788	460	466	470	rBV3	454	524	0.06%	0.008%
5	3.039	534	544	560	rVB4	4968	10559	1.16%	0.166%
6	3.100	560	563	566	rBV	295	235	0.03%	0.004%
7	3.178	574	587	604	rVV	8534	18907	2.08%	0.297%
8	3.599	715	718	724	rVB2	336	315	0.03%	0.005%
9	3.628	724	727	731	rBV2	309	233	0.03%	0.004%
10	3.676	737	742	746	rBV2	340	328	0.04%	0.005%
11	3.698	746	749	753	rBV	238	239	0.03%	0.004%
12	3.792	775	778	784	rVB2	279	280	0.03%	0.004%
13	3.833	784	791	795	rBV2	289	409	0.05%	0.006%
14	3.872	801	803	808	rBV2	248	267	0.03%	0.004%
15	3.930	819	821	826	rBV2	203	224	0.02%	0.004%
16	4.094	869	872	878	rBV	256	287	0.03%	0.005%
17	4.158	886	892	897	rBV2	231	307	0.03%	0.005%
18	4.197	897	904	908	rVB2	213	290	0.03%	0.005%
19	4.438	974	979	983	rVB2	255	208	0.02%	0.003%
20	4.621	1024	1036	1066	rBV	64946	199825	21.99%	3.137%
21	4.875	1112	1115	1119	rBV2	216	224	0.02%	0.004%
22	4.927	1128	1131	1134	rBV	348	252	0.03%	0.004%
23	4.943	1134	1136	1141	rVB2	288	214	0.02%	0.003%
24	5.055	1155	1171	1196	rBV	120031	266881	29.37%	4.189%
25	5.165	1202	1205	1208	rVB2	425	289	0.03%	0.005%
26	5.486	1302	1305	1310	rVV2	203	238	0.03%	0.004%
27	5.718	1357	1377	1402	rBV2	247127	674659	74.23%	10.590%
28	5.981	1456	1459	1461	rBV2	327	221	0.02%	0.003%
29	6.013	1466	1469	1473	rBV2	426	353	0.04%	0.006%
30	6.242	1527	1540	1568	rBV	267303	521020	57.33%	8.179%
31	6.409	1589	1592	1595	rBV3	437	307	0.03%	0.005%
32	6.534	1618	1631	1665	rBV	477117	908816	100.00%	14.266%
33	6.682	1665	1677	1700	rVB	158193	310163	34.13%	4.869%
34	6.801	1712	1714	1721	rVB2	502	476	0.05%	0.007%
35	7.046	1788	1790	1797	rVB2	246	325	0.04%	0.005%
36	7.200	1835	1838	1839	rBV	435	245	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060185.D
Acq On : 25 Jul 2024 20:42
Operator : MD/SY
Sample : P3335-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis

37	7.229	1844	1847	1851	rVB2	355	233	0.03%	0.004%
38	7.251	1851	1854	1857	rBV2	290	266	0.03%	0.004%
39	7.560	1938	1950	1969	rBV	74263	135842	14.95%	2.132%
40	7.788	2017	2021	2022	rBV	302	208	0.02%	0.003%
41	7.833	2033	2035	2041	rVB2	273	213	0.02%	0.003%
42	7.891	2041	2053	2075	rBV	271394	487413	53.63%	7.651%
43	8.091	2111	2115	2116	rBV	330	192	0.02%	0.003%
44	8.174	2129	2141	2163	rBV2	49516	88093	9.69%	1.383%
45	8.406	2210	2213	2215	rBV	335	227	0.02%	0.004%
46	8.460	2227	2230	2232	rBV2	286	246	0.03%	0.004%
47	8.544	2252	2256	2259	rBV	296	215	0.02%	0.003%
48	8.631	2272	2283	2321	rBV2	160150	335853	36.96%	5.272%
49	8.949	2380	2382	2389	rVB2	399	319	0.04%	0.005%
50	8.994	2394	2396	2400	rVB2	358	228	0.03%	0.004%
51	9.033	2405	2408	2415	rVB2	290	251	0.03%	0.004%
52	9.078	2415	2422	2427	rBV2	266	417	0.05%	0.007%
53	9.116	2431	2434	2437	rBV	290	253	0.03%	0.004%
54	9.412	2513	2526	2551	rBV	391346	659803	72.60%	10.357%
55	9.576	2573	2577	2582	rBV4	426	500	0.06%	0.008%
56	9.624	2589	2592	2596	rVB2	248	205	0.02%	0.003%
57	9.653	2596	2601	2603	rBV	216	232	0.03%	0.004%
58	9.695	2612	2614	2618	rVB	348	238	0.03%	0.004%
59	9.801	2644	2647	2649	rBV	252	195	0.02%	0.003%
60	9.885	2670	2673	2676	rVB	362	241	0.03%	0.004%
61	10.190	2763	2768	2770	rBV	257	204	0.02%	0.003%
62	10.348	2813	2817	2819	rBV	219	194	0.02%	0.003%
63	10.415	2835	2838	2844	rBV2	266	243	0.03%	0.004%
64	10.467	2849	2854	2858	rBV2	166	219	0.02%	0.003%
65	10.750	2929	2942	2958	rBV	223833	363308	39.98%	5.703%
66	10.878	2979	2982	2984	rBV	321	222	0.02%	0.003%
67	10.923	2992	2996	3001	rBV	265	290	0.03%	0.005%
68	11.058	3035	3038	3044	rBV	212	213	0.02%	0.003%
69	11.094	3044	3049	3052	rVB2	285	255	0.03%	0.004%
70	11.116	3052	3056	3059	rBV	309	301	0.03%	0.005%
71	11.180	3072	3076	3079	rBV	288	277	0.03%	0.004%
72	11.225	3084	3090	3092	rBV2	217	255	0.03%	0.004%
73	11.290	3106	3110	3114	rBV2	396	463	0.05%	0.007%
74	11.370	3133	3135	3140	rVB2	346	288	0.03%	0.005%
75	11.483	3167	3170	3176	rVB2	423	312	0.03%	0.005%
76	11.695	3233	3236	3240	rBV	198	227	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060185.D
 Acq On : 25 Jul 2024 20:42
 Operator : MD/SY
 Sample : P3335-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E20M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.807	3260	3271	3294	rBV	314194	513012	56.45%	8.053%
78	11.994	3327	3329	3334	rVB	327	203	0.02%	0.003%
79	12.187	3376	3389	3409	rBV	230618	394187	43.37%	6.188%
80	12.495	3481	3485	3489	rVV2	278	347	0.04%	0.005%
81	12.643	3525	3531	3533	rBV2	282	347	0.04%	0.005%
82	12.769	3562	3570	3577	rBV3	929	1596	0.18%	0.025%
83	13.344	3746	3749	3753	rBV2	280	215	0.02%	0.003%
84	13.560	3813	3816	3822	rBV2	296	317	0.03%	0.005%
85	13.592	3822	3826	3829	rBV2	268	272	0.03%	0.004%
86	13.643	3838	3842	3845	rBV2	434	289	0.03%	0.005%
87	13.663	3845	3848	3853	rBV2	285	273	0.03%	0.004%
88	13.766	3878	3880	3885	rBV2	286	271	0.03%	0.004%
89	13.920	3924	3928	3931	rVB2	333	274	0.03%	0.004%
90	14.036	3960	3964	3969	rBV2	398	450	0.05%	0.007%
91	14.071	3972	3975	3977	rBV2	378	259	0.03%	0.004%
92	14.267	4033	4036	4039	rBV	278	218	0.02%	0.003%
93	14.344	4055	4060	4067	rBV3	434	592	0.07%	0.009%
94	14.383	4067	4072	4075	rBV	469	503	0.06%	0.008%
95	14.450	4089	4093	4095	rBV2	398	310	0.03%	0.005%
96	15.090	4289	4292	4294	rBV2	380	266	0.03%	0.004%
97	15.190	4320	4323	4328	rBV4	503	436	0.05%	0.007%
98	15.849	4526	4528	4529	rBV	466	205	0.02%	0.003%
99	15.926	4550	4552	4556	rBV3	444	371	0.04%	0.006%
100	16.122	4609	4613	4615	rBV3	781	606	0.07%	0.010%




Sum of corrected areas: 6370479

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060185.D
Acq On : 25 Jul 2024 20:42
Operator : MD/SY
Sample : P3335-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

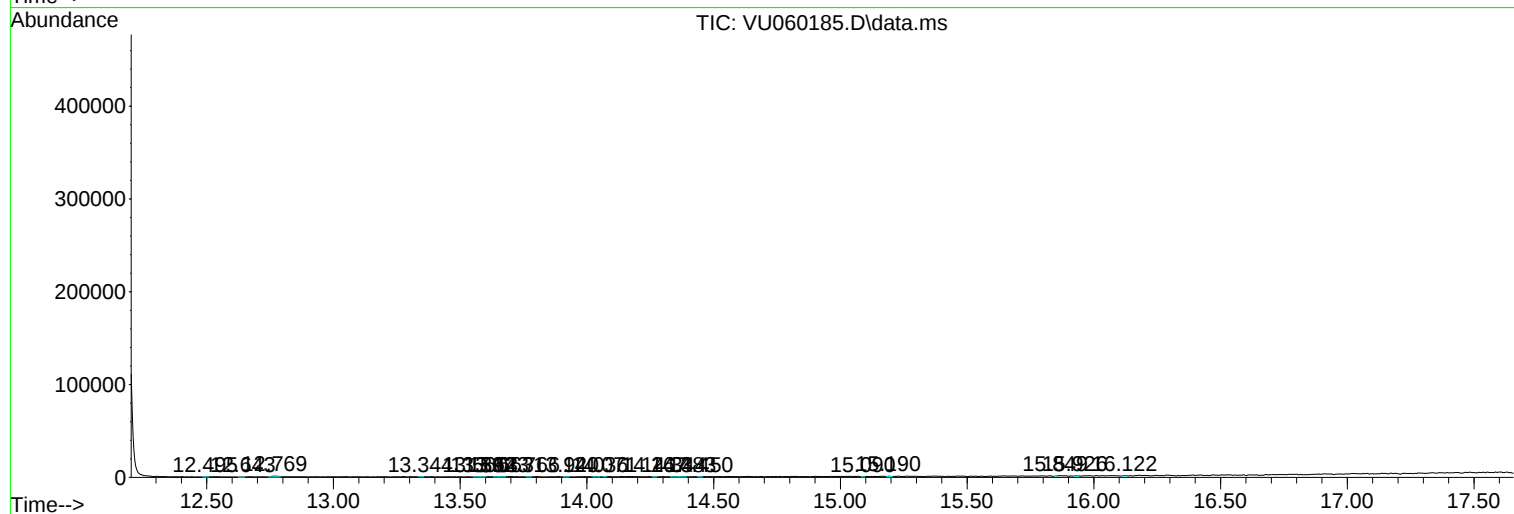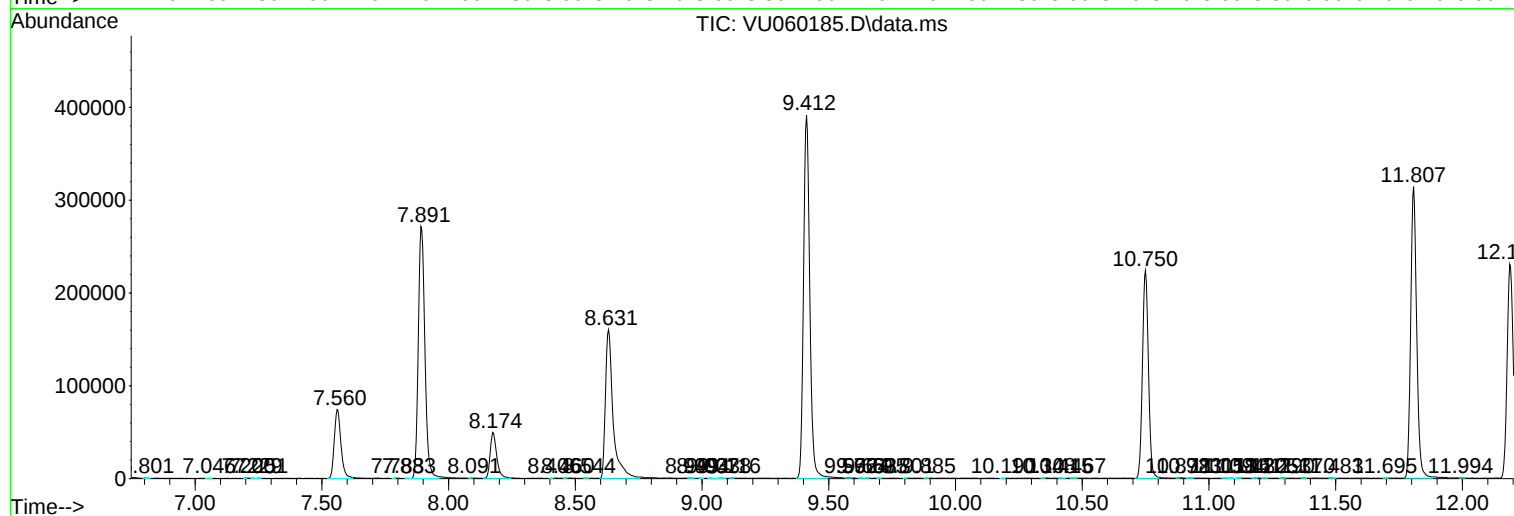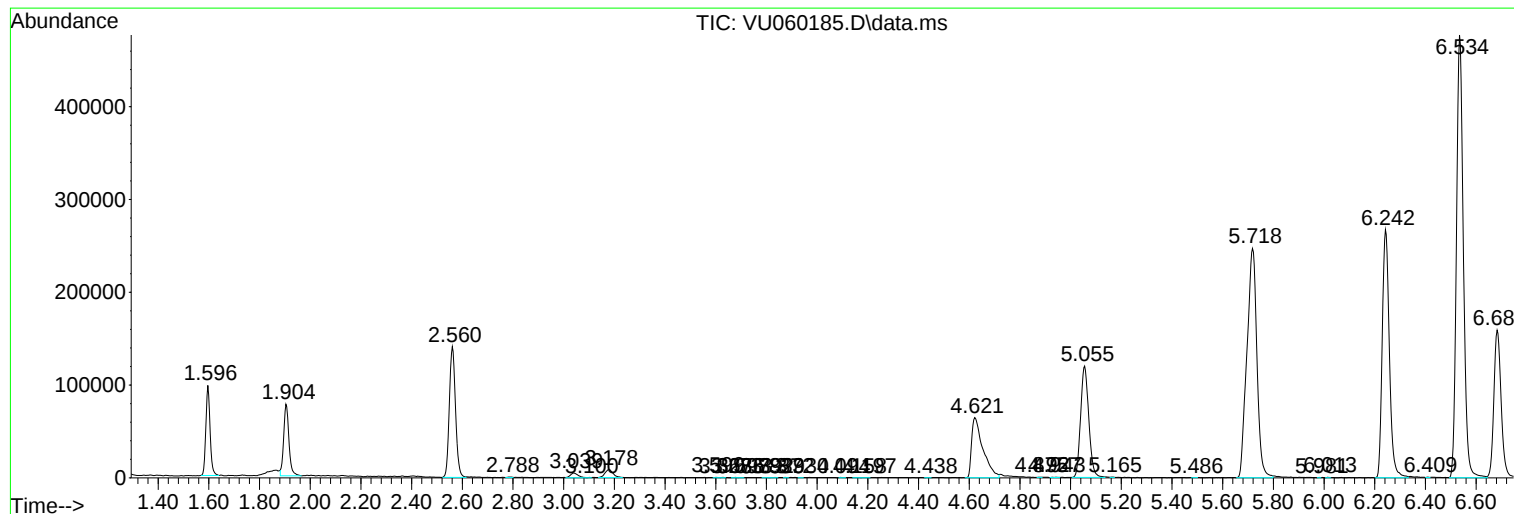

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060185.D
Acq On : 25 Jul 2024 20:42
Operator : MD/SY
Sample : P3335-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060185.D
Acq On : 25 Jul 2024 20:42
Operator : MD/SY
Sample : P3335-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E20M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------