

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060197.D
 Acq On : 26 Jul 2024 01:50
 Operator : MD/SY
 Sample : P3348-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	17	21	28	rBV3	2970	3137	0.46%	0.058%
2	1.489	58	62	67	rVB4	1526	1576	0.23%	0.029%
3	1.595	88	95	114	rVB	97204	115589	17.09%	2.152%
4	1.907	184	192	206	rVB	79211	110174	16.28%	2.052%
5	2.476	366	369	374	rBV2	310	361	0.05%	0.007%
6	2.560	383	395	412	rBV	137720	225119	33.28%	4.192%
7	2.795	458	468	471	rBV4	793	1265	0.19%	0.024%
8	3.042	536	545	559	rVB3	2179	4231	0.63%	0.079%
9	3.177	575	587	607	rVB2	3946	9469	1.40%	0.176%
10	3.264	610	614	617	rVB2	187	173	0.03%	0.003%
11	3.280	617	619	622	rBV	272	172	0.03%	0.003%
12	3.300	622	625	628	rBV2	221	194	0.03%	0.004%
13	3.351	637	641	645	rVB	366	348	0.05%	0.006%
14	3.483	679	682	686	rBV2	217	245	0.04%	0.005%
15	3.525	690	695	698	rBV2	184	239	0.04%	0.004%
16	3.599	714	718	721	rBV2	252	282	0.04%	0.005%
17	3.859	796	799	802	rBV2	289	216	0.03%	0.004%
18	4.142	883	887	897	rVB2	347	524	0.08%	0.010%
19	4.219	908	911	915	rBV2	198	177	0.03%	0.003%
20	4.624	1025	1037	1071	rBV	55131	158080	23.37%	2.944%
21	4.856	1105	1109	1110	rBV2	334	257	0.04%	0.005%
22	5.055	1156	1171	1195	rBV	119451	269878	39.89%	5.025%
23	5.335	1256	1258	1261	rVB2	402	265	0.04%	0.005%
24	5.370	1261	1269	1272	rBV	390	518	0.08%	0.010%
25	5.505	1308	1311	1314	rBV2	216	173	0.03%	0.003%
26	5.576	1329	1333	1338	rBV2	180	222	0.03%	0.004%
27	5.717	1357	1377	1406	rBV3	246525	676538	100.00%	12.598%
28	5.955	1447	1451	1457	rBV3	374	437	0.06%	0.008%
29	5.981	1457	1459	1464	rVB3	301	244	0.04%	0.005%
30	6.180	1515	1521	1527	rBV2	488	667	0.10%	0.012%
31	6.242	1527	1540	1564	rBV	254117	489787	72.40%	9.120%
32	6.425	1594	1597	1600	rBV	265	193	0.03%	0.004%
33	6.479	1610	1614	1616	rBV2	262	227	0.03%	0.004%
34	6.537	1621	1632	1648	rVB7	3813	8500	1.26%	0.158%
35	6.598	1648	1651	1657	rVB2	351	296	0.04%	0.006%
36	6.682	1664	1677	1699	rBV	155658	309370	45.73%	5.761%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060197.D
 Acq On : 26 Jul 2024 01:50
 Operator : MD/SY
 Sample : P3348-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.885	1736	1740	1743	rBV	271	309	0.05%	0.006%
38	6.959	1760	1763	1768	rVB	227	201	0.03%	0.004%
39	7.103	1793	1808	1820	rBV3	3015	5199	0.77%	0.097%
40	7.203	1834	1839	1842	rBV3	282	287	0.04%	0.005%
41	7.508	1931	1934	1939	rBV2	253	266	0.04%	0.005%
42	7.560	1939	1950	1970	rBV2	71720	130075	19.23%	2.422%
43	7.631	1970	1972	1982	rVB5	853	914	0.14%	0.017%
44	7.676	1982	1986	1989	rVB3	262	195	0.03%	0.004%
45	7.717	1993	1999	2001	rBV3	354	386	0.06%	0.007%
46	7.766	2011	2014	2017	rBV2	314	203	0.03%	0.004%
47	7.891	2041	2053	2071	rBV	274703	487217	72.02%	9.073%
48	8.177	2130	2142	2163	rBV	47838	85443	12.63%	1.591%
49	8.467	2218	2232	2243	rVB3	4533	7677	1.13%	0.143%
50	8.537	2251	2254	2256	rBV2	287	214	0.03%	0.004%
51	8.553	2256	2259	2263	rVB	259	197	0.03%	0.004%
52	8.631	2273	2283	2311	rBV2	144716	306330	45.28%	5.704%
53	8.804	2328	2337	2349	rVB5	6689	11177	1.65%	0.208%
54	8.875	2355	2359	2365	rVB2	377	406	0.06%	0.008%
55	8.952	2379	2383	2386	rBV2	248	217	0.03%	0.004%
56	9.010	2398	2401	2405	rBV	258	224	0.03%	0.004%
57	9.145	2440	2443	2447	rBV2	210	211	0.03%	0.004%
58	9.412	2513	2526	2559	rBV	365436	626740	92.64%	11.671%
59	9.692	2609	2613	2624	rVB3	750	1168	0.17%	0.022%
60	9.859	2662	2665	2671	rVB	210	187	0.03%	0.003%
61	10.097	2729	2739	2757	rVB2	21599	36513	5.40%	0.680%
62	10.164	2757	2760	2763	rVB2	270	186	0.03%	0.003%
63	10.190	2763	2768	2771	rBV2	302	332	0.05%	0.006%
64	10.212	2771	2775	2779	rVB	313	264	0.04%	0.005%
65	10.245	2780	2785	2788	rBV2	333	350	0.05%	0.007%
66	10.293	2791	2800	2807	rVB5	2653	4279	0.63%	0.080%
67	10.489	2854	2861	2864	rBV2	384	440	0.07%	0.008%
68	10.598	2892	2895	2898	rVB2	268	184	0.03%	0.003%
69	10.698	2922	2926	2928	rBV	260	215	0.03%	0.004%
70	10.749	2928	2942	2960	rVV	217012	354726	52.43%	6.605%
71	10.888	2975	2985	2996	rVB2	8127	12576	1.86%	0.234%
72	11.090	3045	3048	3051	rBV	272	179	0.03%	0.003%
73	11.473	3164	3167	3168	rBV3	312	177	0.03%	0.003%
74	11.483	3168	3170	3175	rVV2	413	351	0.05%	0.007%
75	11.511	3175	3179	3181	rVV	268	185	0.03%	0.003%
76	11.531	3181	3185	3189	rVV2	216	188	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060197.D
 Acq On : 26 Jul 2024 01:50
 Operator : MD/SY
 Sample : P3348-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.746	3249	3252	3258	rBV3	476	480	0.07%	0.009%
78	11.807	3258	3271	3293	rBV	297775	496722	73.42%	9.250%
79	12.084	3354	3357	3361	rVB2	300	189	0.03%	0.004%
80	12.187	3377	3389	3409	rBV	239244	395827	58.51%	7.371%
81	12.425	3460	3463	3468	rBV	348	203	0.03%	0.004%
82	12.569	3505	3508	3514	rVV2	389	493	0.07%	0.009%
83	12.608	3518	3520	3524	rVV2	373	254	0.04%	0.005%
84	12.643	3525	3531	3536	rVB	283	308	0.05%	0.006%
85	12.769	3561	3570	3583	rVB2	2967	5237	0.77%	0.098%
86	12.830	3583	3589	3593	rBV2	302	421	0.06%	0.008%
87	12.920	3614	3617	3620	rVB2	368	249	0.04%	0.005%
88	13.007	3641	3644	3652	rVB2	335	309	0.05%	0.006%
89	13.232	3712	3714	3717	rBV2	419	212	0.03%	0.004%
90	13.447	3778	3781	3785	rBV2	254	206	0.03%	0.004%
91	13.621	3832	3835	3837	rBV	266	204	0.03%	0.004%
92	13.640	3838	3841	3845	rVV2	439	364	0.05%	0.007%
93	13.855	3906	3908	3911	rVB2	363	207	0.03%	0.004%
94	14.129	3990	3993	3998	rBV2	374	422	0.06%	0.008%
95	14.267	4029	4036	4041	rVB3	392	604	0.09%	0.011%
96	14.511	4109	4112	4114	rBV2	299	224	0.03%	0.004%
97	15.003	4262	4265	4266	rBV2	341	203	0.03%	0.004%
98	15.502	4415	4420	4422	rBV3	438	406	0.06%	0.008%
99	15.849	4525	4528	4530	rBV2	652	456	0.07%	0.008%
100	16.087	4600	4602	4604	rBV	489	290	0.04%	0.005%




Sum of corrected areas: 5370221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060197.D
Acq On : 26 Jul 2024 01:50
Operator : MD/SY
Sample : P3348-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

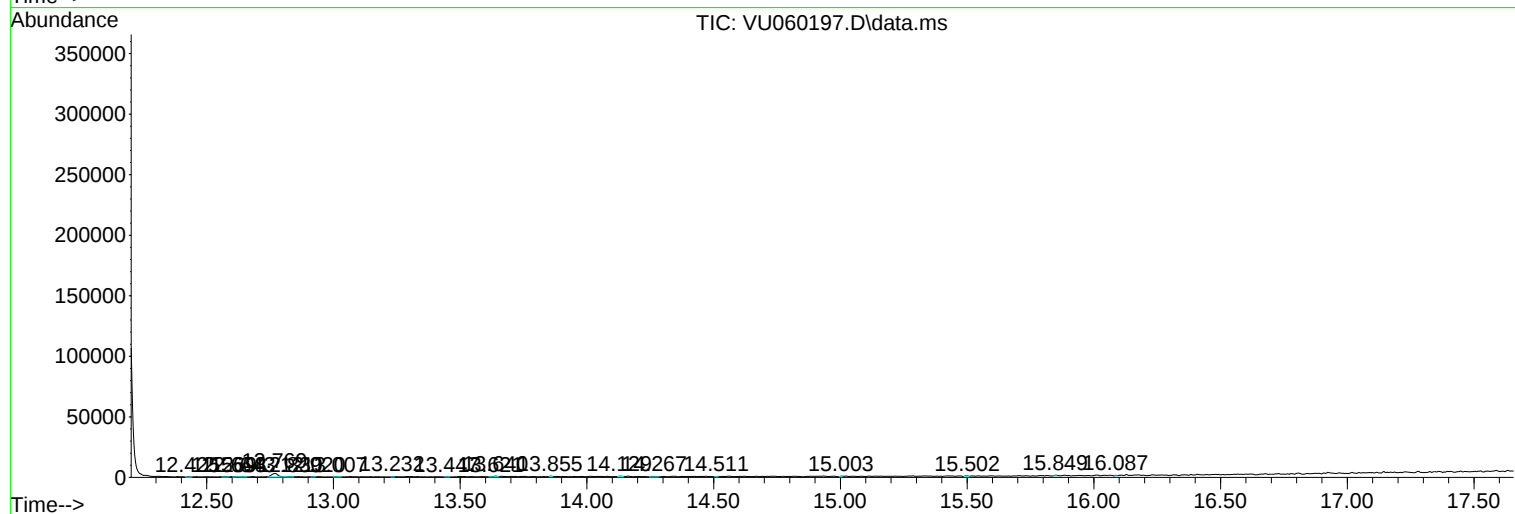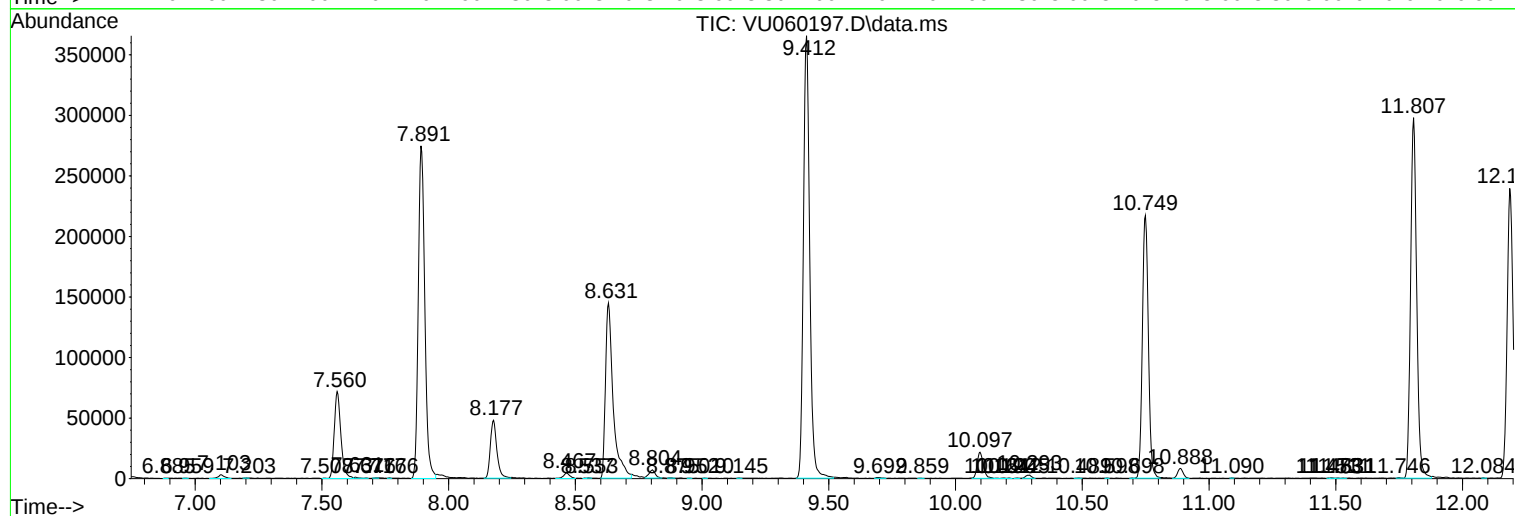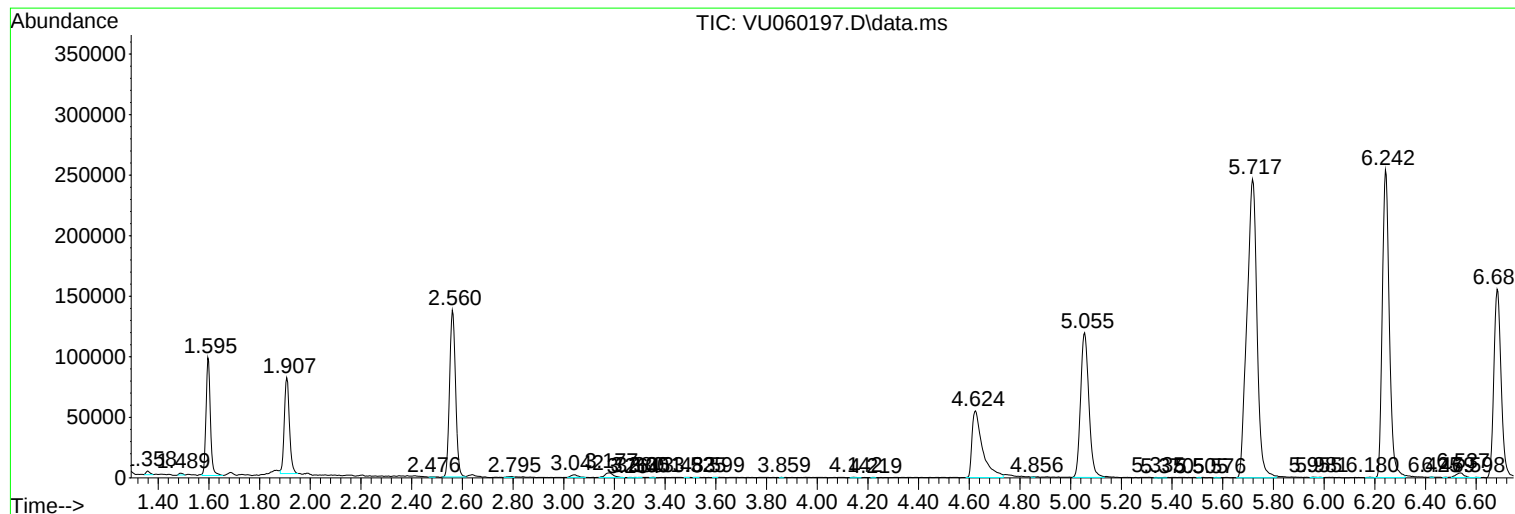

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060197.D
Acq On : 26 Jul 2024 01:50
Operator : MD/SY
Sample : P3348-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060197.D
Acq On : 26 Jul 2024 01:50
Operator : MD/SY
Sample : P3348-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
