

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060217.D
 Acq On : 26 Jul 2024 09:44
 Operator : MD/SY
 Sample : P3260-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	115	rVB	102761	121012	16.46%	2.086%
2	1.904	185	191	208	rVB	79784	112074	15.25%	1.932%
3	2.560	384	395	411	rBV	149589	243234	33.09%	4.192%
4	2.789	458	466	478	rVB	7307	12381	1.68%	0.213%
5	3.039	534	544	557	rBV3	5709	11269	1.53%	0.194%
6	3.178	577	587	601	rBV2	3099	6749	0.92%	0.116%
7	3.252	606	610	613	rBV2	224	207	0.03%	0.004%
8	3.313	626	629	632	rVB2	181	134	0.02%	0.002%
9	3.338	632	637	640	rBV2	177	216	0.03%	0.004%
10	3.403	653	657	660	rBV2	162	124	0.02%	0.002%
11	3.477	679	680	682	rVB	360	127	0.02%	0.002%
12	3.637	725	730	734	rBV	246	290	0.04%	0.005%
13	3.898	807	811	815	rVB2	287	299	0.04%	0.005%
14	3.924	815	819	821	rBV	303	257	0.03%	0.004%
15	4.023	847	850	853	rBV	243	217	0.03%	0.004%
16	4.326	941	944	950	rVB	279	303	0.04%	0.005%
17	4.358	951	954	957	rBV	191	132	0.02%	0.002%
18	4.416	969	972	975	rBV2	136	137	0.02%	0.002%
19	4.483	988	993	996	rBV2	377	376	0.05%	0.006%
20	4.528	1001	1007	1011	rVB2	314	350	0.05%	0.006%
21	4.557	1013	1016	1020	rBV2	201	129	0.02%	0.002%
22	4.621	1027	1036	1060	rBV	62386	161480	21.97%	2.783%
23	4.885	1115	1118	1120	rBV2	324	253	0.03%	0.004%
24	5.055	1156	1171	1198	rBV	125427	279554	38.03%	4.818%
25	5.255	1226	1233	1234	rBV	315	286	0.04%	0.005%
26	5.309	1247	1250	1253	rBV	211	196	0.03%	0.003%
27	5.441	1286	1291	1294	rBV2	219	186	0.03%	0.003%
28	5.502	1304	1310	1313	rBV	233	308	0.04%	0.005%
29	5.554	1320	1326	1328	rBV	258	284	0.04%	0.005%
30	5.718	1357	1377	1404	rBV2	269893	735060	100.00%	12.670%
31	5.956	1445	1451	1453	rVB2	279	241	0.03%	0.004%
32	5.972	1453	1456	1459	rBV2	221	142	0.02%	0.002%
33	5.994	1459	1463	1467	rVB3	393	418	0.06%	0.007%
34	6.039	1474	1477	1480	rVB	207	126	0.02%	0.002%
35	6.055	1480	1482	1486	rBV2	218	156	0.02%	0.003%
36	6.110	1497	1499	1503	rVB2	373	221	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060217.D
 Acq On : 26 Jul 2024 09:44
 Operator : MD/SY
 Sample : P3260-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.136	1503	1507	1510	rBV2	232	255	0.03%	0.004%
38	6.242	1527	1540	1559	rBV	275682	532540	72.45%	9.179%
39	6.682	1665	1677	1703	rBV	167470	330241	44.93%	5.692%
40	6.924	1749	1752	1754	rBV2	178	148	0.02%	0.003%
41	6.981	1765	1770	1775	rBV2	264	329	0.04%	0.006%
42	7.033	1784	1786	1790	rBV2	216	176	0.02%	0.003%
43	7.187	1831	1834	1836	rBV	275	198	0.03%	0.003%
44	7.206	1836	1840	1846	rBV5	523	674	0.09%	0.012%
45	7.316	1871	1874	1877	rBV	254	218	0.03%	0.004%
46	7.351	1882	1885	1889	rBV	173	174	0.02%	0.003%
47	7.438	1907	1912	1914	rBV	238	175	0.02%	0.003%
48	7.473	1920	1923	1927	rBV2	175	130	0.02%	0.002%
49	7.502	1929	1932	1936	rVB	299	223	0.03%	0.004%
50	7.560	1936	1950	1972	rBV	76449	141321	19.23%	2.436%
51	7.702	1992	1994	1996	rBV	317	213	0.03%	0.004%
52	7.798	2019	2024	2026	rBV2	333	270	0.04%	0.005%
53	7.846	2035	2039	2041	rBV	297	233	0.03%	0.004%
54	7.891	2041	2053	2074	rBV	308144	545594	74.22%	9.404%
55	8.177	2131	2142	2164	rBV	51709	91146	12.40%	1.571%
56	8.467	2228	2232	2235	rBV	367	414	0.06%	0.007%
57	8.592	2268	2271	2273	rBV2	301	212	0.03%	0.004%
58	8.631	2273	2283	2316	rVV2	173055	342695	46.62%	5.907%
59	8.859	2351	2354	2356	rBV	441	228	0.03%	0.004%
60	8.923	2372	2374	2377	rBV	299	127	0.02%	0.002%
61	8.988	2391	2394	2395	rBV	263	158	0.02%	0.003%
62	9.017	2400	2403	2407	rBV2	310	204	0.03%	0.004%
63	9.087	2422	2425	2430	rVB2	169	195	0.03%	0.003%
64	9.148	2441	2444	2446	rBV	272	199	0.03%	0.003%
65	9.248	2472	2475	2478	rBV2	195	173	0.02%	0.003%
66	9.303	2487	2492	2495	rBV2	181	171	0.02%	0.003%
67	9.332	2497	2501	2503	rBV2	251	189	0.03%	0.003%
68	9.412	2514	2526	2552	rBV	397315	671055	91.29%	11.566%
69	9.618	2588	2590	2593	rVB2	307	174	0.02%	0.003%
70	9.644	2593	2598	2600	rBV	251	189	0.03%	0.003%
71	9.904	2676	2679	2682	rVB	302	176	0.02%	0.003%
72	9.923	2682	2685	2689	rBV	203	130	0.02%	0.002%
73	9.949	2689	2693	2697	rVV2	272	285	0.04%	0.005%
74	9.984	2701	2704	2708	rVV2	240	179	0.02%	0.003%
75	10.020	2713	2715	2719	rBV	224	196	0.03%	0.003%
76	10.100	2737	2740	2744	rVV3	314	306	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060217.D
 Acq On : 26 Jul 2024 09:44
 Operator : MD/SY
 Sample : P3260-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.296	2798	2801	2803	rBV2	303	208	0.03%	0.004%
78	10.444	2841	2847	2850	rBV2	294	333	0.05%	0.006%
79	10.464	2850	2853	2857	rBV2	365	356	0.05%	0.006%
80	10.608	2895	2898	2902	rBV2	235	171	0.02%	0.003%
81	10.631	2902	2905	2908	rBV2	171	145	0.02%	0.002%
82	10.750	2930	2942	2963	rBV	235438	382552	52.04%	6.594%
83	10.946	3000	3003	3005	rVB2	215	122	0.02%	0.002%
84	11.068	3037	3041	3045	rBV	338	348	0.05%	0.006%
85	11.283	3105	3108	3111	rBV	280	206	0.03%	0.004%
86	11.447	3157	3159	3161	rBV	222	129	0.02%	0.002%
87	11.515	3176	3180	3184	rVB2	296	235	0.03%	0.004%
88	11.537	3184	3187	3189	rBV	252	165	0.02%	0.003%
89	11.586	3197	3202	3205	rBV2	226	230	0.03%	0.004%
90	11.608	3205	3209	3210	rBV	238	178	0.02%	0.003%
91	11.808	3259	3271	3295	rBV	360516	580049	78.91%	9.998%
92	12.062	3347	3350	3351	rBV	284	124	0.02%	0.002%
93	12.187	3377	3389	3410	rBV	276637	461506	62.78%	7.955%
94	12.640	3527	3530	3532	rBV	339	229	0.03%	0.004%
95	12.808	3578	3582	3583	rBV2	328	234	0.03%	0.004%
96	12.840	3589	3592	3594	rBV2	254	149	0.02%	0.003%
97	13.036	3650	3653	3655	rBV	237	171	0.02%	0.003%
98	13.367	3753	3756	3757	rBV	242	130	0.02%	0.002%
99	13.412	3767	3770	3774	rBV2	336	297	0.04%	0.005%
100	14.090	3973	3981	3998	rBV2	11439	22668	3.08%	0.391%




Sum of corrected areas: 5801776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060217.D
Acq On : 26 Jul 2024 09:44
Operator : MD/SY
Sample : P3260-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

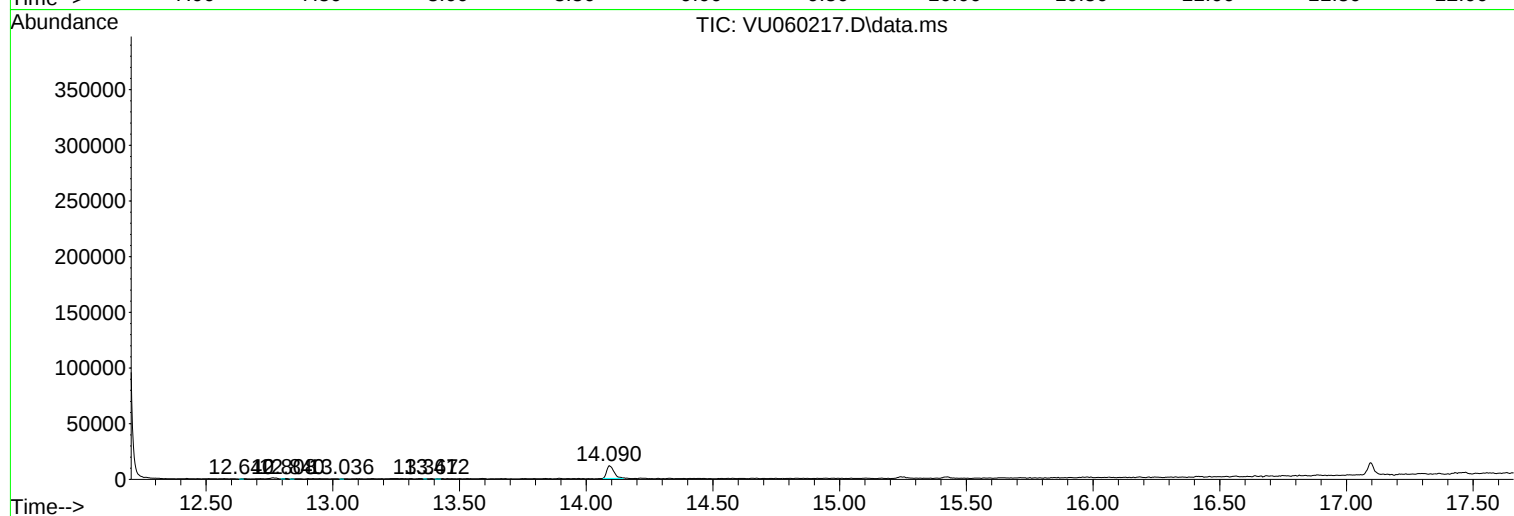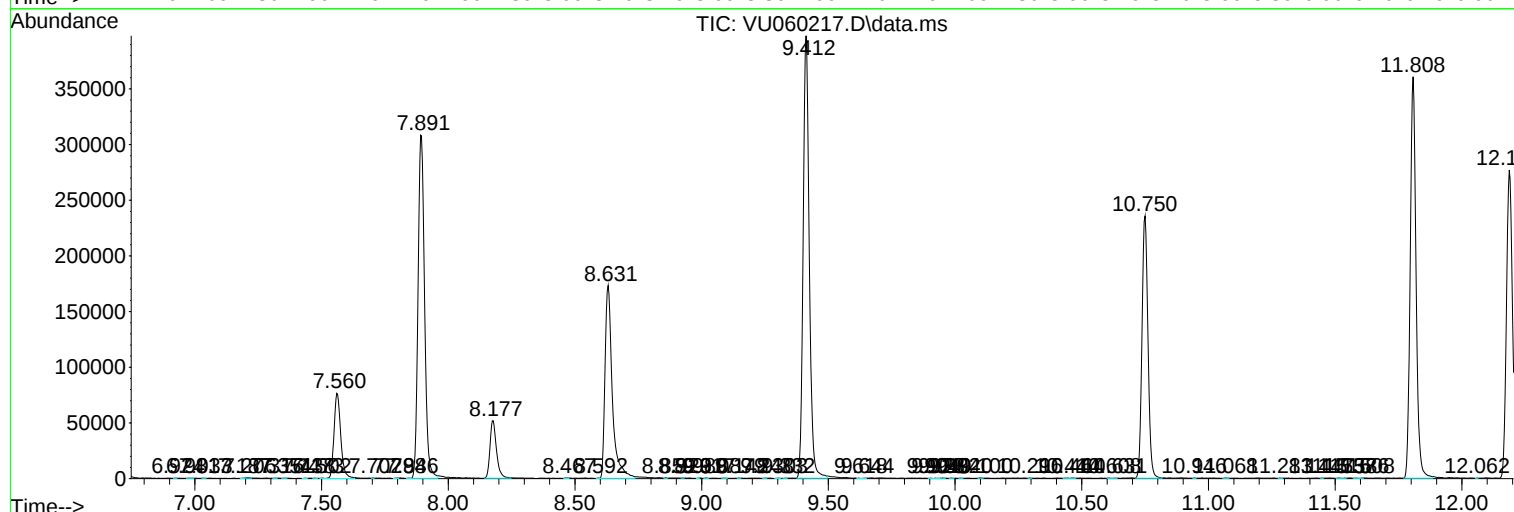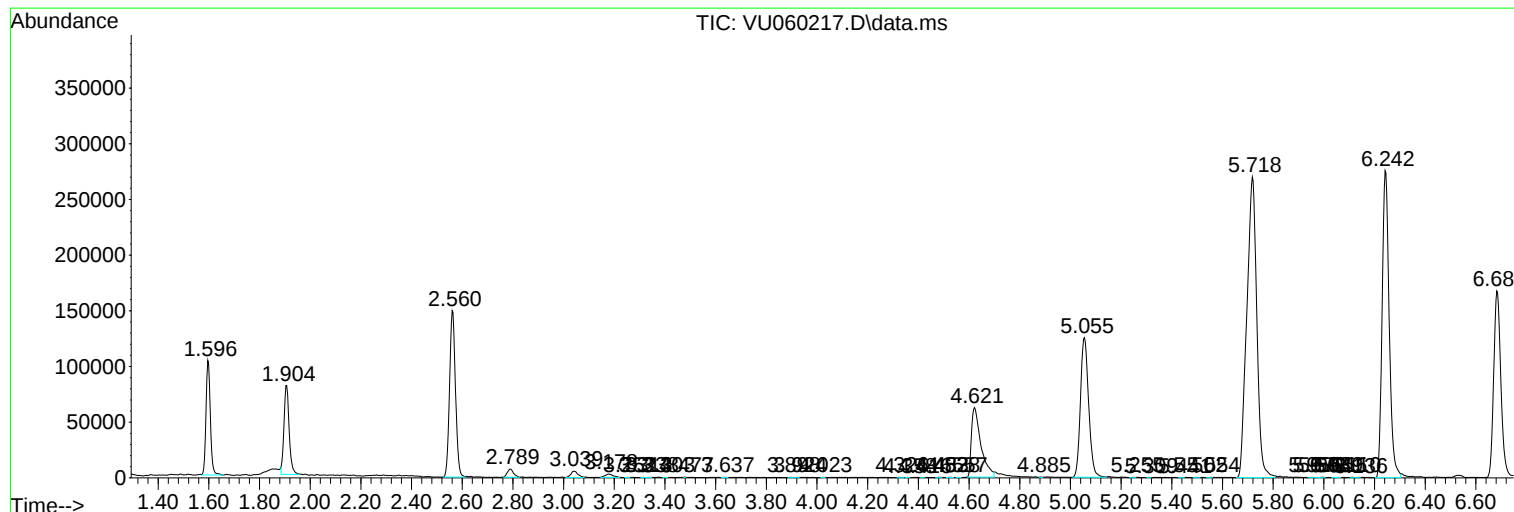

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060217.D
Acq On : 26 Jul 2024 09:44
Operator : MD/SY
Sample : P3260-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060217.D
Acq On : 26 Jul 2024 09:44
Operator : MD/SY
Sample : P3260-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------