

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060218.D
 Acq On : 26 Jul 2024 10:08
 Operator : MD/SY
 Sample : P3260-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	112	rVB	106328	124283	15.99%	2.056%
2	1.904	184	191	216	rVB	78580	113949	14.66%	1.885%
3	2.560	383	395	412	rBV	154504	255191	32.82%	4.221%
4	2.679	429	432	436	rBV2	287	211	0.03%	0.003%
5	2.721	442	445	446	rBV	251	156	0.02%	0.003%
6	2.789	458	466	479	rVB	5172	9369	1.21%	0.155%
7	2.869	490	491	495	rBV2	293	183	0.02%	0.003%
8	3.046	537	546	556	rVB2	2607	4474	0.58%	0.074%
9	3.174	578	586	595	rBV2	1373	2683	0.35%	0.044%
10	3.239	603	606	611	rBV2	208	219	0.03%	0.004%
11	3.493	682	685	690	rBV2	264	273	0.04%	0.005%
12	3.551	700	703	709	rBV2	166	194	0.02%	0.003%
13	3.686	740	745	748	rBV	333	344	0.04%	0.006%
14	3.907	812	814	818	rVB	270	175	0.02%	0.003%
15	3.940	821	824	826	rBV	262	190	0.02%	0.003%
16	4.100	871	874	880	rBV	218	269	0.03%	0.004%
17	4.194	900	903	909	rVB	321	324	0.04%	0.005%
18	4.239	914	917	918	rBV2	165	109	0.01%	0.002%
19	4.329	942	945	949	rVB2	163	117	0.02%	0.002%
20	4.457	983	985	990	rBV	193	121	0.02%	0.002%
21	4.618	1026	1035	1074	rBV2	68648	186032	23.93%	3.077%
22	5.055	1155	1171	1196	rBV	135474	302682	38.93%	5.007%
23	5.187	1209	1212	1214	rBV2	569	356	0.05%	0.006%
24	5.268	1235	1237	1240	rVB2	300	146	0.02%	0.002%
25	5.296	1243	1246	1248	rBV	164	126	0.02%	0.002%
26	5.332	1253	1257	1258	rBV	181	138	0.02%	0.002%
27	5.406	1276	1280	1281	rBV2	201	139	0.02%	0.002%
28	5.451	1291	1294	1296	rBV	295	219	0.03%	0.004%
29	5.502	1306	1310	1312	rBV	144	135	0.02%	0.002%
30	5.718	1358	1377	1413	rVV2	288044	777460	100.00%	12.860%
31	5.904	1433	1435	1437	rBV2	311	163	0.02%	0.003%
32	6.007	1464	1467	1469	rBV2	199	139	0.02%	0.002%
33	6.075	1485	1488	1495	rVB3	284	328	0.04%	0.005%
34	6.107	1495	1498	1499	rBV2	207	143	0.02%	0.002%
35	6.155	1510	1513	1515	rBV	275	218	0.03%	0.004%
36	6.197	1523	1526	1528	rBV	172	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060218.D
 Acq On : 26 Jul 2024 10:08
 Operator : MD/SY
 Sample : P3260-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.242	1528	1540	1559	rBV	275986	535092	68.83%	8.851%
38	6.528	1622	1629	1631	rBV5	1810	1986	0.26%	0.033%
39	6.621	1655	1658	1659	rBV	249	154	0.02%	0.003%
40	6.682	1664	1677	1706	rBV	175893	348943	44.88%	5.772%
41	6.872	1732	1736	1741	rBV2	132	139	0.02%	0.002%
42	6.920	1748	1751	1754	rBV2	181	127	0.02%	0.002%
43	6.972	1762	1767	1771	rBV2	256	246	0.03%	0.004%
44	6.994	1771	1774	1775	rBV	227	150	0.02%	0.002%
45	7.068	1787	1797	1800	rBV2	288	455	0.06%	0.008%
46	7.132	1815	1817	1821	rVB2	209	155	0.02%	0.003%
47	7.155	1821	1824	1828	rBV2	213	168	0.02%	0.003%
48	7.303	1868	1870	1872	rVB	222	113	0.01%	0.002%
49	7.322	1872	1876	1880	rBV2	250	220	0.03%	0.004%
50	7.351	1880	1885	1890	rVB2	196	230	0.03%	0.004%
51	7.377	1890	1893	1894	rBV	183	129	0.02%	0.002%
52	7.483	1923	1926	1929	rBV	272	200	0.03%	0.003%
53	7.560	1938	1950	1974	rBV	89144	162322	20.88%	2.685%
54	7.801	2021	2025	2028	rBV	406	384	0.05%	0.006%
55	7.891	2039	2053	2074	rBV	326211	574684	73.92%	9.506%
56	8.110	2119	2121	2126	rBV2	344	269	0.03%	0.004%
57	8.174	2131	2141	2162	rBV	59024	104998	13.51%	1.737%
58	8.332	2187	2190	2194	rBV2	204	169	0.02%	0.003%
59	8.428	2217	2220	2222	rBV	266	176	0.02%	0.003%
60	8.518	2245	2248	2251	rBV	207	163	0.02%	0.003%
61	8.554	2256	2259	2267	rVB2	454	502	0.06%	0.008%
62	8.628	2272	2282	2313	rBV	188237	369106	47.48%	6.105%
63	8.904	2365	2368	2369	rBV	293	176	0.02%	0.003%
64	8.994	2391	2396	2399	rBV2	256	317	0.04%	0.005%
65	9.058	2411	2416	2419	rBV2	238	277	0.04%	0.005%
66	9.097	2426	2428	2431	rBV	199	135	0.02%	0.002%
67	9.119	2432	2435	2439	rVV2	228	184	0.02%	0.003%
68	9.300	2484	2491	2493	rBV	268	266	0.03%	0.004%
69	9.364	2509	2511	2514	rBV	188	110	0.01%	0.002%
70	9.412	2514	2526	2553	rBV	391911	670802	86.28%	11.096%
71	9.640	2593	2597	2601	rBV2	261	315	0.04%	0.005%
72	9.673	2605	2607	2610	rBV	222	114	0.01%	0.002%
73	9.692	2610	2613	2615	rBV2	457	284	0.04%	0.005%
74	9.878	2668	2671	2672	rBV	221	147	0.02%	0.002%
75	9.962	2693	2697	2699	rBV2	200	128	0.02%	0.002%
76	10.033	2716	2719	2721	rBV2	209	153	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
 Data File : VU060218.D
 Acq On : 26 Jul 2024 10:08
 Operator : MD/SY
 Sample : P3260-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.235	2780	2782	2786	rVB	230	109	0.01%	0.002%
78	10.254	2786	2788	2790	rBV	163	113	0.01%	0.002%
79	10.309	2800	2805	2809	rBV2	310	408	0.05%	0.007%
80	10.370	2821	2824	2826	rBV	261	153	0.02%	0.003%
81	10.428	2838	2842	2845	rVB2	241	196	0.03%	0.003%
82	10.444	2845	2847	2851	rBV	186	176	0.02%	0.003%
83	10.547	2876	2879	2882	rBV2	183	130	0.02%	0.002%
84	10.592	2889	2893	2896	rBV2	320	328	0.04%	0.005%
85	10.750	2929	2942	2961	rBV	251951	410652	52.82%	6.793%
86	10.959	3004	3007	3010	rBV2	203	193	0.02%	0.003%
87	11.039	3030	3032	3036	rVB2	333	192	0.02%	0.003%
88	11.071	3039	3042	3046	rBV2	350	313	0.04%	0.005%
89	11.164	3069	3071	3074	rBV2	193	145	0.02%	0.002%
90	11.261	3098	3101	3102	rBV	222	130	0.02%	0.002%
91	11.428	3148	3153	3159	rVB2	338	259	0.03%	0.004%
92	11.457	3159	3162	3164	rBV2	222	185	0.02%	0.003%
93	11.666	3224	3227	3231	rBV	241	196	0.03%	0.003%
94	11.727	3243	3246	3248	rBV	206	148	0.02%	0.002%
95	11.807	3258	3271	3290	rBV	345524	573339	73.75%	9.484%
96	12.187	3377	3389	3412	rBV	287634	483045	62.13%	7.990%
97	12.373	3443	3447	3450	rBV	316	306	0.04%	0.005%
98	12.512	3487	3490	3493	rBV2	279	218	0.03%	0.004%
99	13.624	3833	3836	3839	rBV	189	148	0.02%	0.002%
100	14.094	3972	3982	4000	rBV	8592	18464	2.37%	0.305%




Sum of corrected areas: 6045629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060218.D
Acq On : 26 Jul 2024 10:08
Operator : MD/SY
Sample : P3260-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

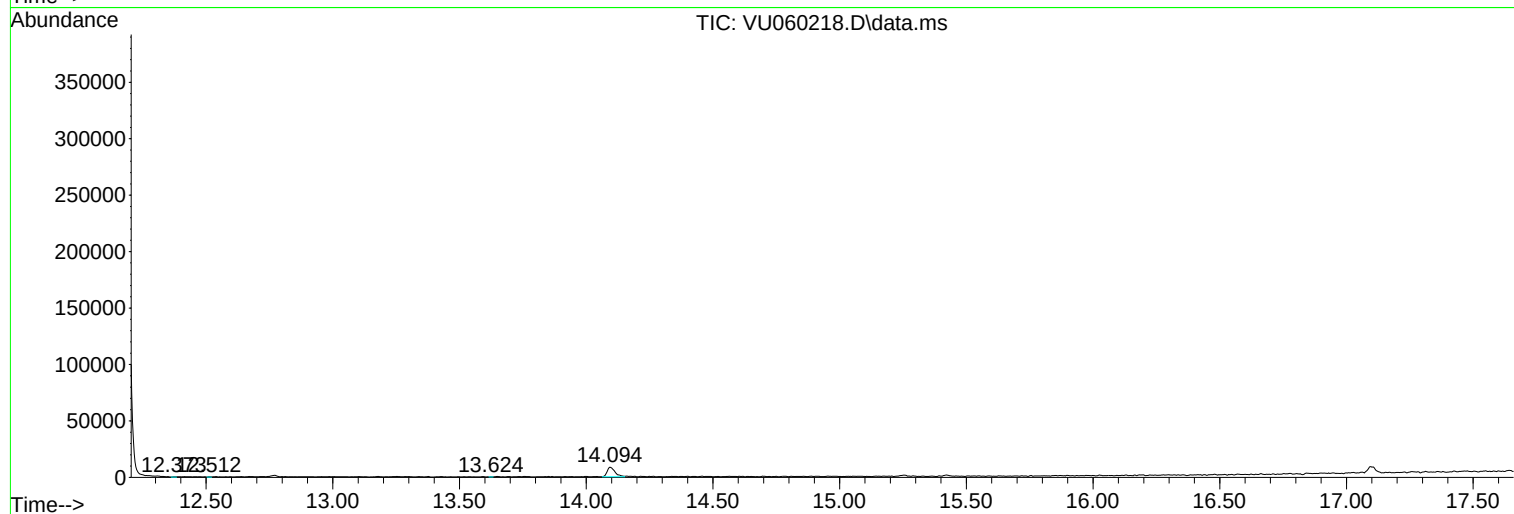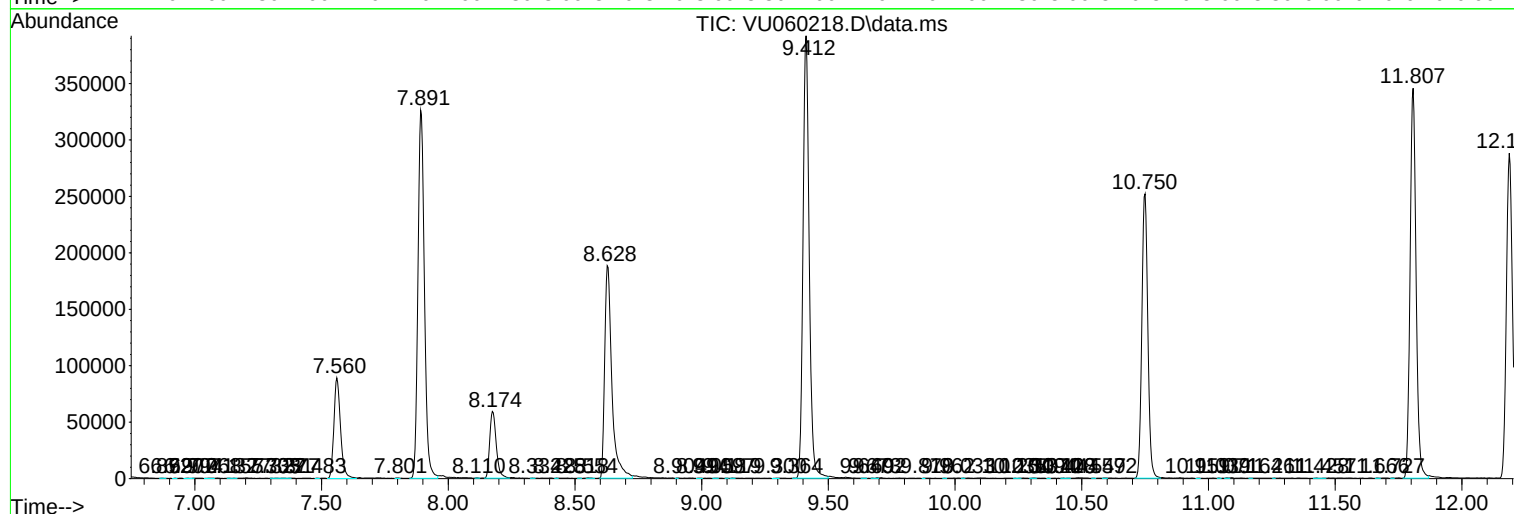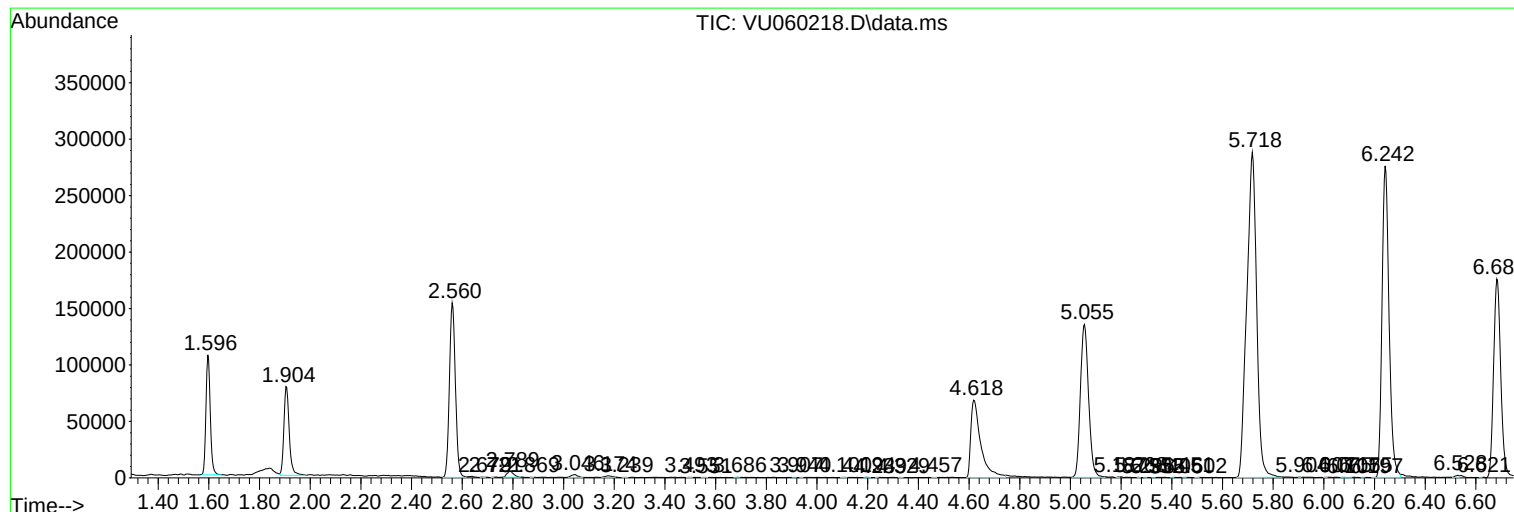

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060218.D
Acq On : 26 Jul 2024 10:08
Operator : MD/SY
Sample : P3260-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060218.D
Acq On : 26 Jul 2024 10:08
Operator : MD/SY
Sample : P3260-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc