


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072524\
Data File : VU060168.D
Acq On : 25 Jul 2024 12:17
Operator : MD/SY
Sample : BFB074
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB074

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Fri Jul 26 04:34:35 2024

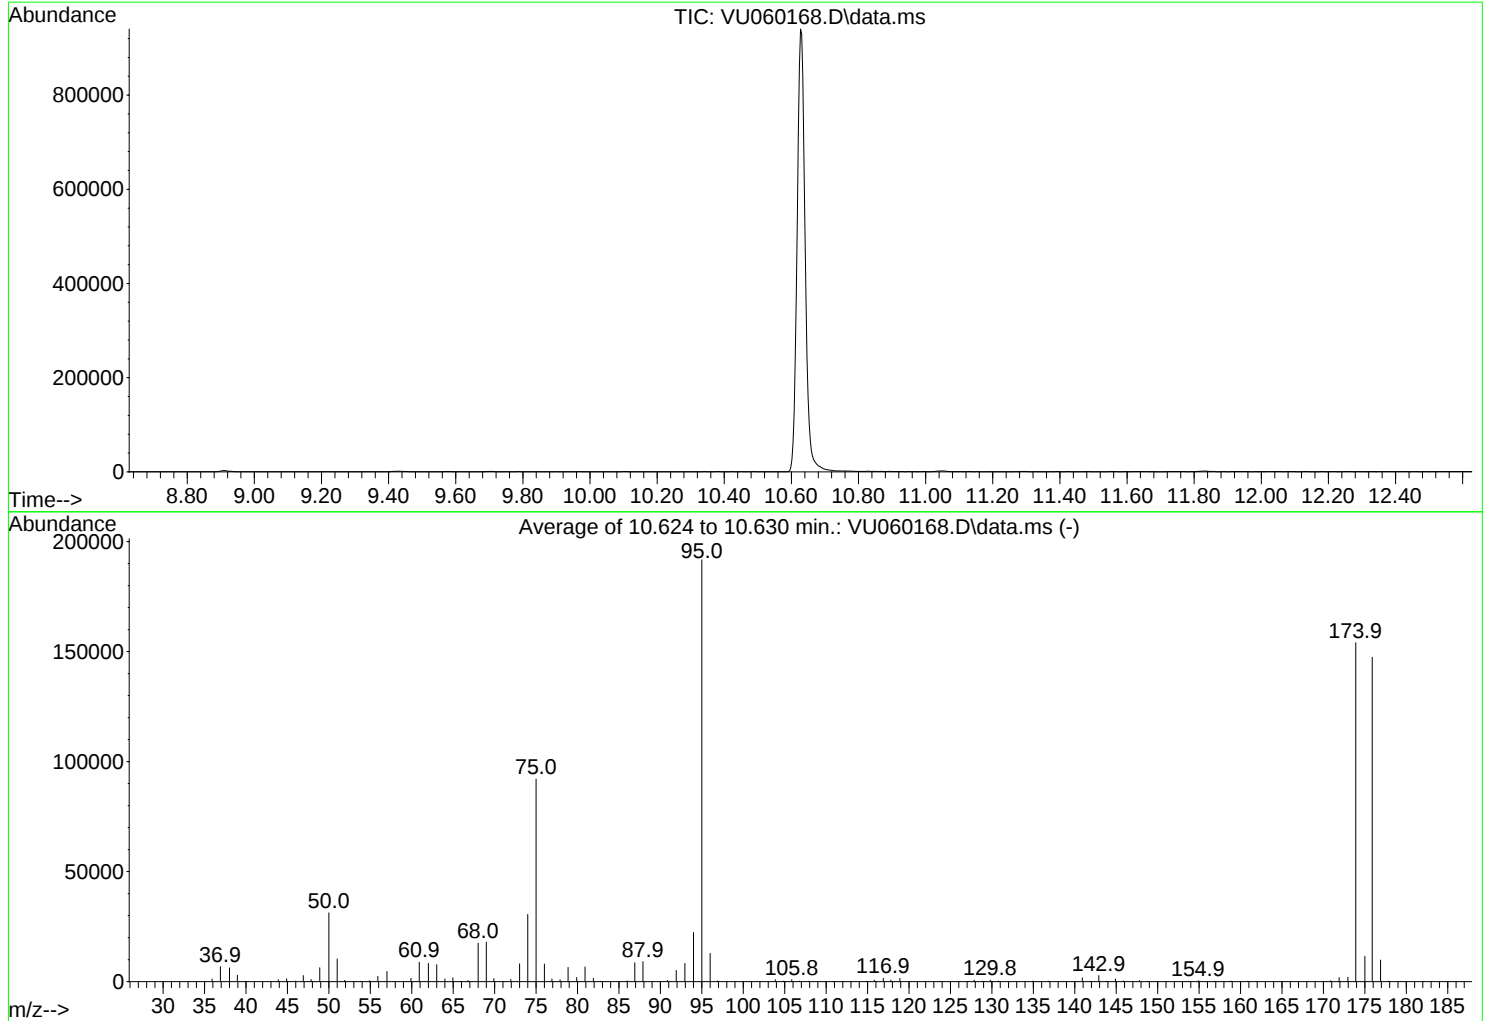

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	31240	PASS
75	95	30	80	48.0	92043	PASS
95	95	100	100	100.0	191701	PASS
96	95	5	9	6.7	12799	PASS
173	174	0.00	2	1.3	2056	PASS
174	95	50	120	80.3	153984	PASS
175	174	5	9	7.5	11579	PASS
176	174	95	101	95.7	147371	PASS
177	176	5	9	6.7	9855	PASS

m/z	Abundance
43.80	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	1094.0
36.90	6400.0
38.00	6034.0
38.90	2813.0
40.00	274.0
43.90	1054.0
44.90	1221.0
46.00	267.0
46.90	2585.0
47.90	985.0
48.90	6026.0
50.00	29760.0
51.00	10111.0
51.90	551.0
52.90	148.0
53.80	133.0
54.90	490.0
55.90	2415.0
57.00	4680.0
57.80	184.0
59.90	1507.0
60.90	8488.0
62.00	7976.0
63.00	7552.0
64.00	1270.0
64.90	1776.0
65.90	171.0
66.80	466.0
68.00	16520.0
69.00	17048.0
69.90	1410.0
72.00	943.0
73.00	7690.0
74.00	29008.0
75.00	88096.0
76.00	7775.0
76.90	1127.0
77.90	755.0
78.80	6367.0
79.90	1684.0
80.90	6763.0
81.90	1391.0
82.80	127.0
86.00	289.0
86.90	8229.0
87.90	8538.0
90.90	469.0
91.90	4910.0
92.90	7928.0
94.00	21624.0
95.00	182912.0
96.00	12474.0
96.90	452.0
103.90	802.0
104.80	265.0
105.90	857.0
106.80	211.0
107.90	204.0
110.80	107.0
111.90	117.0
113.00	122.0
114.90	168.0
115.80	698.0
116.90	1498.0
117.80	688.0
118.90	1365.0
127.90	680.0
128.80	193.0
129.80	758.0
130.80	310.0
134.90	257.0
136.90	259.0
140.90	1655.0
142.00	154.0
142.90	2786.0
143.80	204.0
144.90	1324.0
145.80	345.0
147.80	528.0
148.80	111.0
150.00	102.0
153.70	137.0
154.90	408.0
156.90	213.0
158.90	273.0
160.90	177.0
170.90	529.0
171.90	1734.0
173.00	1937.0
173.90	142528.0
175.00	10850.0
175.90	137088.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

176.909086.0

177.90297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	1266.0
36.90	7073.0
38.00	6559.0
38.90	3079.0
39.90	256.0
44.00	1195.0
44.90	1334.0
45.90	329.0
46.90	2845.0
47.90	983.0
48.90	6506.0
50.00	32288.0
51.00	10657.0
51.90	615.0
53.00	169.0
53.80	114.0
54.90	488.0
55.90	2468.0
57.00	4828.0
57.90	133.0
59.90	1608.0
60.90	9112.0
62.00	8564.0
63.00	8050.0
64.00	1260.0
65.00	1846.0
65.90	151.0
66.80	523.0
68.00	18064.0
69.00	18432.0
69.90	1448.0
71.90	973.0
73.00	8302.0
74.00	31352.0
75.00	94992.0
76.00	8305.0
76.90	1275.0
77.90	790.0
78.80	6689.0
79.90	1950.0
80.90	6852.0
81.90	1499.0
82.80	155.0
86.00	396.0
86.90	8789.0
87.90	9510.0
90.80	573.0
91.90	5184.0
93.00	8662.0
94.00	23096.0
95.00	198144.0
96.00	13335.0
96.90	408.0
103.80	866.0
104.80	311.0
105.80	895.0
106.80	242.0
107.90	201.0
110.80	149.0
113.00	163.0
114.80	174.0
115.80	759.0
116.90	1552.0
117.80	730.0
118.90	1522.0
123.80	122.0
125.80	121.0
127.80	774.0
128.80	242.0
129.80	771.0
130.80	334.0
135.00	298.0
136.90	279.0
140.90	1808.0
141.90	254.0
142.90	2843.0
143.80	239.0
144.90	1346.0
145.90	395.0
147.80	554.0
148.80	129.0
149.90	135.0
153.80	134.0
154.90	481.0
156.90	250.0
158.90	276.0
160.90	165.0
170.90	494.0
171.90	1863.0
173.00	2140.0
173.90	158272.0
175.00	11958.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

175.90152000.0

176.9010192.0

177.90287.0

Instrument :
MSVOA_U

ClientSampleId :
BFB074

m/z	Abundance
35.90	1302.0
36.90	6992.0
38.00	6262.0
39.00	2958.0
39.80	252.0
44.00	1289.0
44.90	1344.0
45.90	332.0
46.90	2857.0
47.80	964.0
48.90	6537.0
50.00	31672.0
51.00	10328.0
51.90	530.0
52.90	165.0
54.90	426.0
55.90	2269.0
57.00	4493.0
59.90	1573.0
60.90	8801.0
62.00	8402.0
63.00	7622.0
64.00	1154.0
65.00	1715.0
65.90	117.0
66.80	542.0
68.00	17920.0
69.00	18344.0
69.90	1328.0
71.90	971.0
73.00	8177.0
74.00	31320.0
75.00	93040.0
76.00	7937.0
76.90	1248.0
77.90	773.0
78.90	6446.0
79.90	1994.0
80.90	6392.0
81.90	1419.0
82.80	165.0
86.00	405.0
86.90	8669.0
87.90	9268.0
90.80	662.0
91.90	5300.0
93.00	8377.0
94.00	22328.0
95.00	194048.0
96.00	12589.0
96.90	337.0
103.90	859.0
104.80	300.0
105.80	856.0
106.80	222.0
107.90	173.0
110.80	195.0
113.00	146.0
114.80	169.0
115.80	703.0
116.90	1437.0
117.80	693.0
118.90	1472.0
123.80	174.0
125.80	135.0
127.90	773.0
128.90	255.0
129.80	716.0
130.80	310.0
134.90	295.0
136.80	242.0
140.90	1786.0
141.90	305.0
142.90	2628.0
143.80	210.0
144.90	1121.0
145.90	368.0
147.80	572.0
148.80	109.0
149.90	174.0
153.80	124.0
154.90	540.0
156.90	326.0
158.80	270.0
160.80	172.0
170.90	379.0
171.90	1968.0
172.90	2090.0
173.90	161152.0
175.00	11930.0
175.90	153024.0
176.90	10288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

177.90

271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074