

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
 Data File : VU060315.D
 Acq On : 06 Aug 2024 11:38
 Operator : MD/SY
 Sample : VU0806WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0806WBL01

Quant Time: Aug 07 06:57:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 06 11:07:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	29846	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	7832	0.770	ug/l	0.00
Spiked Amount 1.000			Recovery	=	77.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	9194	0.832	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060315.D
Acq On : 06 Aug 2024 11:38
Operator : MD/SY
Sample : VU0806WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0806WBL01

Quant Time: Aug 07 06:57:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 06 11:07:28 2024
Response via : Initial Calibration




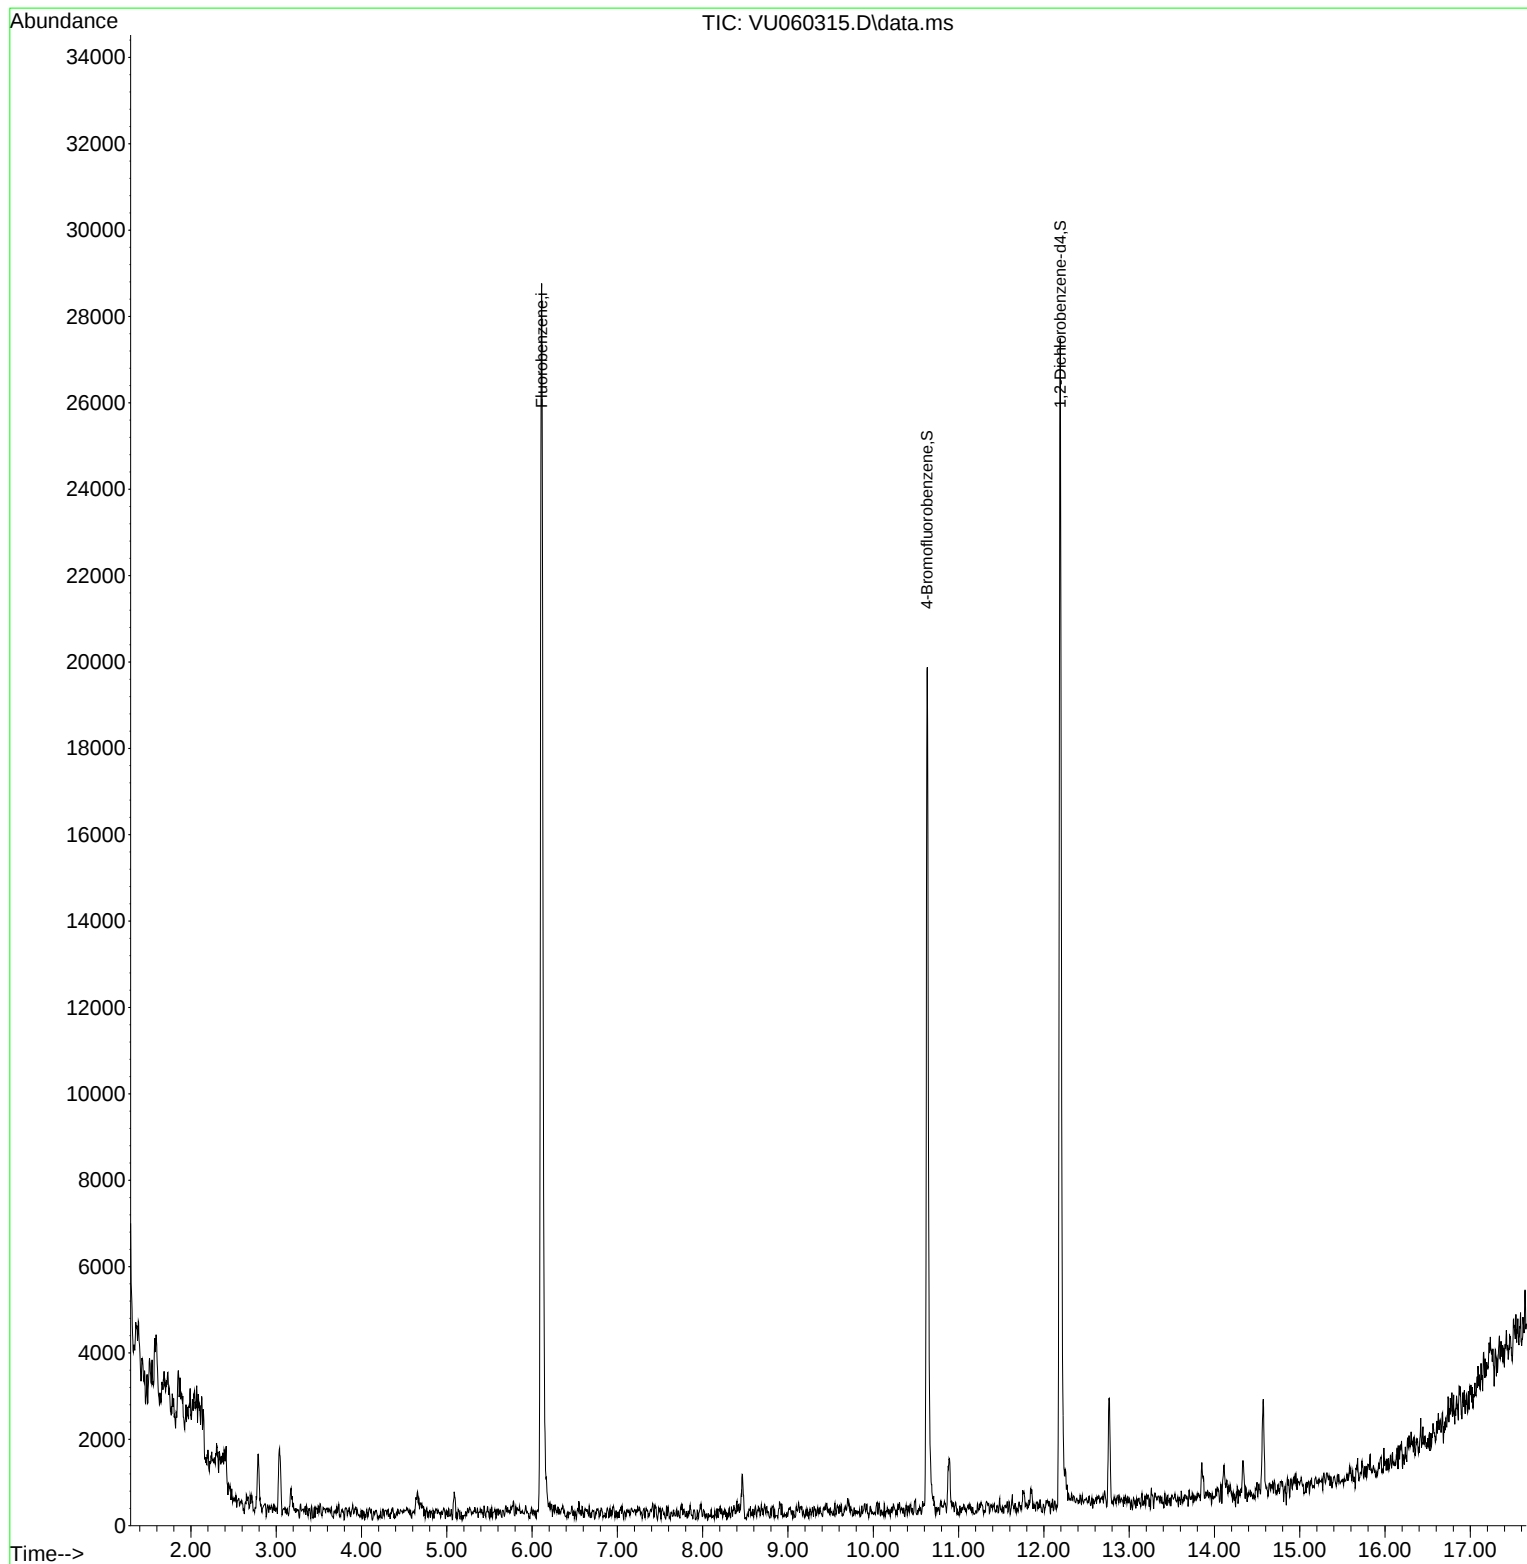


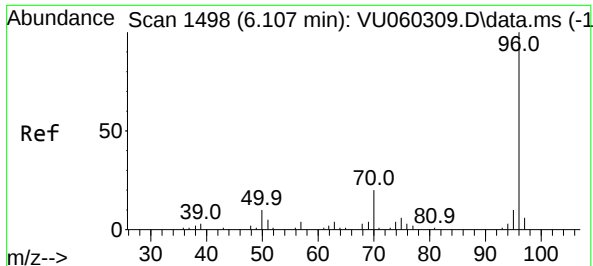

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU060315.D
Acq: 06 Aug 2024 11:38




Instrument :
MSVOA_U
ClientSampleId :
VU0806WBL01


Tgt Ion: 96	Resp: 29846
Ion Ratio	Lower Upper
96 100	
70 19.1	17.2 25.8
95 9.5	7.9 11.9
97 6.2	0.0 0.0

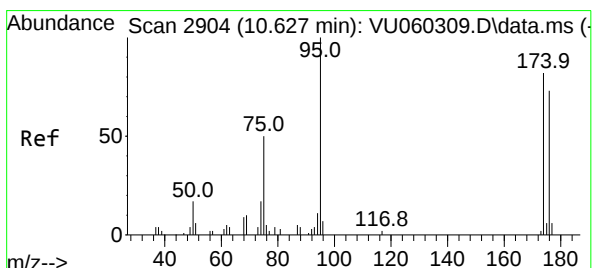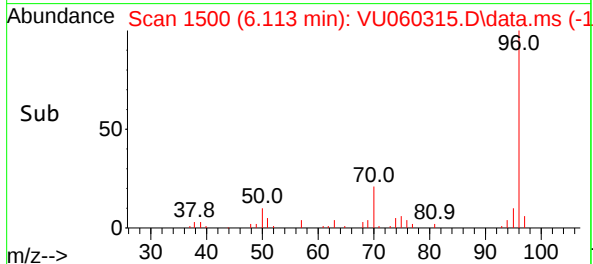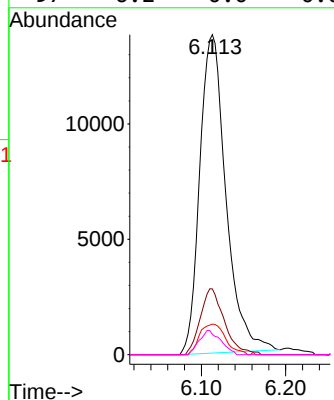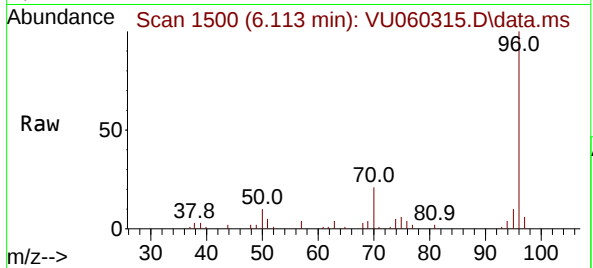

#57
4-Bromofluorobenzene
Concen: 0.770 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU060315.D
Acq: 06 Aug 2024 11:38


Tgt Ion: 95	Resp: 7832
Ion Ratio	Lower Upper
95 100	
174 84.9	65.6 98.4
176 81.6	60.4 90.6

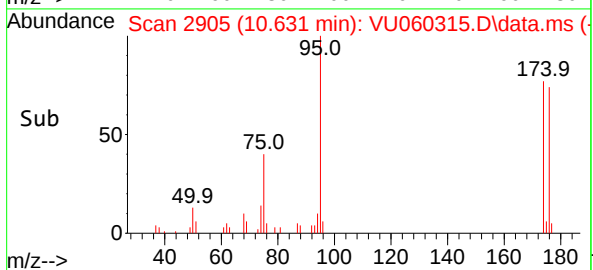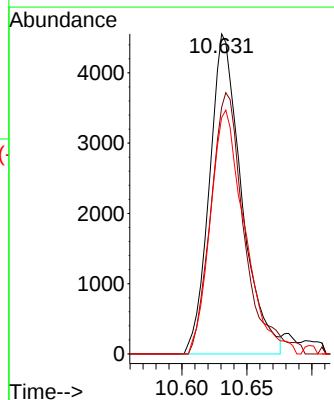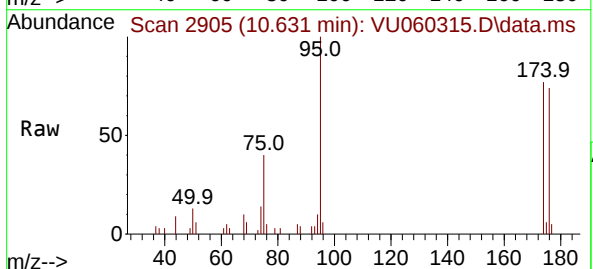

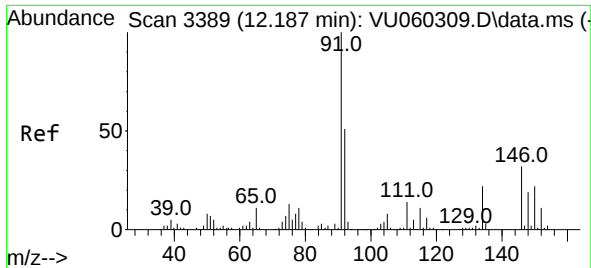

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.832 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VU060315.D
 Acq: 06 Aug 2024 11:38

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0806WBL01

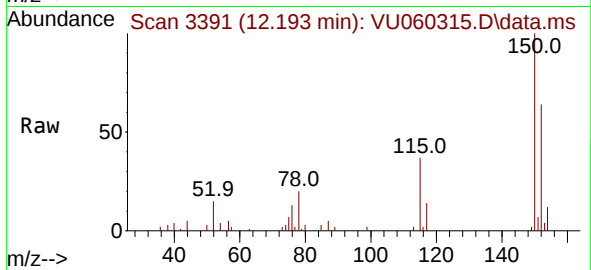

Tgt Ion:	152	Resp:	9194
Ion	Ratio	Lower	Upper
152	100		
115	58.6	0.0	325.2
150	154.8	0.0	684.2

