

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
 Data File : VU060315.D
 Acq On : 06 Aug 2024 11:38
 Operator : MD/SY
 Sample : VU0806WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0806WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.853	170	175	178	rBV4	1055	1167	2.00%	0.694%
2	2.087	245	248	252	rVV3	717	667	1.14%	0.397%
3	2.126	256	260	263	rVB2	768	651	1.12%	0.387%
4	2.412	346	349	356	rVB3	1127	1055	1.81%	0.628%
5	2.788	460	466	475	rVB3	1183	1697	2.91%	1.010%
6	2.869	480	491	495	rVB2	310	672	1.15%	0.400%
7	3.039	536	544	553	rVB5	1553	2855	4.89%	1.699%
8	3.174	577	586	589	rBV3	633	844	1.45%	0.502%
9	5.087	1174	1181	1188	rBV4	651	981	1.68%	0.584%
10	6.113	1488	1500	1524	rBV	28414	58359	100.00%	34.722%
11	8.463	2229	2231	2240	rVB3	1027	1220	2.09%	0.726%
12	10.634	2896	2906	2928	rBV2	19417	33324	57.10%	19.827%
13	10.878	2976	2982	2983	rBV	1077	826	1.42%	0.491%
14	11.631	3208	3216	3222	rBV3	460	589	1.01%	0.350%
15	12.190	3380	3390	3407	rBV	27060	47943	82.15%	28.525%
16	12.766	3561	3569	3580	rBV	2511	4014	6.88%	2.388%
17	13.852	3902	3907	3912	rBV3	894	1161	1.99%	0.691%
18	14.113	3980	3988	3994	rBV3	892	1611	2.76%	0.959%
19	14.335	4052	4057	4065	rVV3	883	1276	2.19%	0.759%
20	14.573	4121	4131	4142	rVV3	2199	3785	6.49%	2.252%
21	14.855	4215	4219	4222	rBV	645	647	1.11%	0.385%
22	16.418	4700	4705	4708	rBV3	809	605	1.04%	0.360%
23	16.868	4842	4845	4848	rBV3	794	699	1.20%	0.416%
24	16.913	4855	4859	4862	rBV3	613	593	1.02%	0.353%
25	17.158	4931	4935	4938	rBV4	894	834	1.43%	0.496%




Sum of corrected areas: 168075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060315.D
Acq On : 06 Aug 2024 11:38
Operator : MD/SY
Sample : VU0806WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0806WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

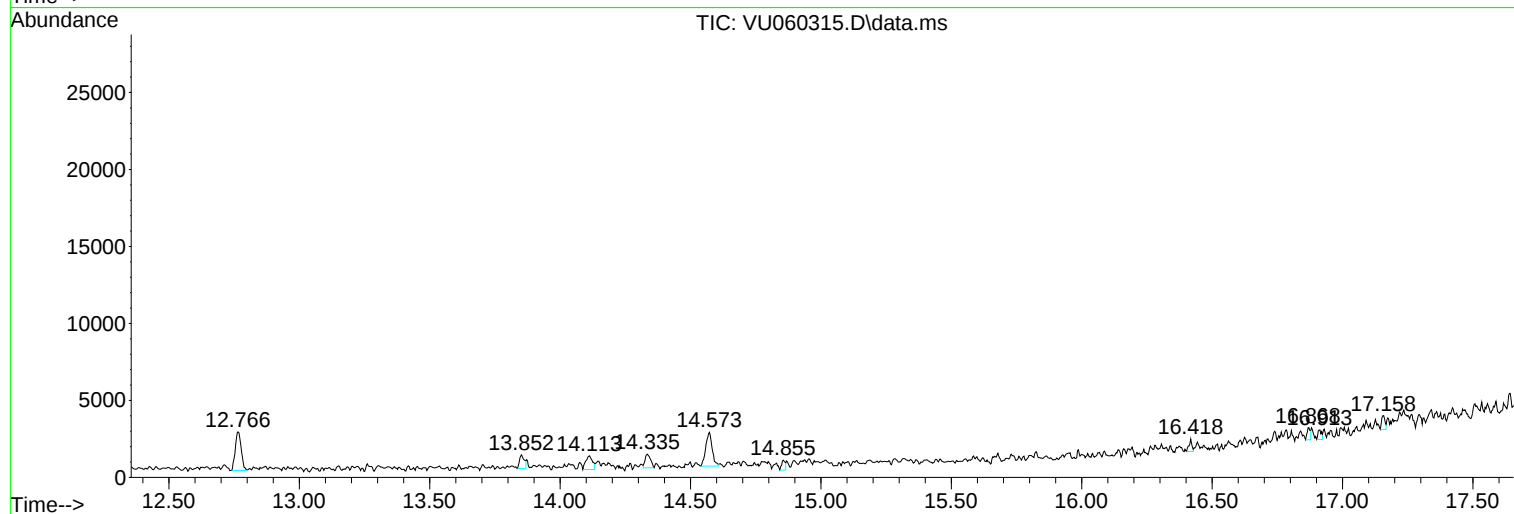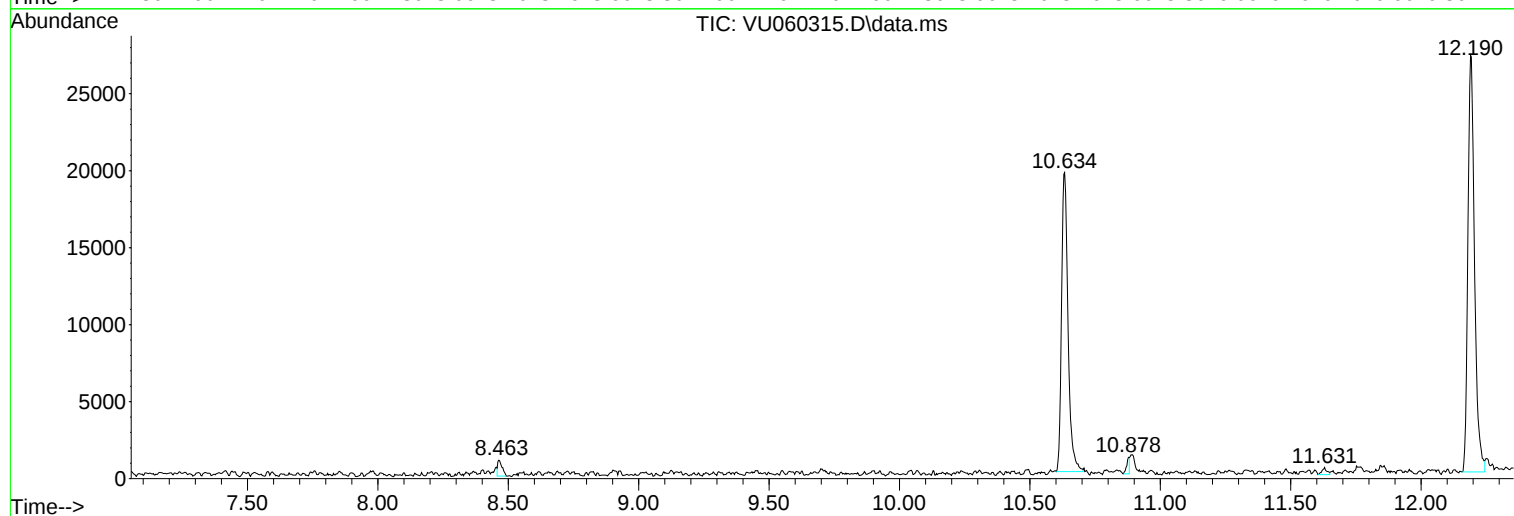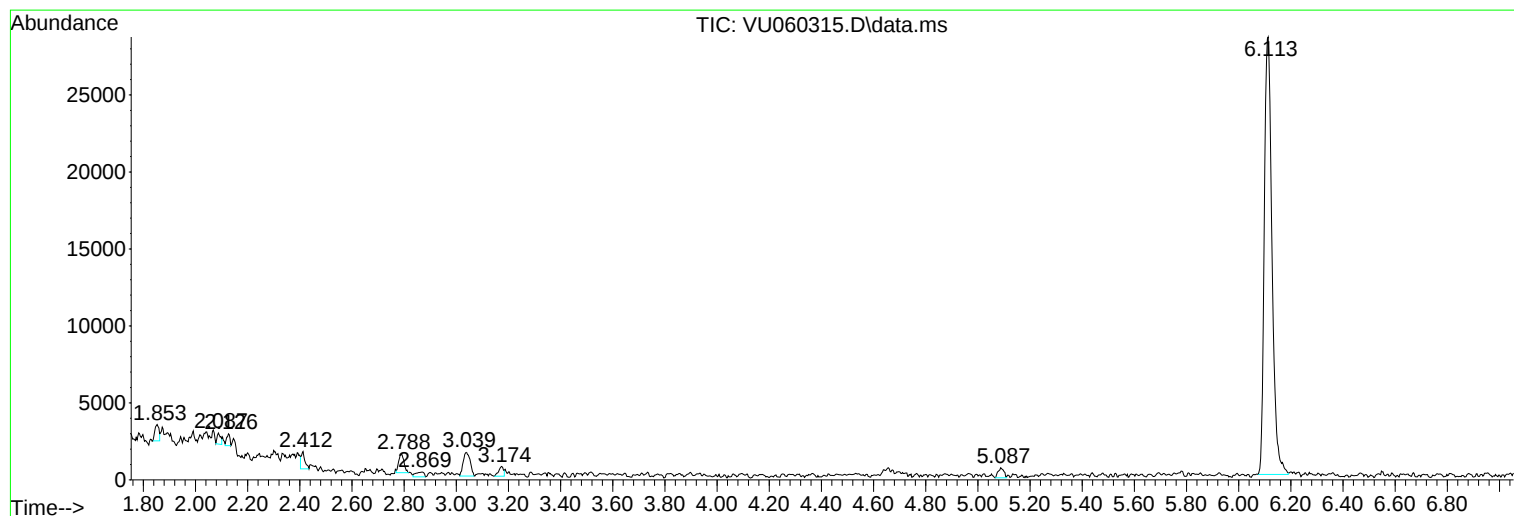

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060315.D
Acq On : 06 Aug 2024 11:38
Operator : MD/SY
Sample : VU0806WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0806WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060315.D
Acq On : 06 Aug 2024 11:38
Operator : MD/SY
Sample : VU0806WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0806WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------