

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
 Data File : VU060320.D
 Acq On : 06 Aug 2024 14:07
 Operator : MD/SY
 Sample : P3204-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.020	222	227	231	rBV4	625	749	1.23%	0.222%
2	2.464	362	365	374	rBV2	417	618	1.02%	0.183%
3	2.647	415	422	426	rVB3	561	666	1.10%	0.198%
4	2.788	458	466	472	rVV3	770	1225	2.02%	0.363%
5	3.039	533	544	560	rVB4	11401	22506	37.09%	6.678%
6	3.181	576	588	602	rBV2	5257	11441	18.85%	3.395%
7	4.634	1029	1040	1057	rBV2	8092	23674	39.01%	7.024%
8	6.113	1488	1500	1519	rBV	30739	60686	100.00%	18.006%
9	8.463	2226	2231	2242	rVB2	1394	1998	3.29%	0.593%
10	8.920	2361	2373	2390	rBV2	21069	41316	68.08%	12.259%
11	9.579	2573	2578	2584	rVB3	588	696	1.15%	0.207%
12	10.634	2893	2906	2919	rBV2	22477	38424	63.32%	11.401%
13	10.820	2950	2964	2976	rBV2	32596	53715	88.51%	15.937%
14	10.888	2980	2985	2995	rVB3	1338	2113	3.48%	0.627%
15	11.756	3249	3255	3261	rBV3	544	809	1.33%	0.240%
16	11.843	3277	3282	3291	rVB3	1013	1202	1.98%	0.357%
17	12.193	3379	3391	3417	rBV	31229	56175	92.57%	16.667%
18	12.769	3561	3570	3578	rVB2	2737	4185	6.90%	1.242%
19	13.000	3635	3642	3650	rBV5	2097	3410	5.62%	1.012%
20	13.855	3902	3908	3918	rBV4	1370	1916	3.16%	0.568%
21	14.100	3978	3984	3986	rBV2	672	674	1.11%	0.200%
22	14.338	4047	4058	4068	rVV3	1319	2482	4.09%	0.736%
23	14.572	4121	4131	4141	rBV2	3342	5691	9.38%	1.689%
24	16.186	4628	4633	4635	rBV3	621	665	1.10%	0.197%


Sum of corrected areas: 337036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060320.D
Acq On : 06 Aug 2024 14:07
Operator : MD/SY
Sample : P3204-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

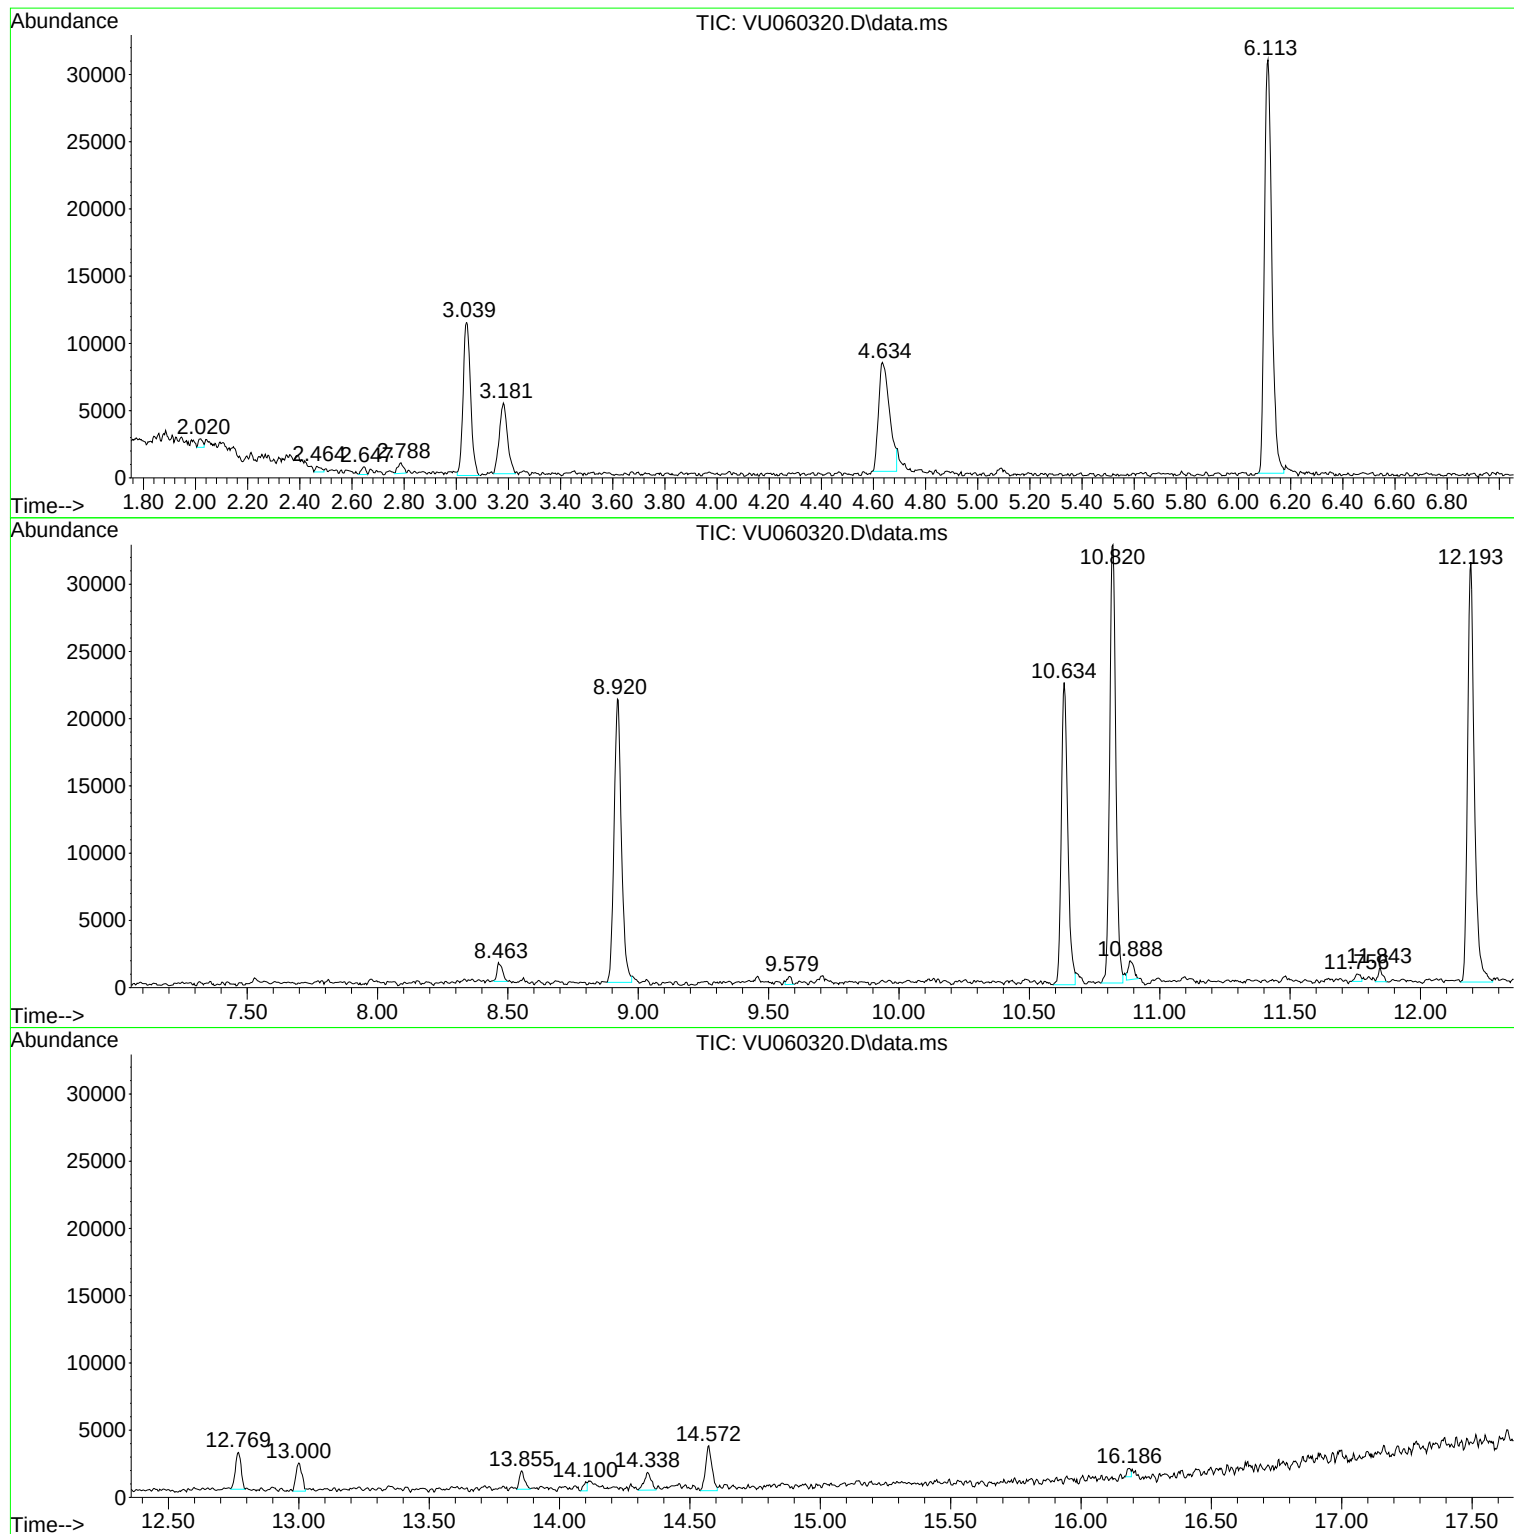

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060320.D
Acq On : 06 Aug 2024 14:07
Operator : MD/SY
Sample : P3204-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060320.D
Acq On : 06 Aug 2024 14:07
Operator : MD/SY
Sample : P3204-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------