

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
 Data File : VU060322.D
 Acq On : 06 Aug 2024 14:55
 Operator : MD/SY
 Sample : P3204-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.573	384	399	419	rBV	387262	635590	30.65%	4.660%
2	3.036	525	543	569	rBV	406807	788766	38.04%	5.784%
3	3.348	626	640	663	rBV	126702	256817	12.38%	1.883%
4	4.660	1026	1048	1084	rBV2	159158	390936	18.85%	2.867%
5	5.309	1234	1250	1269	rBV2	119742	268139	12.93%	1.966%
6	5.518	1296	1315	1337	rBV	111547	244931	11.81%	1.796%
7	5.772	1378	1394	1432	rBV2	254874	647931	31.24%	4.751%
8	6.110	1488	1499	1518	rBV	32371	65060	3.14%	0.477%
9	6.537	1620	1632	1653	rBV	66968	128362	6.19%	0.941%
10	6.785	1695	1709	1735	rBV	184284	357091	17.22%	2.618%
11	7.965	2061	2076	2111	rBV	714341	1240327	59.81%	9.095%
12	8.393	2196	2209	2230	rBV	320676	552731	26.65%	4.053%
13	8.547	2244	2257	2280	rBV	673347	1158962	55.89%	8.498%
14	9.441	2521	2535	2559	rBV	214199	364475	17.58%	2.673%
15	9.566	2559	2574	2600	rVV	1296121	2073782	100.00%	15.206%
16	9.688	2600	2612	2634	rVB	195087	334799	16.14%	2.455%
17	10.106	2723	2742	2778	rBV2	1172779	2071544	99.89%	15.190%
18	10.631	2894	2905	2925	rBV	31368	52681	2.54%	0.386%
19	11.830	3266	3278	3305	rBV	408702	662584	31.95%	4.858%
20	12.206	3377	3395	3419	rBV2	358779	664896	32.06%	4.875%
21	13.833	3889	3901	3923	rBV	413360	677468	32.67%	4.968%




Sum of corrected areas: 13637872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060322.D
Acq On : 06 Aug 2024 14:55
Operator : MD/SY
Sample : P3204-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

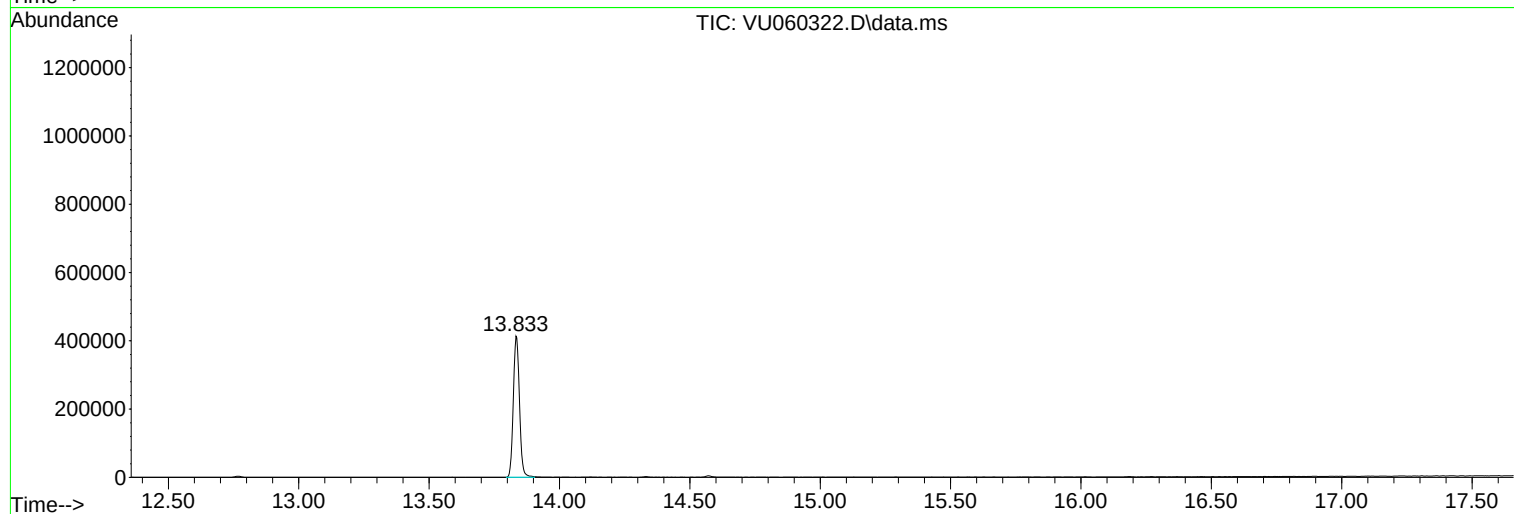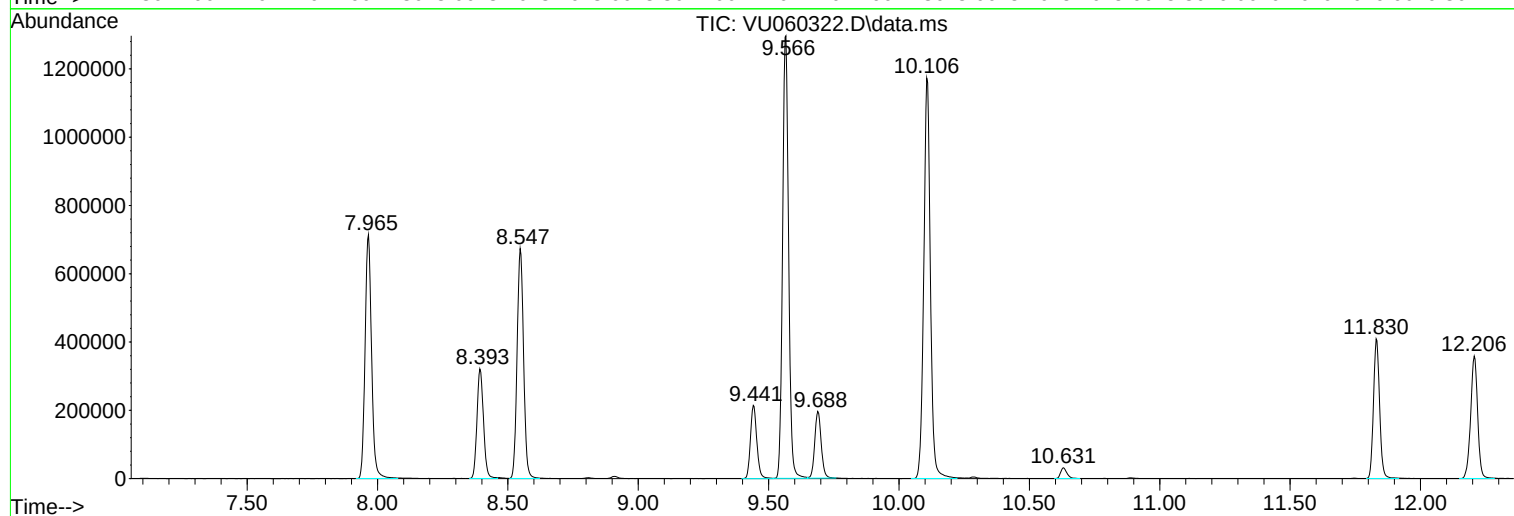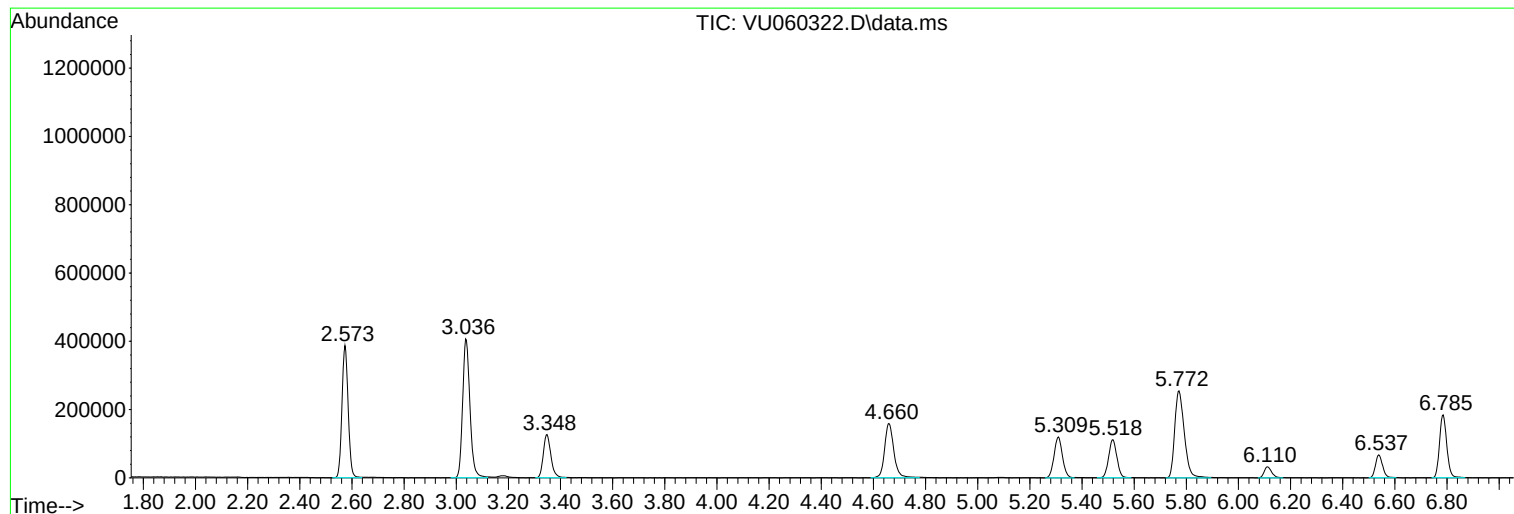

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060322.D
Acq On : 06 Aug 2024 14:55
Operator : MD/SY
Sample : P3204-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060322.D
Acq On : 06 Aug 2024 14:55
Operator : MD/SY
Sample : P3204-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------