

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
 Data File : VU060323.D
 Acq On : 06 Aug 2024 15:25
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.830	163	168	170	rBV2	943	793	1.38%	0.337%
2	2.068	240	242	248	rVB2	699	588	1.02%	0.250%
3	2.142	261	265	271	rVB4	1451	1685	2.93%	0.717%
4	2.409	345	348	358	rVB3	1120	1160	2.02%	0.494%
5	2.573	392	399	408	rVB4	1853	2992	5.21%	1.273%
6	3.039	535	544	555	rVB2	3155	5784	10.07%	2.461%
7	3.181	584	588	597	rVB3	541	780	1.36%	0.332%
8	3.358	641	643	650	rVB3	900	725	1.26%	0.309%
9	5.091	1173	1182	1190	rBV3	659	1095	1.91%	0.466%
10	5.782	1391	1397	1403	rBV	511	632	1.10%	0.269%
11	6.113	1487	1500	1518	rBV	28605	57430	100.00%	24.440%
12	6.550	1630	1636	1640	rBV4	721	849	1.48%	0.361%
13	8.402	2208	2212	2220	rVB5	827	829	1.44%	0.353%
14	8.467	2226	2232	2243	rVB	933	1655	2.88%	0.704%
15	8.550	2251	2258	2266	rBB4	3290	4993	8.69%	2.125%
16	8.820	2333	2342	2349	rBV4	554	957	1.67%	0.407%
17	9.457	2532	2540	2549	rVB3	1054	1710	2.98%	0.728%
18	9.573	2565	2576	2592	rVB3	4083	6786	11.82%	2.888%
19	9.698	2606	2615	2621	rBV3	886	1400	2.44%	0.596%
20	10.119	2736	2746	2760	rBV3	3516	7114	12.39%	3.027%
21	10.634	2896	2906	2919	rBV2	20792	35326	61.51%	15.034%
22	10.891	2978	2986	2997	rVB2	1218	2019	3.52%	0.859%
23	11.293	3104	3111	3116	rBV2	403	693	1.21%	0.295%
24	11.846	3273	3283	3293	rBV4	4567	7493	13.05%	3.189%
25	12.193	3380	3391	3413	rBV2	29450	57127	99.47%	24.311%
26	12.766	3561	3569	3578	rVB3	2689	4294	7.48%	1.827%
27	13.531	3798	3807	3812	rBV2	361	701	1.22%	0.298%
28	13.843	3895	3904	3916	rBV4	10699	18552	32.30%	7.895%
29	14.122	3982	3991	3994	rBV3	490	610	1.06%	0.260%
30	14.573	4123	4131	4141	rVB2	2456	4012	6.99%	1.707%
31	16.405	4697	4701	4705	rBV4	818	748	1.30%	0.318%
32	16.521	4732	4737	4740	rBV4	785	831	1.45%	0.354%
33	16.952	4867	4871	4874	rVV5	752	634	1.10%	0.270%
34	17.087	4910	4913	4917	rVB2	1017	717	1.25%	0.305%
35	17.296	4975	4978	4982	rBV4	632	603	1.05%	0.257%
36	17.486	5035	5037	5040	rBV3	985	664	1.16%	0.283%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060323.D
Acq On : 06 Aug 2024 15:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER




Sum of corrected areas: 234981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060323.D
Acq On : 06 Aug 2024 15:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

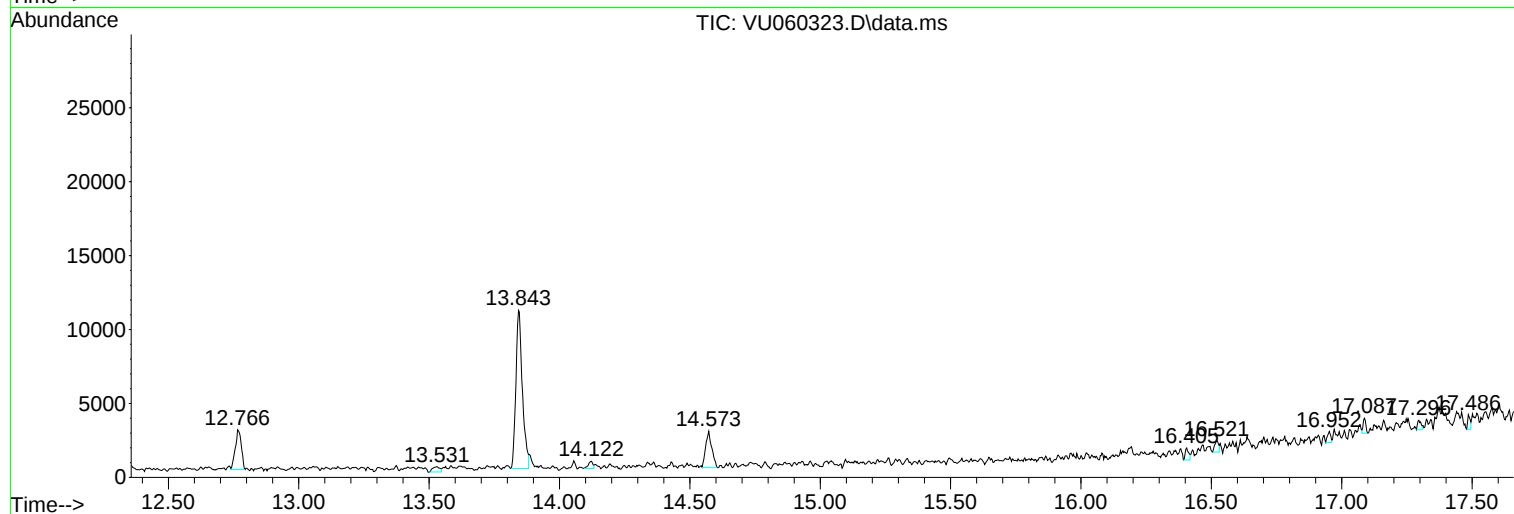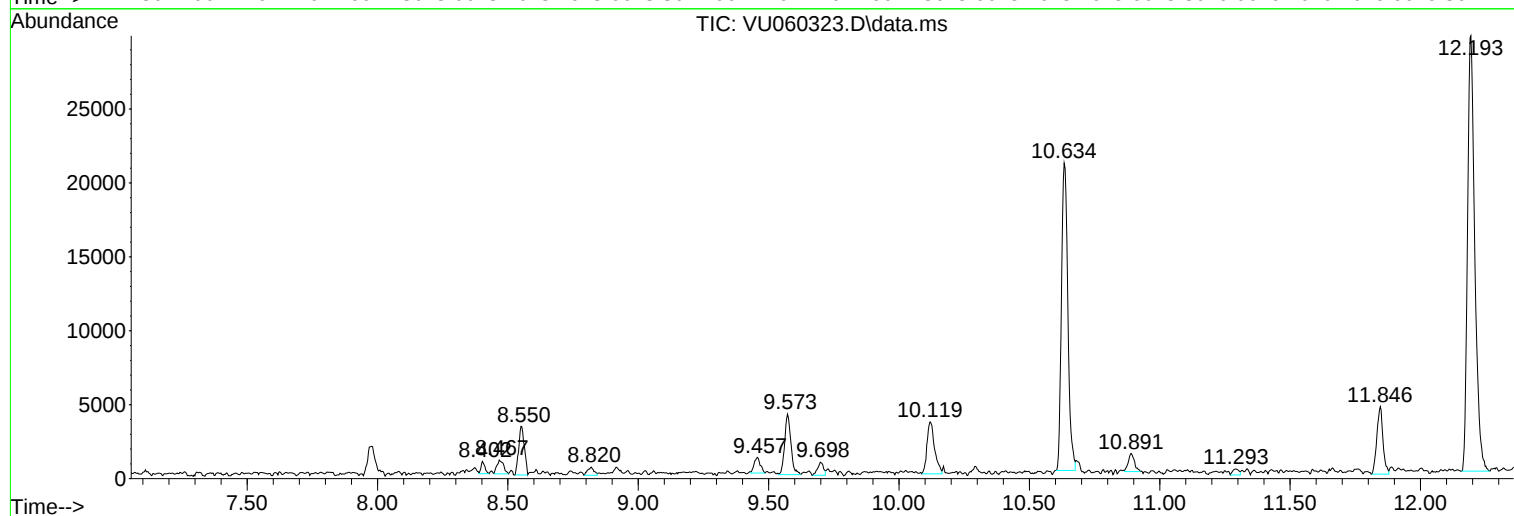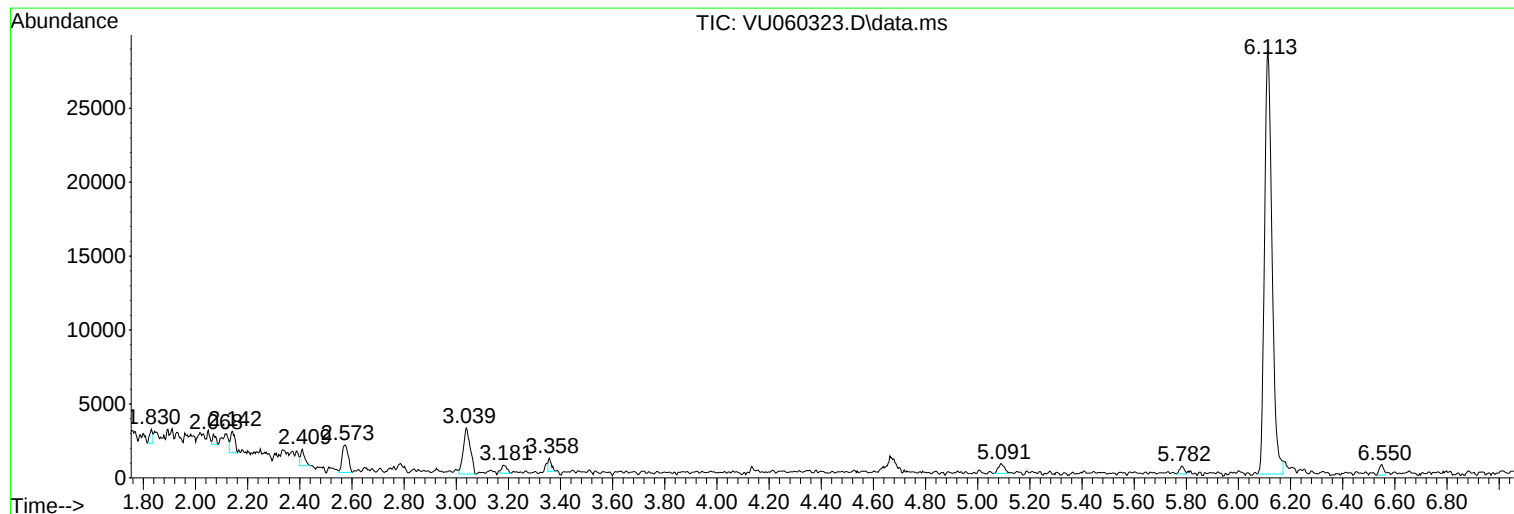

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060323.D
Acq On : 06 Aug 2024 15:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080624\
Data File : VU060323.D
Acq On : 06 Aug 2024 15:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------