

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
 Data File : VU060331.D
 Acq On : 07 Aug 2024 11:05
 Operator : MD/SY
 Sample : VU0807WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0807WBL01

Quant Time: Aug 08 05:54:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 06 11:07:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	29866	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	8431	0.829	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	9265	0.838	ug/l	0.00
Spiked Amount 1.000			Recovery	=	84.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060331.D
Acq On : 07 Aug 2024 11:05
Operator : MD/SY
Sample : VU0807WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01

Quant Time: Aug 08 05:54:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 06 11:07:28 2024
Response via : Initial Calibration




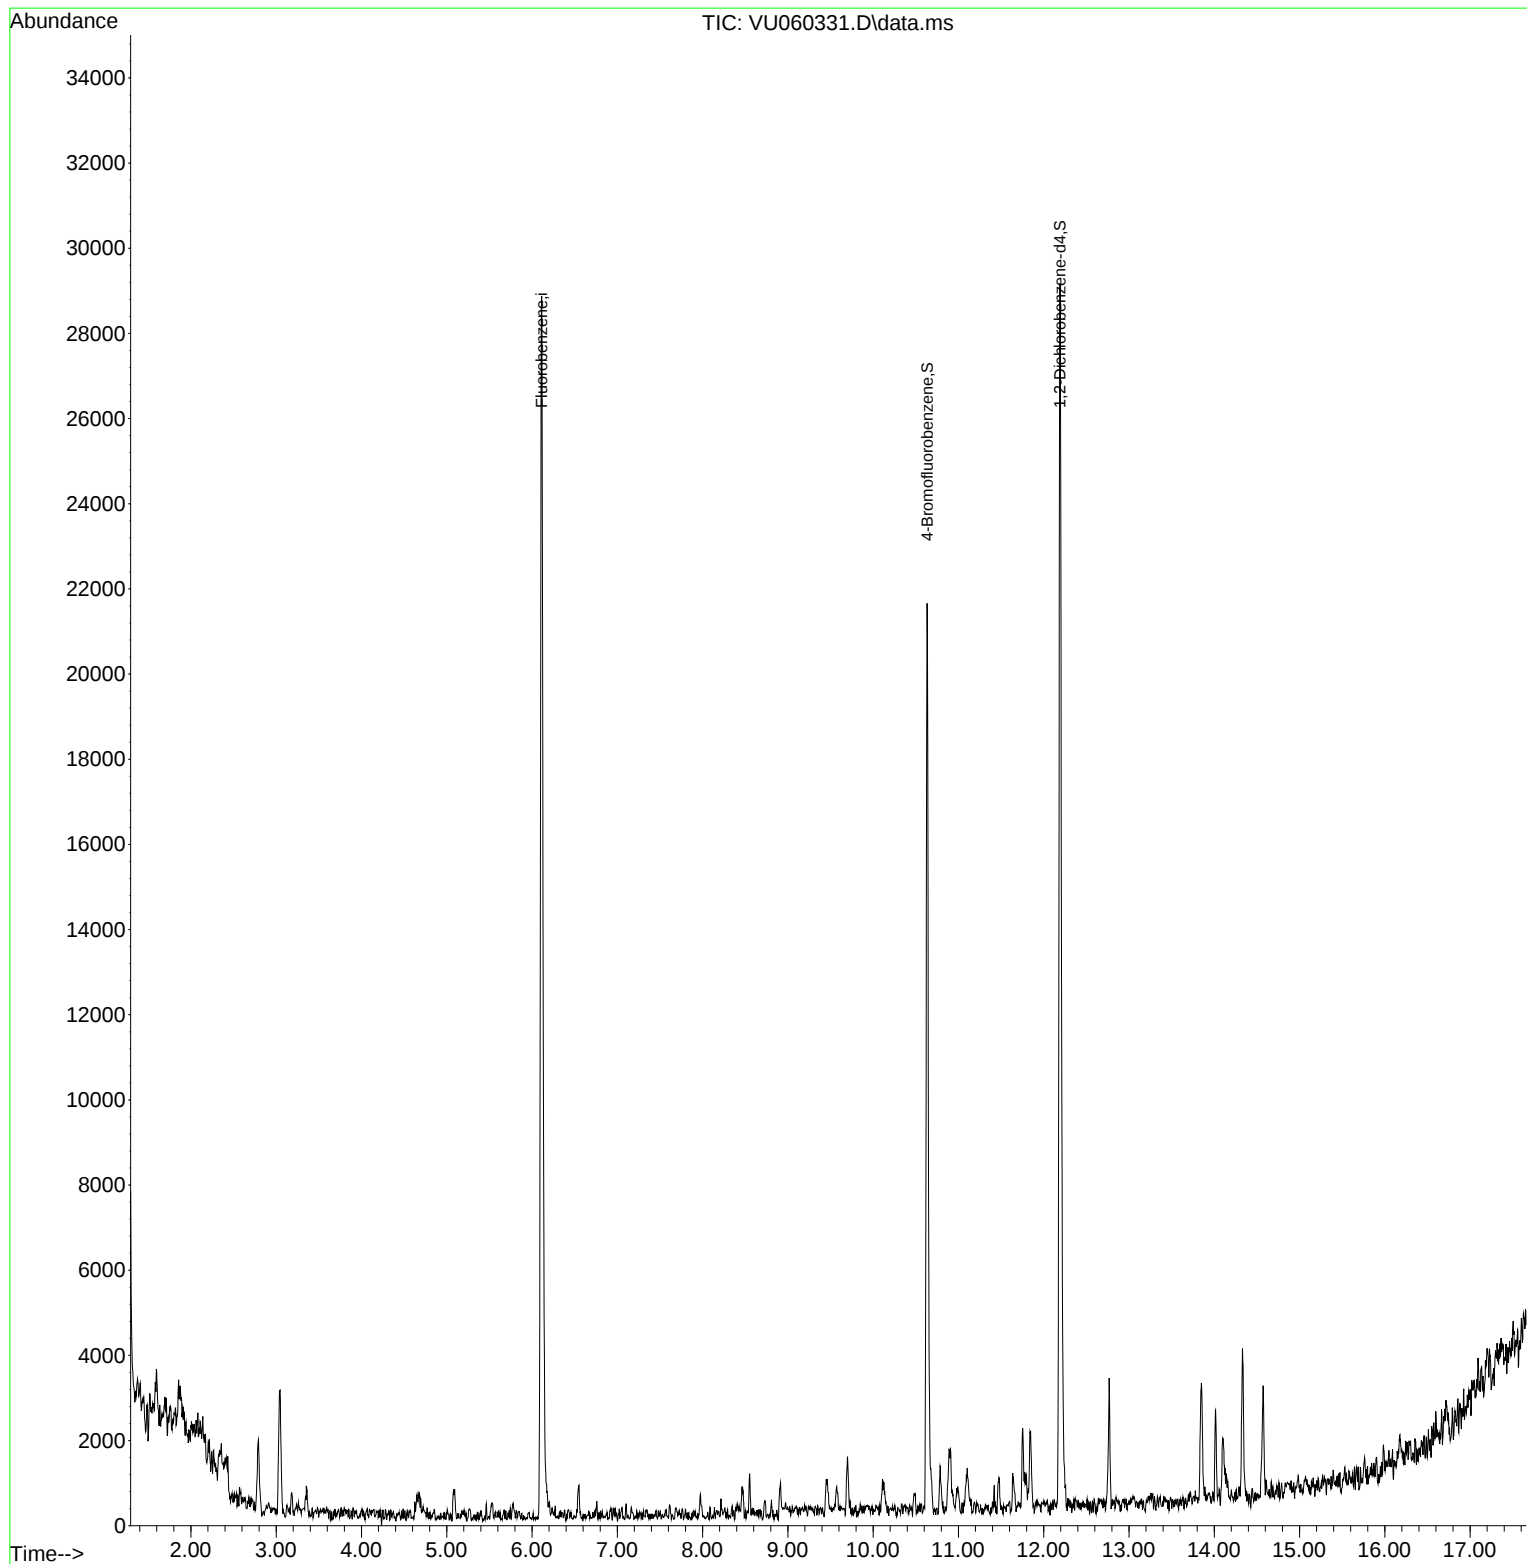


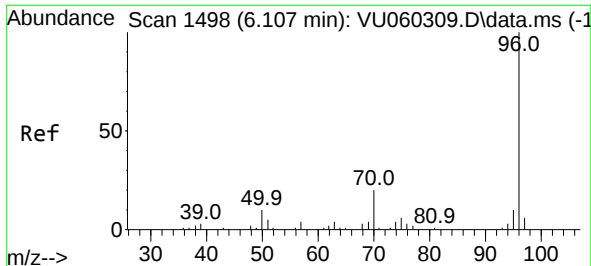

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU060331.D
Acq: 07 Aug 2024 11:05




Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01


Tgt Ion: 96	Resp: 29866
Ion Ratio	Lower Upper
96 100	
70 19.7	17.2 25.8
95 8.8	7.9 11.9
97 5.5	0.0 0.0

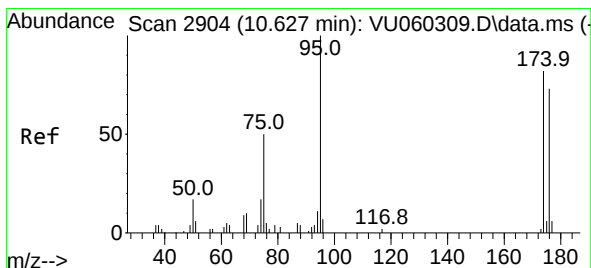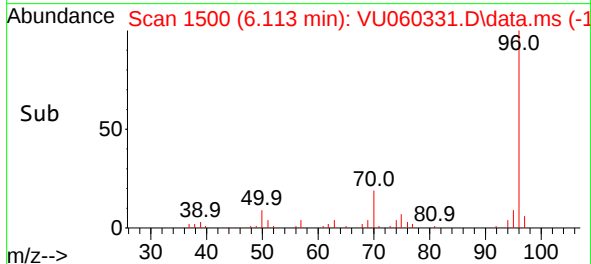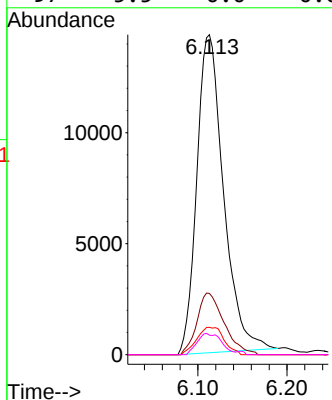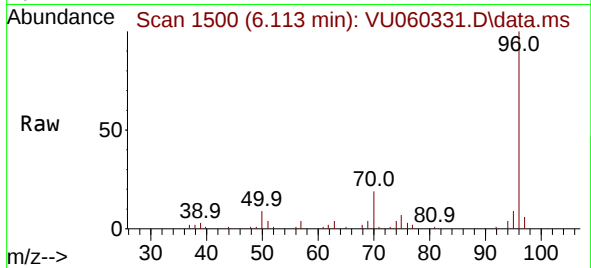

#57
4-Bromofluorobenzene
Concen: 0.829 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.006 min
Lab File: VU060331.D
Acq: 07 Aug 2024 11:05

Tgt Ion: 95	Resp: 8431
Ion Ratio	Lower Upper
95 100	
174 90.9	65.6 98.4
176 81.3	60.4 90.6

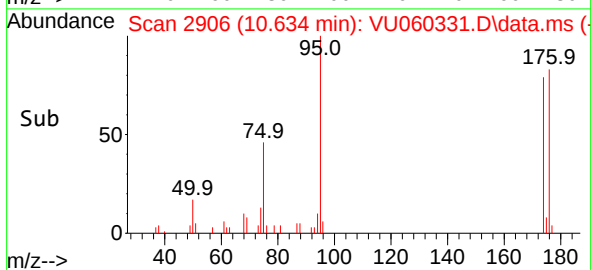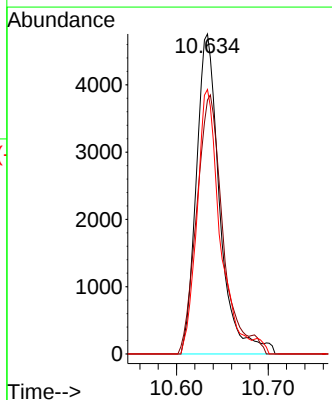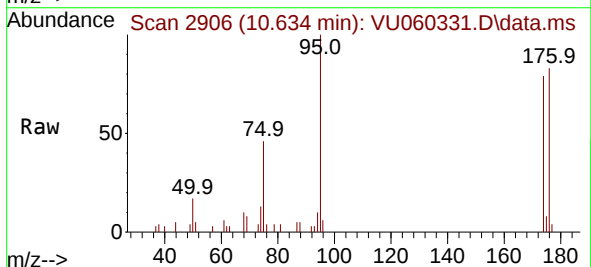

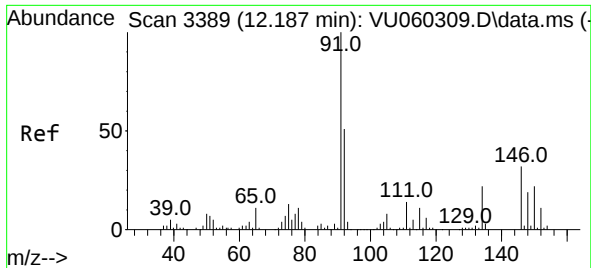

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.838 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU060331.D
 Acq: 07 Aug 2024 11:05

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0807WBL01

Tgt Ion:152 Resp: 9265
 Ion Ratio Lower Upper
 152 100
 115 67.0 0.0 325.2
 150 164.1 0.0 684.2

