

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
 Data File : VU060338.D
 Acq On : 07 Aug 2024 15:37
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Aug 08 05:58:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 06 11:07:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	27767	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	7519	0.795	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	9594	0.933	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060338.D
Acq On : 07 Aug 2024 15:37
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Aug 08 05:58:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 06 11:07:28 2024
Response via : Initial Calibration




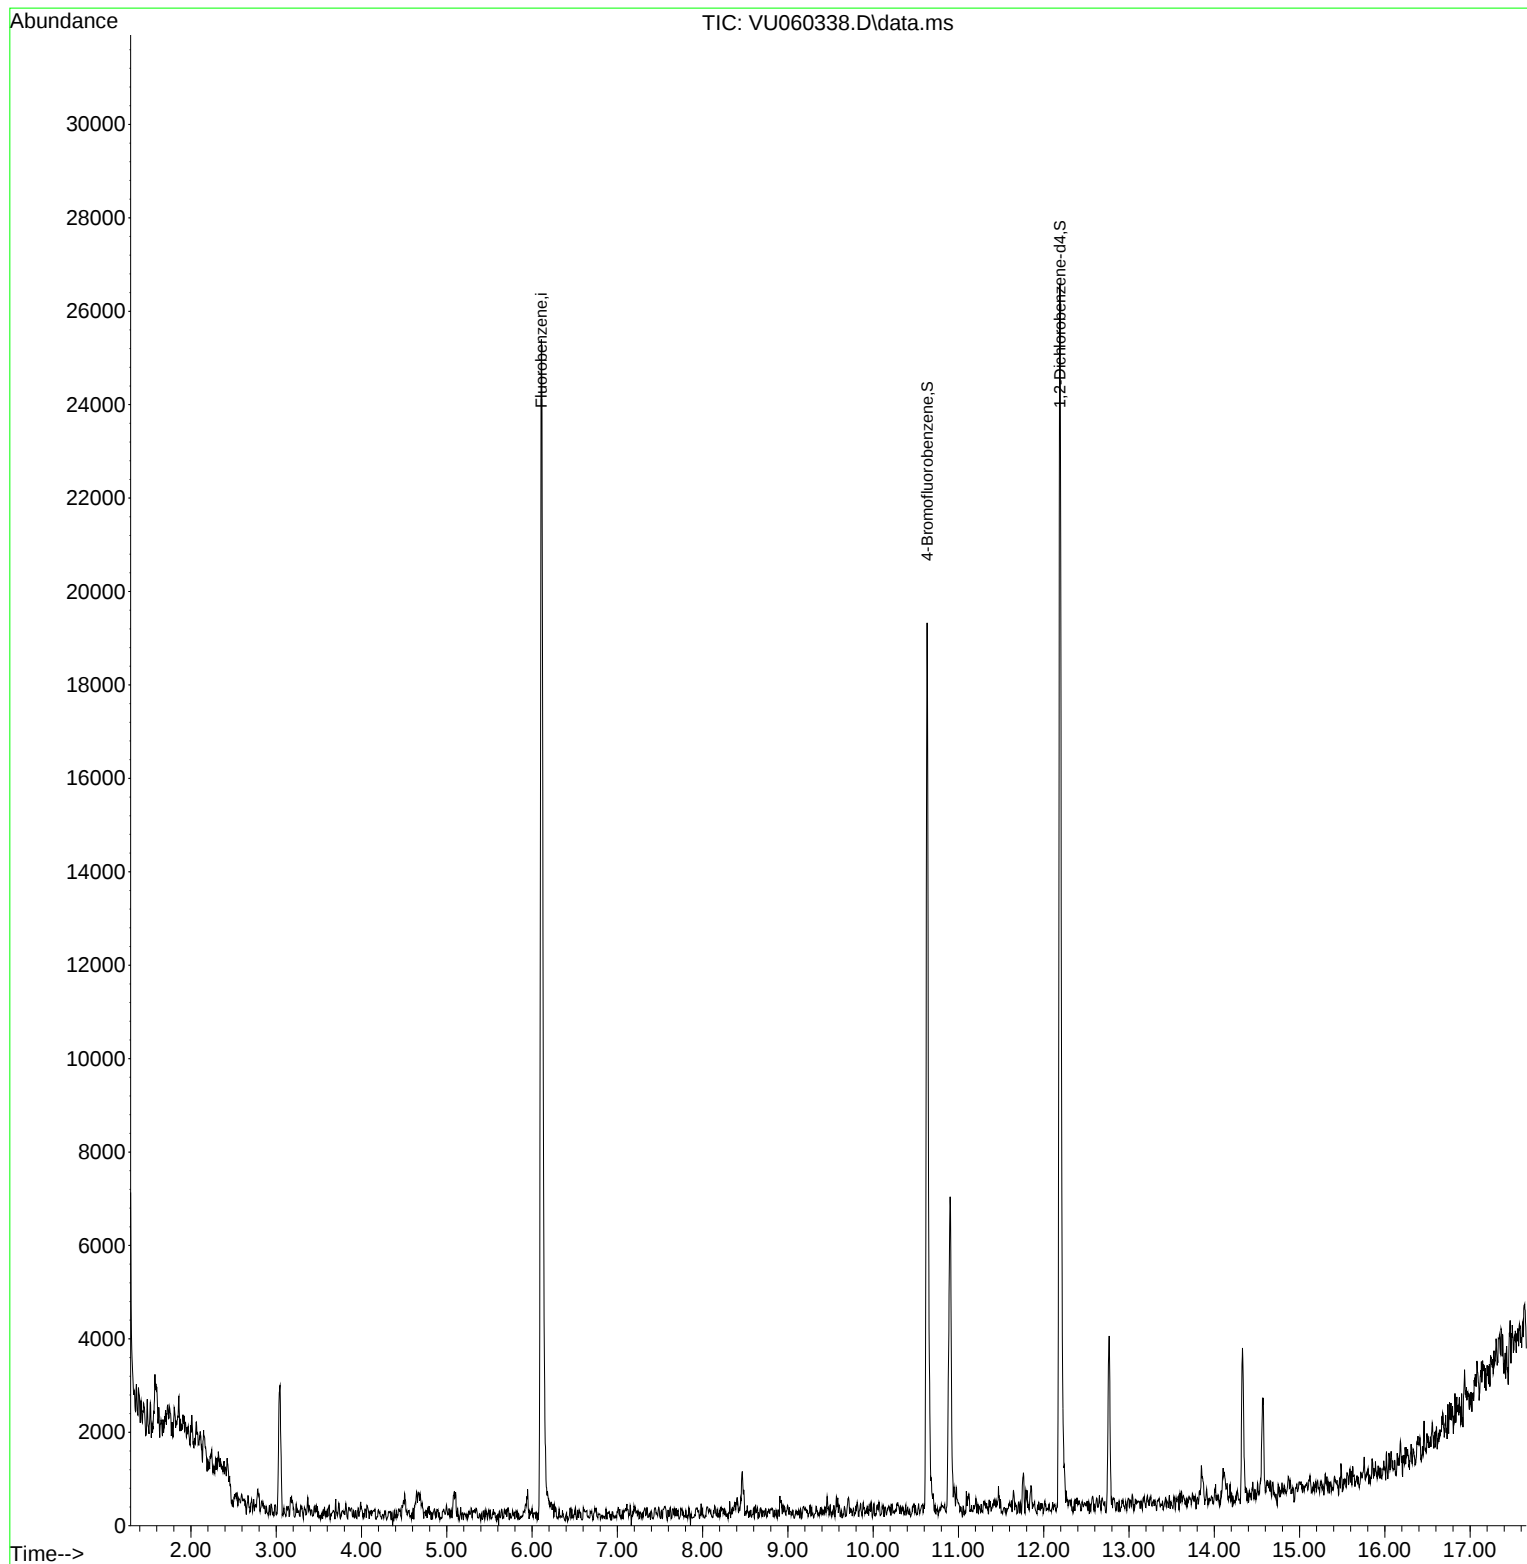


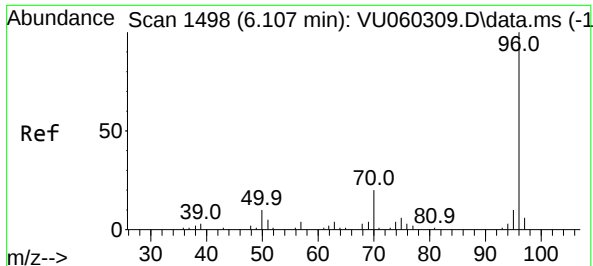

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1498
Delta R.T. 0.003 min
Lab File: VU060338.D
Acq: 07 Aug 2024 15:37




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion:	96	Resp:	27767
Ion Ratio	Lower	Upper	
96	100		
70	19.1	17.2	25.8
95	7.4	7.9	11.9#
97	5.7	0.0	0.0#

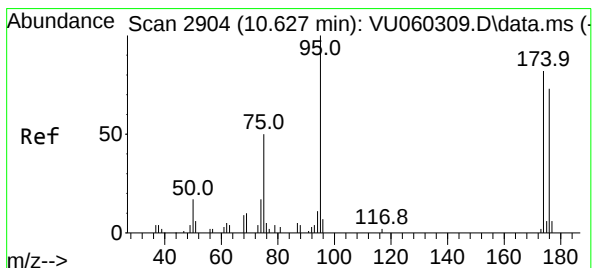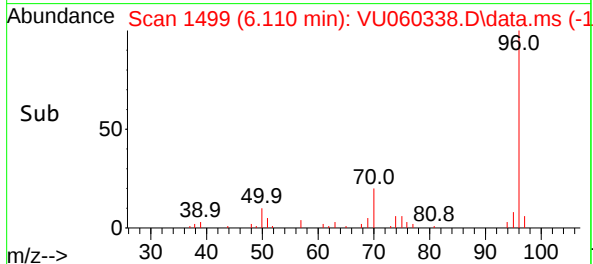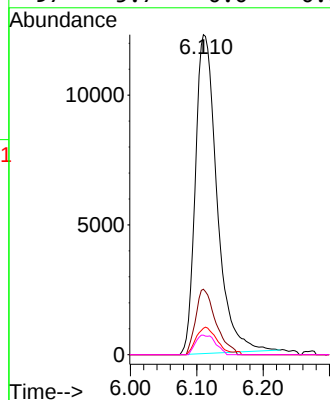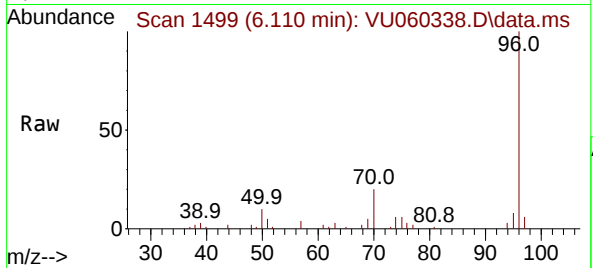

#57
4-Bromofluorobenzene
Concen: 0.795 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.006 min
Lab File: VU060338.D
Acq: 07 Aug 2024 15:37


Tgt Ion:	95	Resp:	7519
Ion Ratio	Lower	Upper	
95	100		
174	94.9	65.6	98.4
176	88.1	60.4	90.6

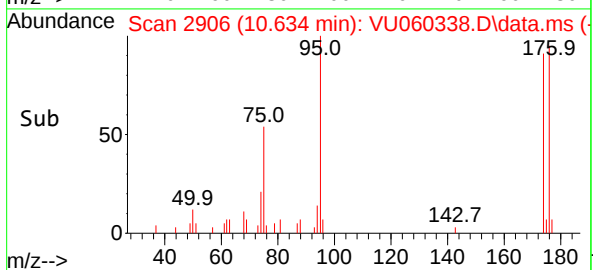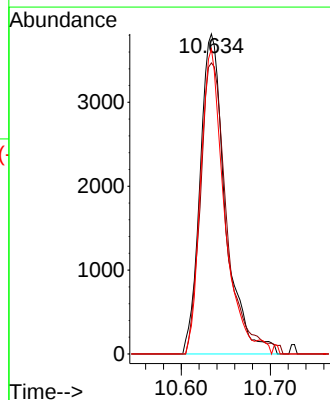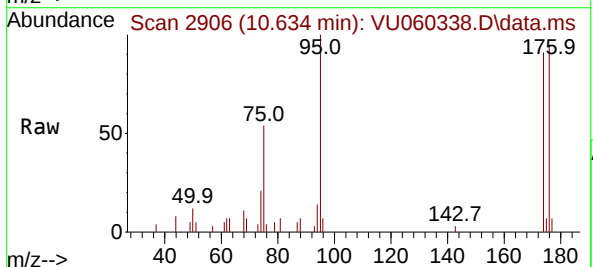

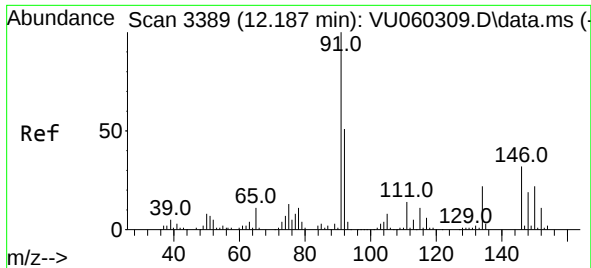

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.933 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU060338.D
 Acq: 07 Aug 2024 15:37

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

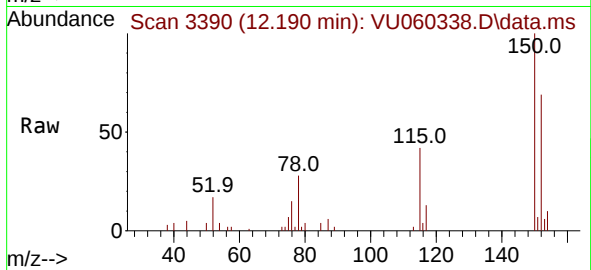

Tgt Ion:	152	Resp:	9594
Ion Ratio	Lower	Upper	
152	100		
115	60.0	0.0	325.2
150	141.2	0.0	684.2

