

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
 Data File : VU060331.D
 Acq On : 07 Aug 2024 11:05
 Operator : MD/SY
 Sample : VU0807WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0807WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.431	354	355	363	rVB2	1003	644	1.07%	0.302%
2	2.792	457	467	479	rVB2	1789	3550	5.92%	1.667%
3	3.046	535	546	556	rBB3	2901	5627	9.39%	2.643%
4	3.184	583	589	593	rBV4	510	653	1.09%	0.307%
5	3.354	641	642	651	rVB3	709	626	1.04%	0.294%
6	5.084	1173	1180	1181	rBV3	748	815	1.36%	0.383%
7	5.531	1310	1319	1326	rBV3	382	670	1.12%	0.315%
8	6.113	1487	1500	1524	rBV	28723	59938	100.00%	28.153%
9	6.550	1629	1636	1640	rVB2	646	820	1.37%	0.385%
10	7.975	2071	2079	2083	rBV3	550	666	1.11%	0.313%
11	8.553	2254	2259	2264	rVB4	980	1003	1.67%	0.471%
12	8.730	2306	2314	2319	rBV3	447	645	1.08%	0.303%
13	8.913	2364	2371	2376	rBV3	885	1341	2.24%	0.630%
14	9.450	2530	2538	2540	rBV3	887	956	1.59%	0.449%
15	9.698	2607	2615	2622	rBV4	1361	2121	3.54%	0.996%
16	10.110	2736	2743	2745	rBV	759	740	1.23%	0.348%
17	10.634	2897	2906	2918	rBV3	21250	35666	59.50%	16.752%
18	10.785	2946	2953	2962	rBV4	1126	1707	2.85%	0.802%
19	10.891	2976	2986	2989	rBV3	1408	2103	3.51%	0.988%
20	10.994	3015	3018	3028	rVB3	598	818	1.36%	0.384%
21	11.093	3042	3049	3050	rBV2	728	685	1.14%	0.322%
22	11.103	3050	3052	3061	rVB2	801	884	1.47%	0.415%
23	11.476	3160	3168	3174	rBV3	860	1418	2.37%	0.666%
24	11.753	3247	3254	3260	rBV4	1862	2559	4.27%	1.202%
25	11.794	3265	3267	3272	rVV4	771	693	1.16%	0.326%
26	11.839	3276	3281	3292	rVB3	1763	2937	4.90%	1.380%
27	12.190	3379	3390	3409	rBV	28666	55419	92.46%	26.031%
28	12.769	3560	3570	3577	rVB2	3077	4150	6.92%	1.949%
29	13.849	3897	3906	3916	rBV5	2739	4954	8.27%	2.327%
30	14.016	3952	3958	3965	rBV6	2138	2642	4.41%	1.241%
31	14.100	3975	3984	3991	rBV4	1588	3024	5.05%	1.420%
32	14.331	4047	4056	4068	rVB4	3469	5453	9.10%	2.561%
33	14.572	4120	4131	4139	rBV3	2618	4160	6.94%	1.954%
34	15.904	4540	4545	4550	rVB2	622	673	1.12%	0.316%
35	15.984	4566	4570	4576	rBV2	703	734	1.22%	0.345%
36	16.823	4827	4831	4835	rBV4	573	649	1.08%	0.305%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060331.D
Acq On : 07 Aug 2024 11:05
Operator : MD/SY
Sample : VU0807WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

37	16.878	4845	4848	4854	rbV5	700	757	1.26%	0.356%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 212900

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060331.D
Acq On : 07 Aug 2024 11:05
Operator : MD/SY
Sample : VU0807WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

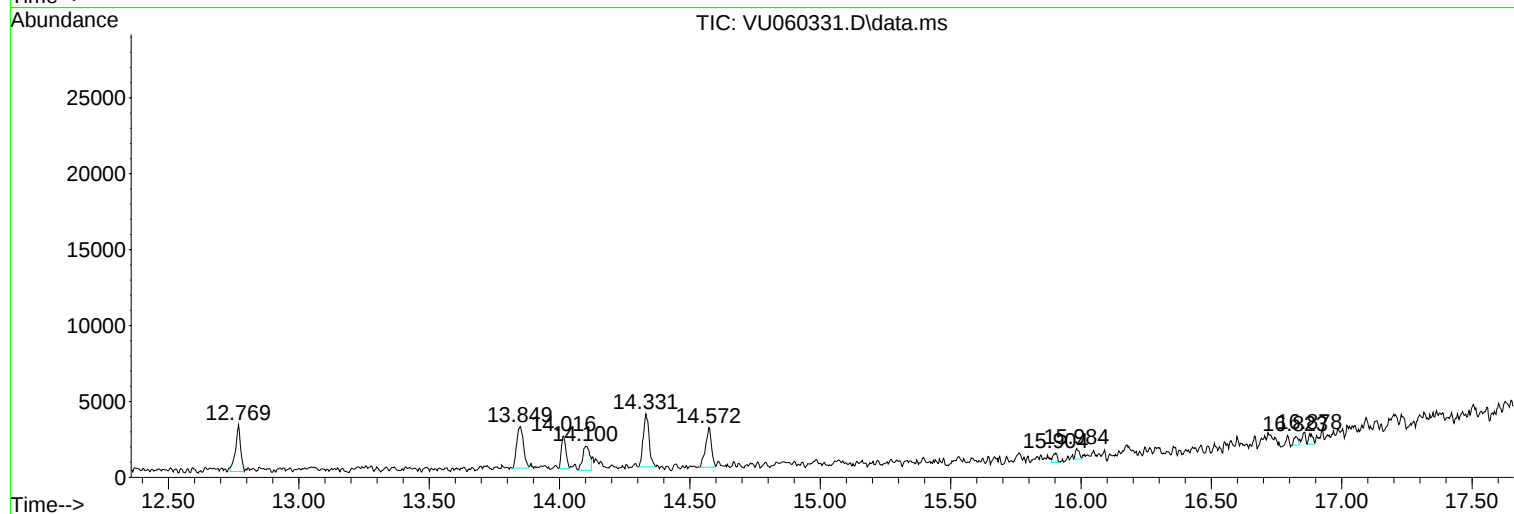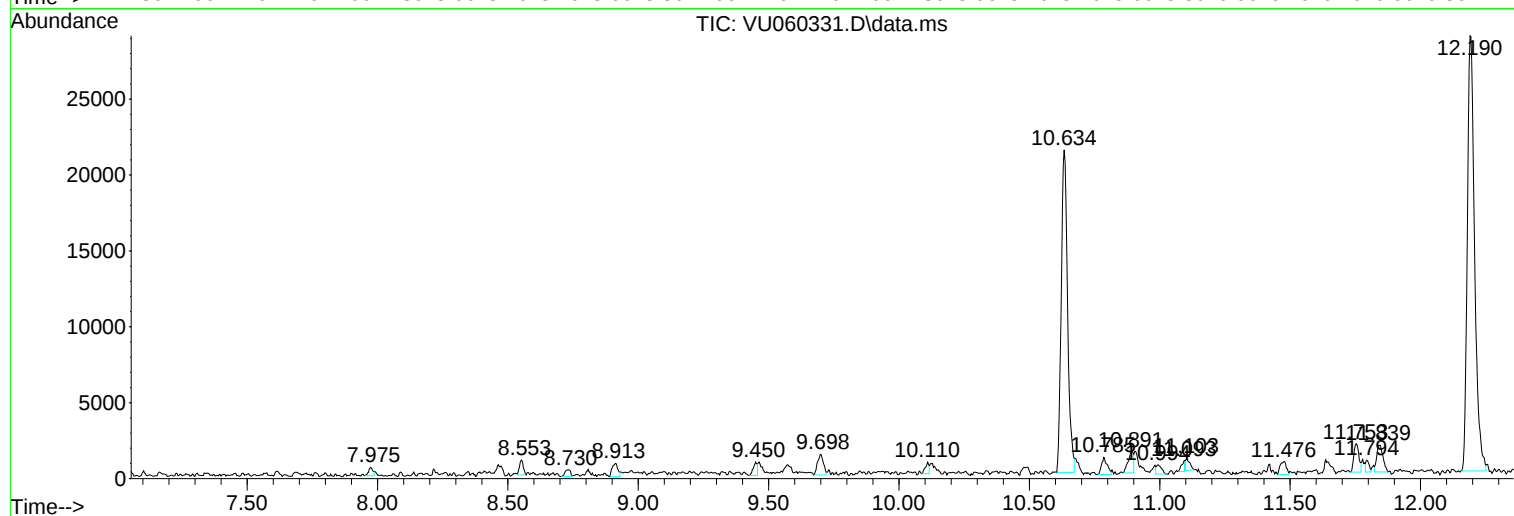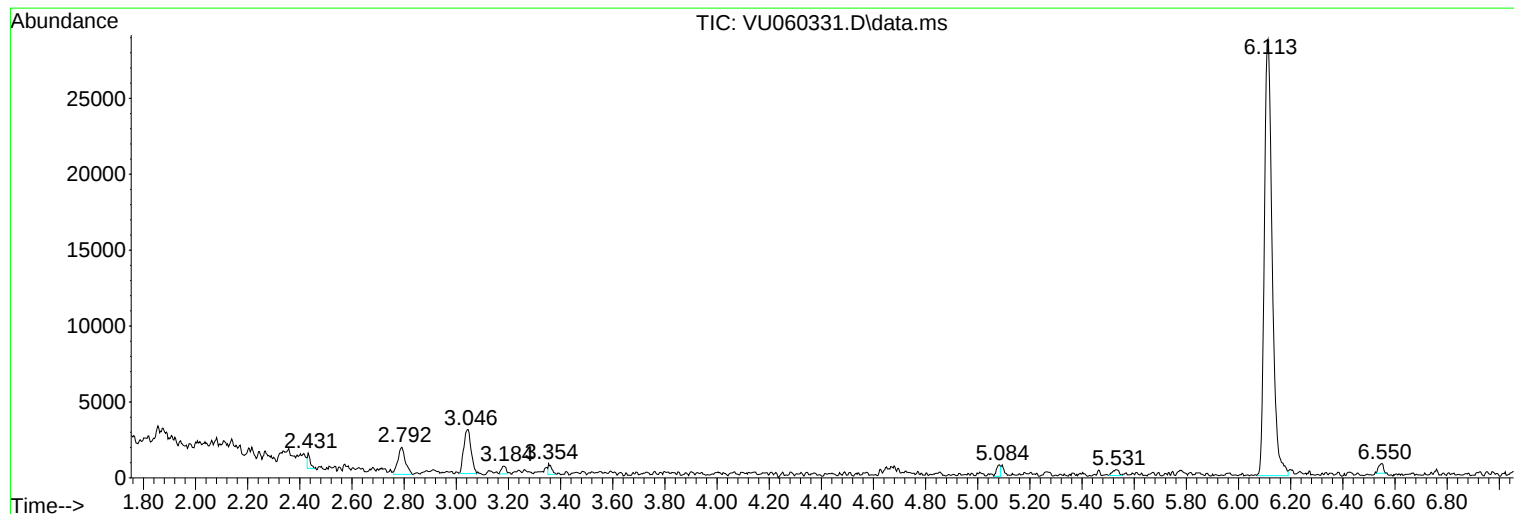

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060331.D
Acq On : 07 Aug 2024 11:05
Operator : MD/SY
Sample : VU0807WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060331.D
Acq On : 07 Aug 2024 11:05
Operator : MD/SY
Sample : VU0807WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0807WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------