

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
 Data File : VU060335.D
 Acq On : 07 Aug 2024 14:26
 Operator : MD/SY
 Sample : P3204-07DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WSDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.576	388	400	413	rBV	72346	117996	38.55%	4.827%
2	3.039	531	544	566	rBV	89134	176968	57.82%	7.240%
3	3.178	577	587	588	rBV	3793	4364	1.43%	0.179%
4	3.351	629	641	657	rBV3	23320	45994	15.03%	1.882%
5	4.663	1027	1049	1068	rBV2	33208	88670	28.97%	3.628%
6	5.309	1236	1250	1267	rBV3	20136	46467	15.18%	1.901%
7	5.518	1300	1315	1332	rVB3	18542	42072	13.75%	1.721%
8	5.775	1380	1395	1417	rBV2	41472	112854	36.87%	4.617%
9	6.113	1488	1500	1521	rBV2	28582	58375	19.07%	2.388%
10	6.541	1624	1633	1647	rBV2	11784	22004	7.19%	0.900%
11	6.785	1697	1709	1732	rVB3	32948	64862	21.19%	2.654%
12	7.965	2065	2076	2100	rBV	109098	198017	64.70%	8.101%
13	8.396	2199	2210	2226	rBV	55443	97551	31.87%	3.991%
14	8.547	2246	2257	2278	rBV	121800	209019	68.29%	8.551%
15	8.907	2361	2369	2381	rVB2	4271	7313	2.39%	0.299%
16	9.444	2525	2536	2555	rBV2	37593	64901	21.21%	2.655%
17	9.566	2562	2574	2598	rBV	179527	306059	100.00%	12.521%
18	9.692	2602	2613	2629	rVB2	28819	50662	16.55%	2.073%
19	10.110	2727	2743	2769	rBV3	145317	286651	93.66%	11.727%
20	10.631	2896	2905	2927	rVB2	26573	45952	15.01%	1.880%
21	10.888	2974	2985	2988	rBV3	2366	3329	1.09%	0.136%
22	11.833	3268	3279	3298	rVB	68926	113942	37.23%	4.661%
23	12.203	3379	3394	3413	rBV3	71024	164058	53.60%	6.712%
24	12.769	3556	3570	3578	rBV3	3234	5531	1.81%	0.226%
25	13.836	3891	3902	3920	rBV	62178	105974	34.63%	4.335%
26	14.569	4118	4130	4141	rBV2	3012	4768	1.56%	0.195%




Sum of corrected areas: 2444353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060335.D
Acq On : 07 Aug 2024 14:26
Operator : MD/SY
Sample : P3204-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WSDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

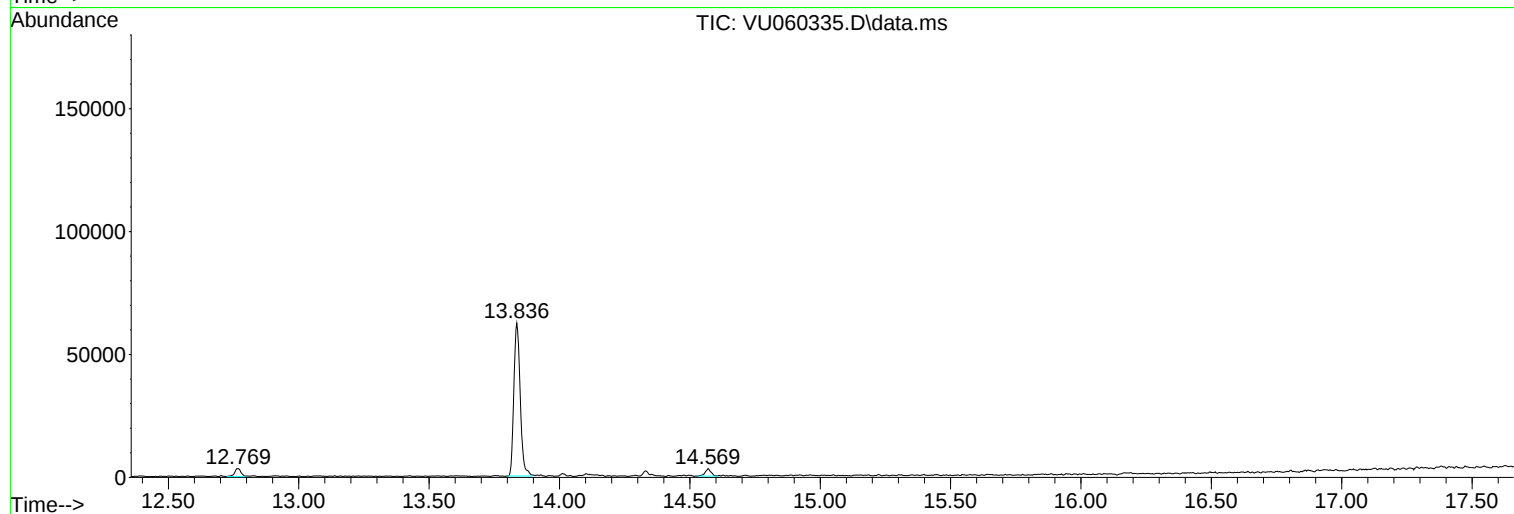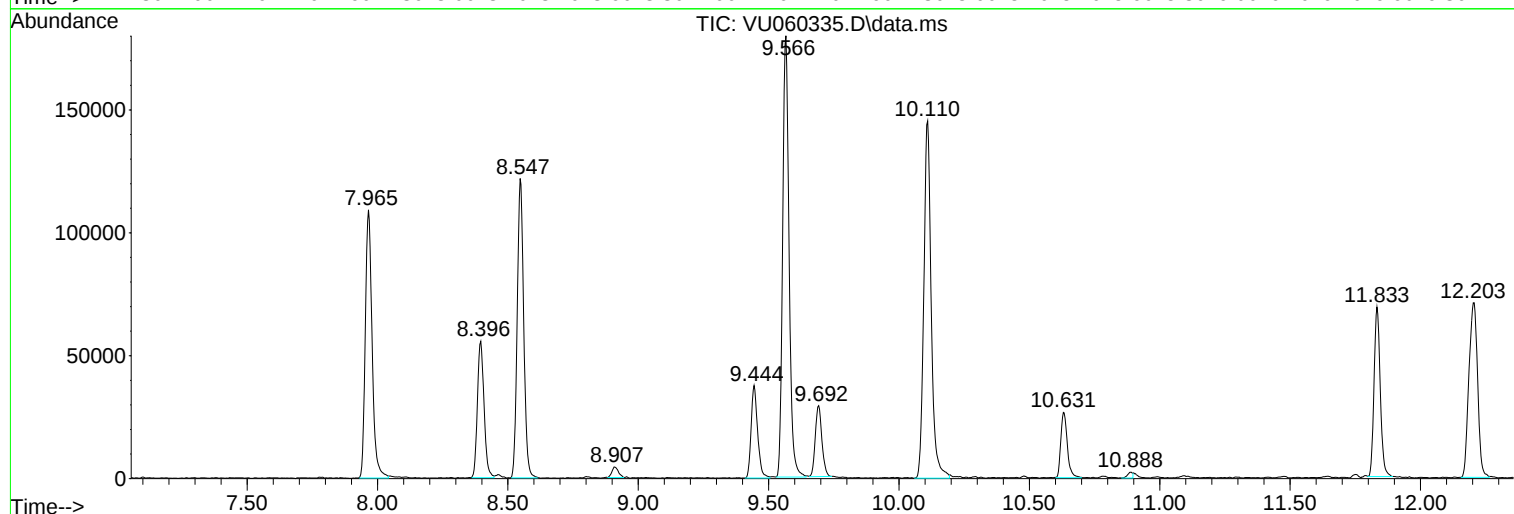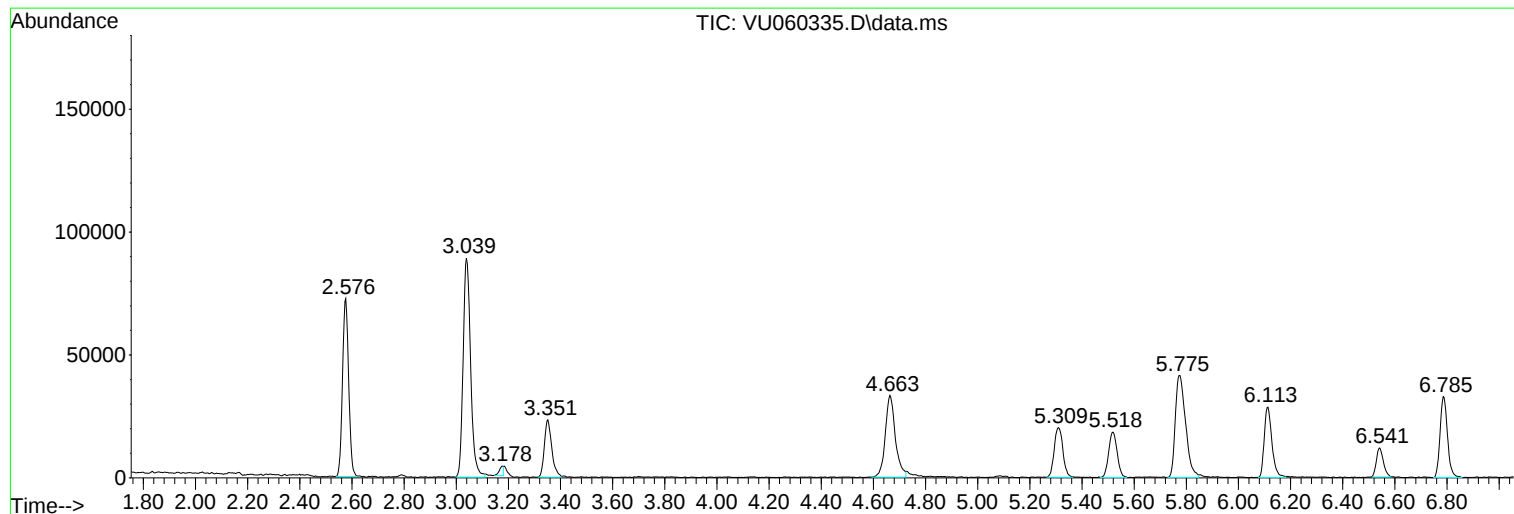

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060335.D
Acq On : 07 Aug 2024 14:26
Operator : MD/SY
Sample : P3204-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WSDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060335.D
Acq On : 07 Aug 2024 14:26
Operator : MD/SY
Sample : P3204-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WSDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------