

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
 Data File : VU060345.D
 Acq On : 07 Aug 2024 18:47
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	265	268	274	rVV4	661	731	1.44%	0.441%
2	2.788	460	466	467	rBV2	542	566	1.11%	0.342%
3	3.042	535	545	556	rBV4	3601	6629	13.04%	4.000%
4	3.177	582	587	593	rBV3	746	928	1.83%	0.560%
5	4.647	1038	1044	1047	rBV2	402	513	1.01%	0.310%
6	5.097	1181	1184	1190	rVB3	605	629	1.24%	0.380%
7	6.113	1487	1500	1520	rBV	25294	50842	100.00%	30.678%
8	8.917	2370	2372	2379	rVB4	755	756	1.49%	0.456%
9	9.457	2534	2540	2547	rVB2	473	517	1.02%	0.312%
10	10.634	2897	2906	2930	rVB3	18638	33882	66.64%	20.444%
11	10.891	2976	2986	3002	rBV3	3200	5978	11.76%	3.607%
12	11.640	3214	3219	3225	rBV2	373	598	1.18%	0.361%
13	11.843	3278	3282	3291	rVB2	695	761	1.50%	0.459%
14	12.190	3378	3390	3414	rBV	26237	47241	92.92%	28.505%
15	12.769	3559	3570	3578	rBV2	3328	5714	11.24%	3.448%
16	13.852	3900	3907	3909	rBV3	667	731	1.44%	0.441%
17	14.338	4048	4058	4064	rBV4	997	1647	3.24%	0.994%
18	14.569	4123	4130	4140	rBV	1944	2977	5.86%	1.796%
19	16.344	4676	4682	4687	rBV4	798	816	1.60%	0.492%
20	16.543	4740	4744	4747	rBV5	694	546	1.07%	0.329%
21	16.585	4753	4757	4762	rBV4	765	844	1.66%	0.509%
22	16.727	4797	4801	4805	rBV5	756	619	1.22%	0.374%
23	16.913	4854	4859	4862	rBV4	702	656	1.29%	0.396%
24	17.186	4941	4944	4948	rBV3	837	608	1.20%	0.367%




Sum of corrected areas: 165729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060345.D
Acq On : 07 Aug 2024 18:47
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

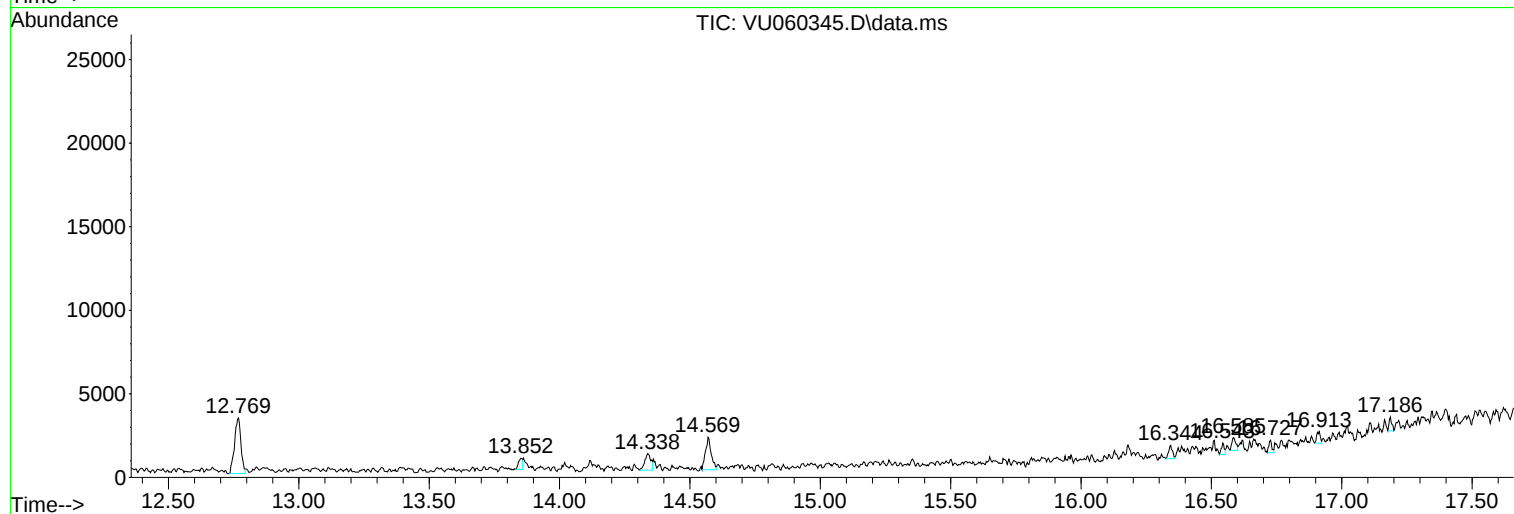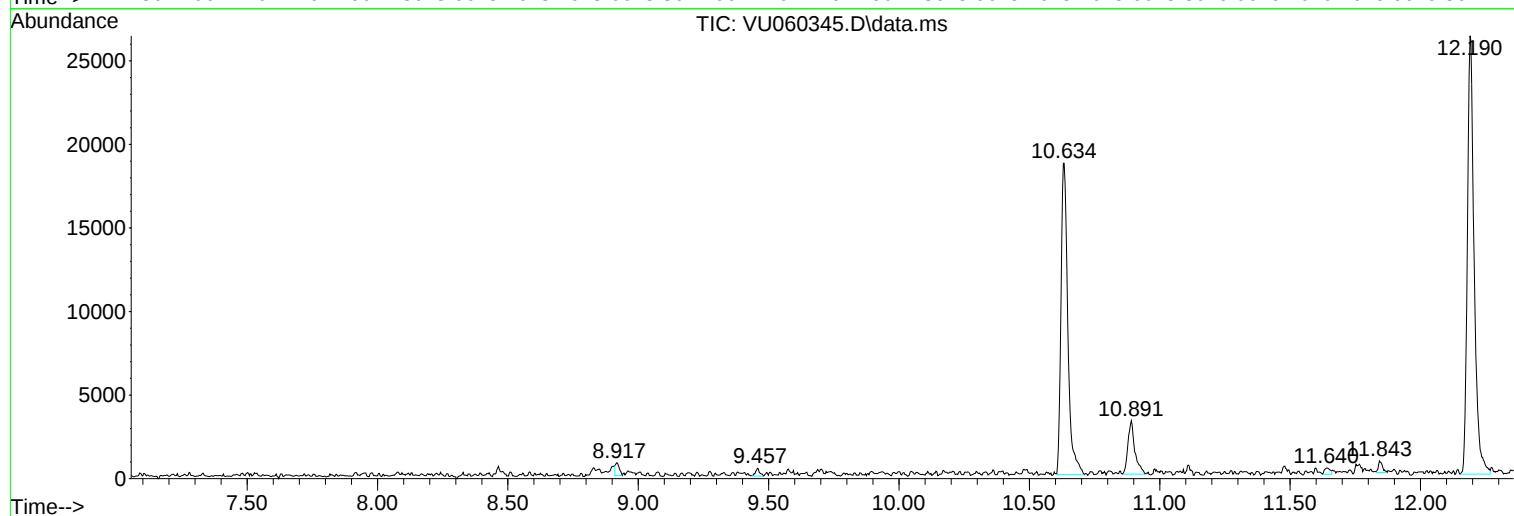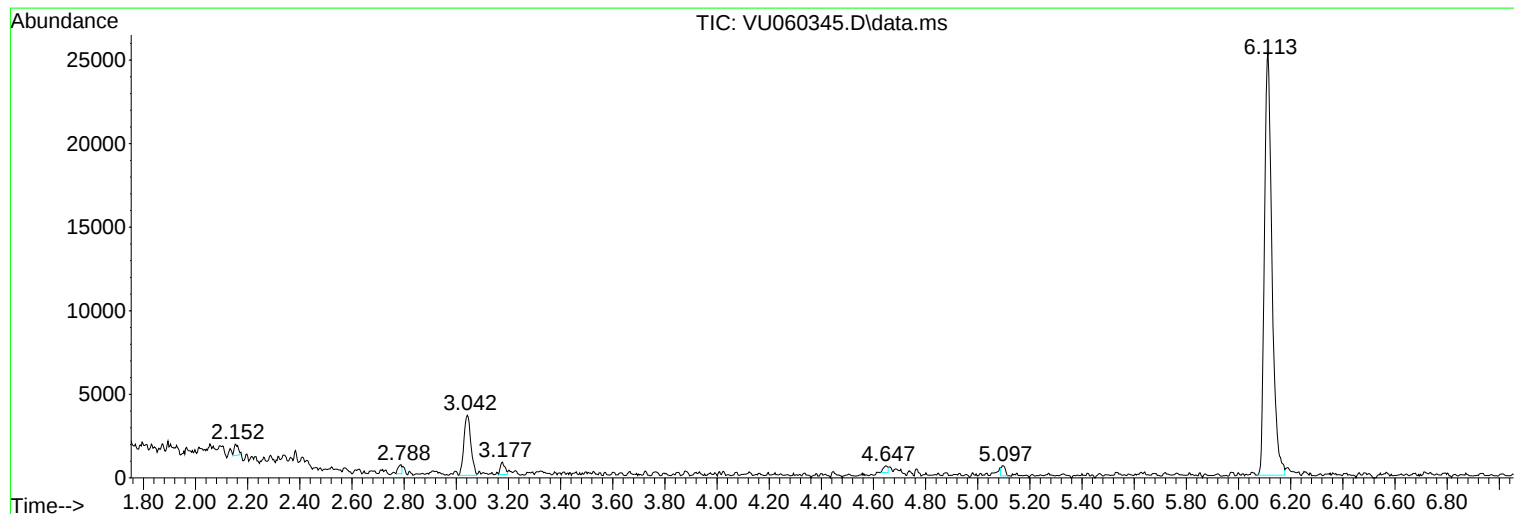

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060345.D
Acq On : 07 Aug 2024 18:47
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080724\
Data File : VU060345.D
Acq On : 07 Aug 2024 18:47
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------