

Data File : VU033654.D
Acq On : 08 Aug 2019 21:38
Operator : JC/SP
Sample : K4202-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B25

Quant Time: Aug 09 12:07:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080819WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 07:39:51 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	299249	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	302486	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	139157	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	143292	42.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.84%
7) Chloroethane-d5	1.67	69	119938	41.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.90%
11) 1,1-Dichloroethene-d2	2.26	63	182921	33.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.00%
21) 2-Butanone-d5	4.15	46	210922	85.25	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.25%
24) Chloroform-d	4.62	84	206263	36.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.70%
26) 1,2-Dichloroethane-d4	5.29	65	148762	41.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.42%
32) Benzene-d6	5.32	84	469524	41.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.24%
36) 1,2-Dichloropropane-d6	6.31	67	151506	42.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.48%
41) Toluene-d8	7.55	98	418205	40.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.20%
43) trans-1,3-Dichloropropene-	7.83	79	68933	39.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.54%
47) 2-Hexanone-d5	8.29	63	168671	93.93	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.93%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	230518	41.09	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.18%
64) 1,2-Dichlorobenzene-d4	11.85	152	158617	41.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.44%


Target Compounds						Qvalue
13) Acetone	2.31	43	4063	2.414	ug/L	99
42) Toluene	7.62	91	41105	4.014	ug/L	98
53) m,p-Xylene	9.36	106	5955	1.428	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU033654.D
Acq On : 08 Aug 2019 21:38
Operator : JC/SP
Sample : K4202-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B25

Quant Time: Aug 09 12:07:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080819WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 07:39:51 2019
Response via : Initial Calibration

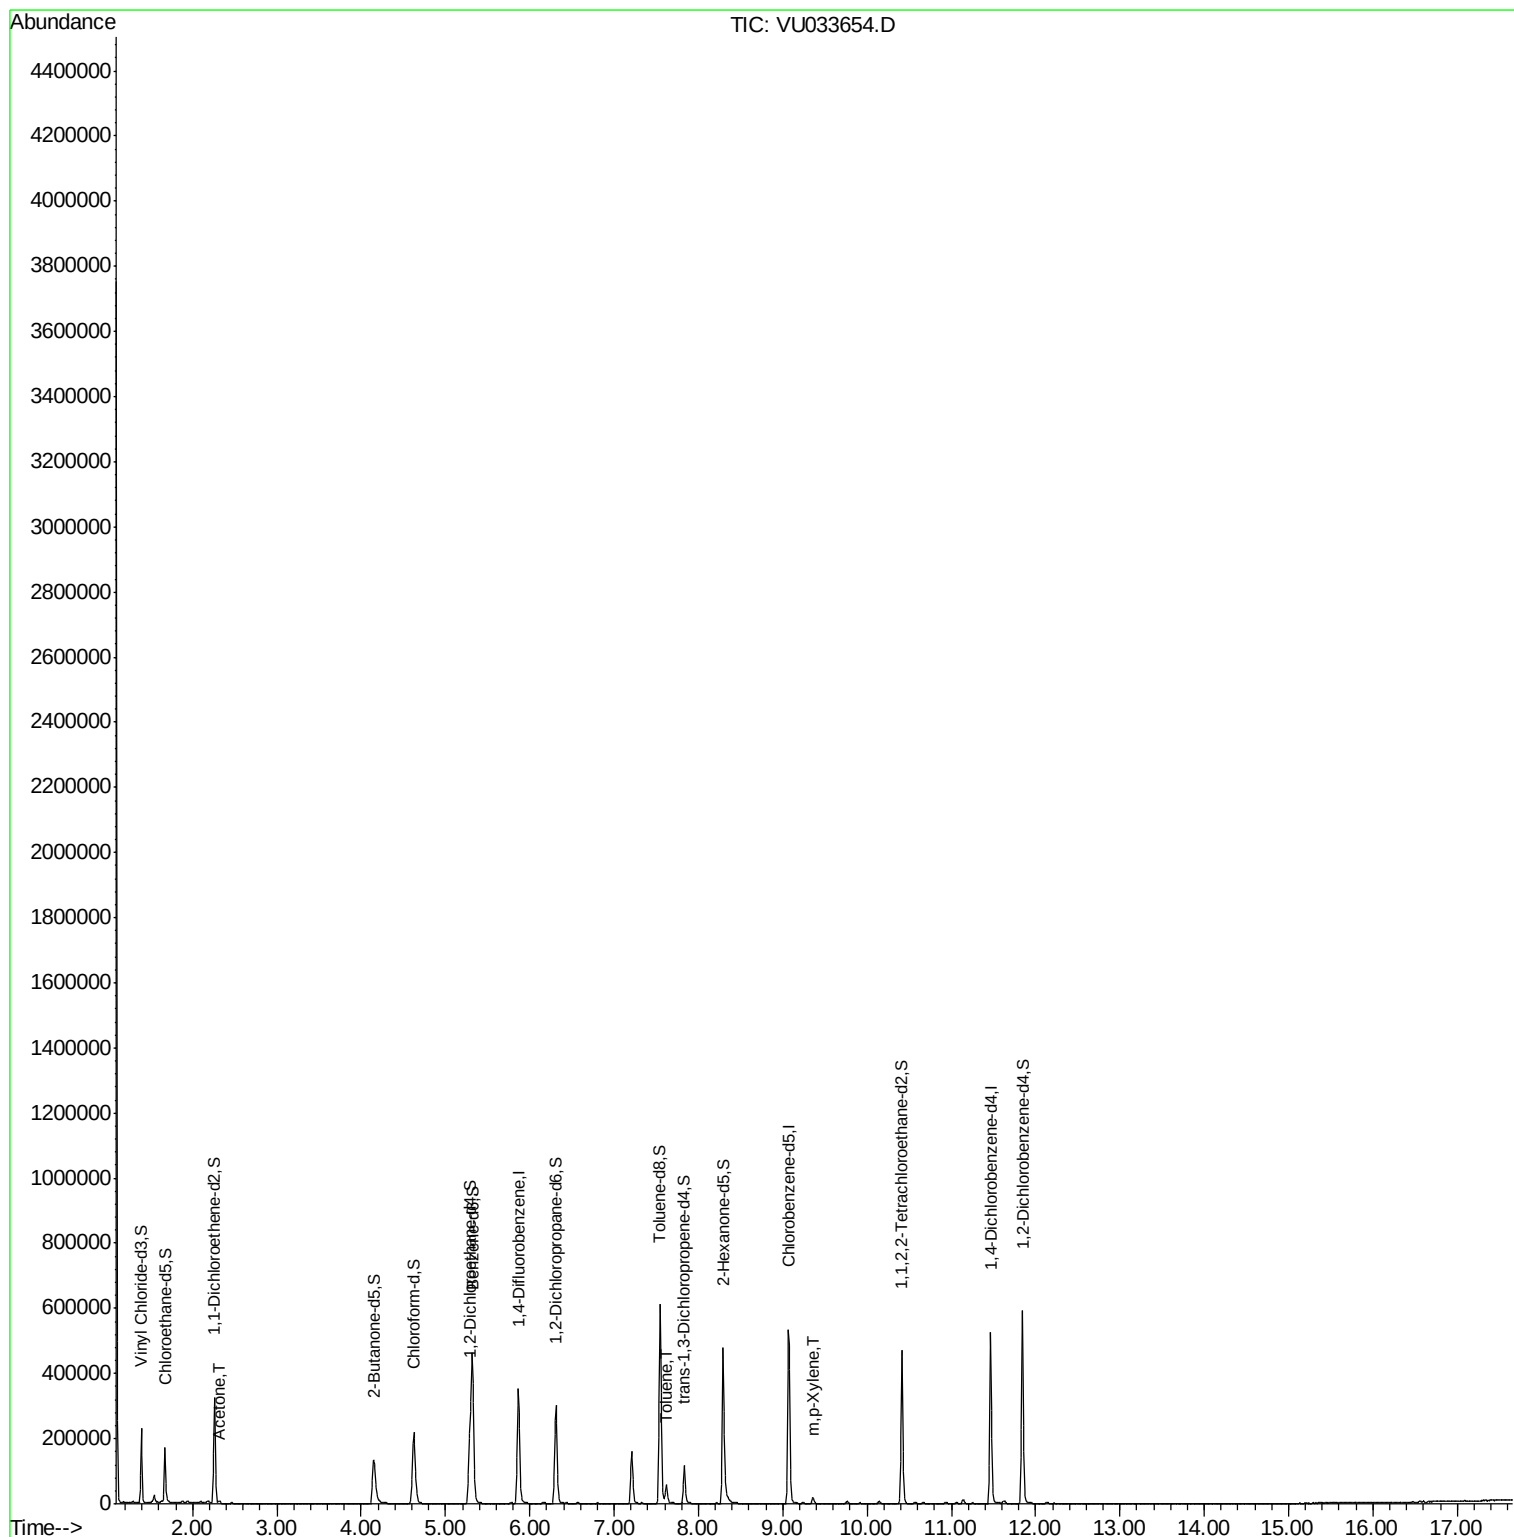

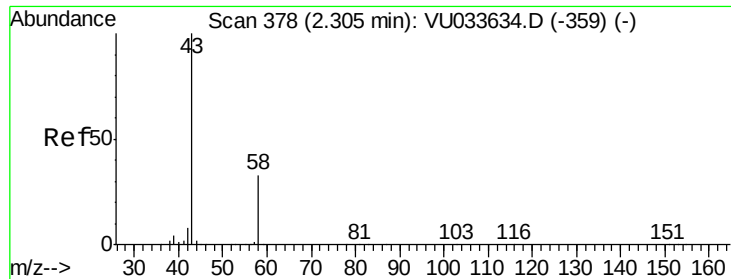

#13

Acetone

Concen: 2.414 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VU033654.D

Acq: 08 Aug 2019 21:38

Instrument :

MSVOA_U

ClientSampled :


F2B25

Tgt Ion: 43 Resp: 4063

Ion Ratio Lower Upper

43 100

58 32.0 0.0 65.0

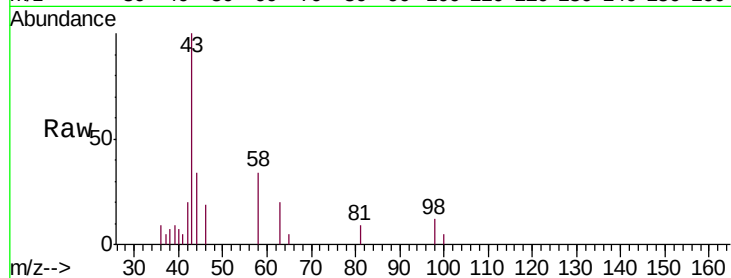




Abundance Ion 43.00 (42.70 to 43.70): VU033634.D (-359) (-)

Ion 58.00 (57.70 to 58.70): VU033634.D (-359) (-)

2.31

2.30

2.35

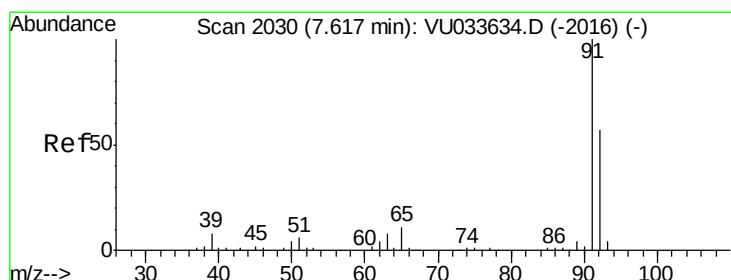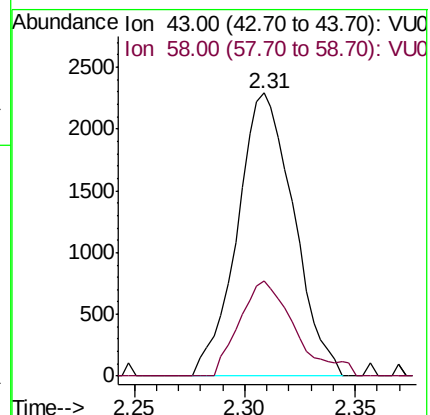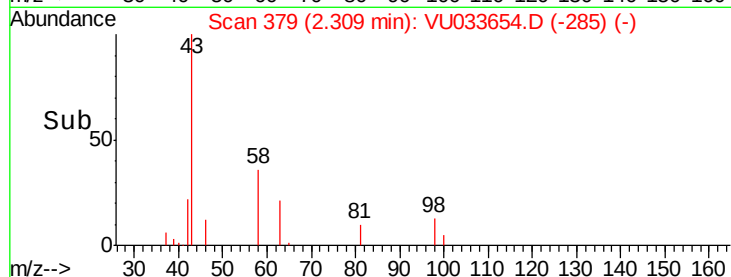

#42

Toluene

Concen: 4.014 ug/L

RT: 7.62 min Scan# 2031

Delta R.T. 0.00 min

Lab File: VU033654.D


Acq: 08 Aug 2019 21:38

Tgt Ion: 91 Resp: 41105

Ion Ratio Lower Upper

91 100

92 58.1 39.6 73.6

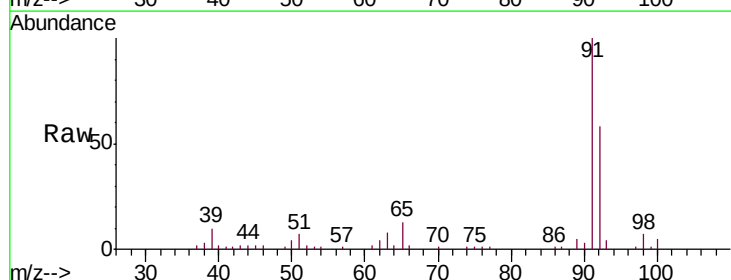

Abundance Ion 91.00 (90.70 to 91.70): VU033634.D (-2016) (-)

Ion 92.00 (91.70 to 92.70): VU033634.D (-2016) (-)



7.62


7.55

7.60

7.65

7.70

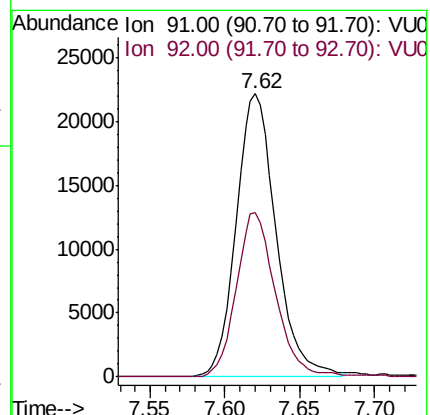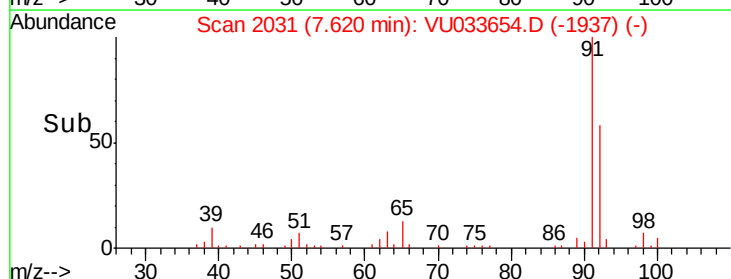

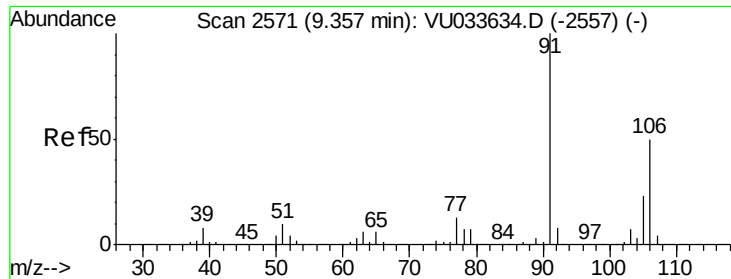

#53
 m,p-Xylene
 Concen: 1.428 ug/L
 RT: 9.36 min Scan# 2572
 Delta R.T. 0.00 min
 Lab File: VU033654.D
 Acq: 08 Aug 2019 21:38

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B25

Tgt Ion:106 Resp: 5955
 Ion Ratio Lower Upper
 106 100
 91 194.3 138.5 257.3

