

Data File : VU033665.D
Acq On : 09 Aug 2019 02:37
Operator : JC/SP
Sample : K4161-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOE8

Quant Time: Aug 09 09:35:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080819WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 09:08:24 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	311341	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	314781	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	144830	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	142506	40.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.10%
7) Chloroethane-d5	1.68	69	125833	42.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.60%
11) 1,1-Dichloroethene-d2	2.26	63	187629	33.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.04%
21) 2-Butanone-d5	4.15	46	220134	85.52	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.52%
24) Chloroform-d	4.62	84	237904	40.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.70%
26) 1,2-Dichloroethane-d4	5.29	65	158224	42.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.26%
32) Benzene-d6	5.32	84	495087	42.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.36%
36) 1,2-Dichloropropane-d6	6.31	67	158592	42.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.98%
41) Toluene-d8	7.55	98	444866	40.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.98%
43) trans-1,3-Dichloropropene-	7.83	79	68504	37.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.00%
47) 2-Hexanone-d5	8.29	63	160364	85.82	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.82%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	242431	41.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.04%
64) 1,2-Dichlorobenzene-d4	11.85	152	171173	43.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.52%


Target Compounds					Qvalue
13) Acetone	2.31	43	4987	2.848 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU033665.D
Acq On : 09 Aug 2019 02:37
Operator : JC/SP
Sample : K4161-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOE8

Quant Time: Aug 09 09:35:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080819WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 09:08:24 2019
Response via : Initial Calibration

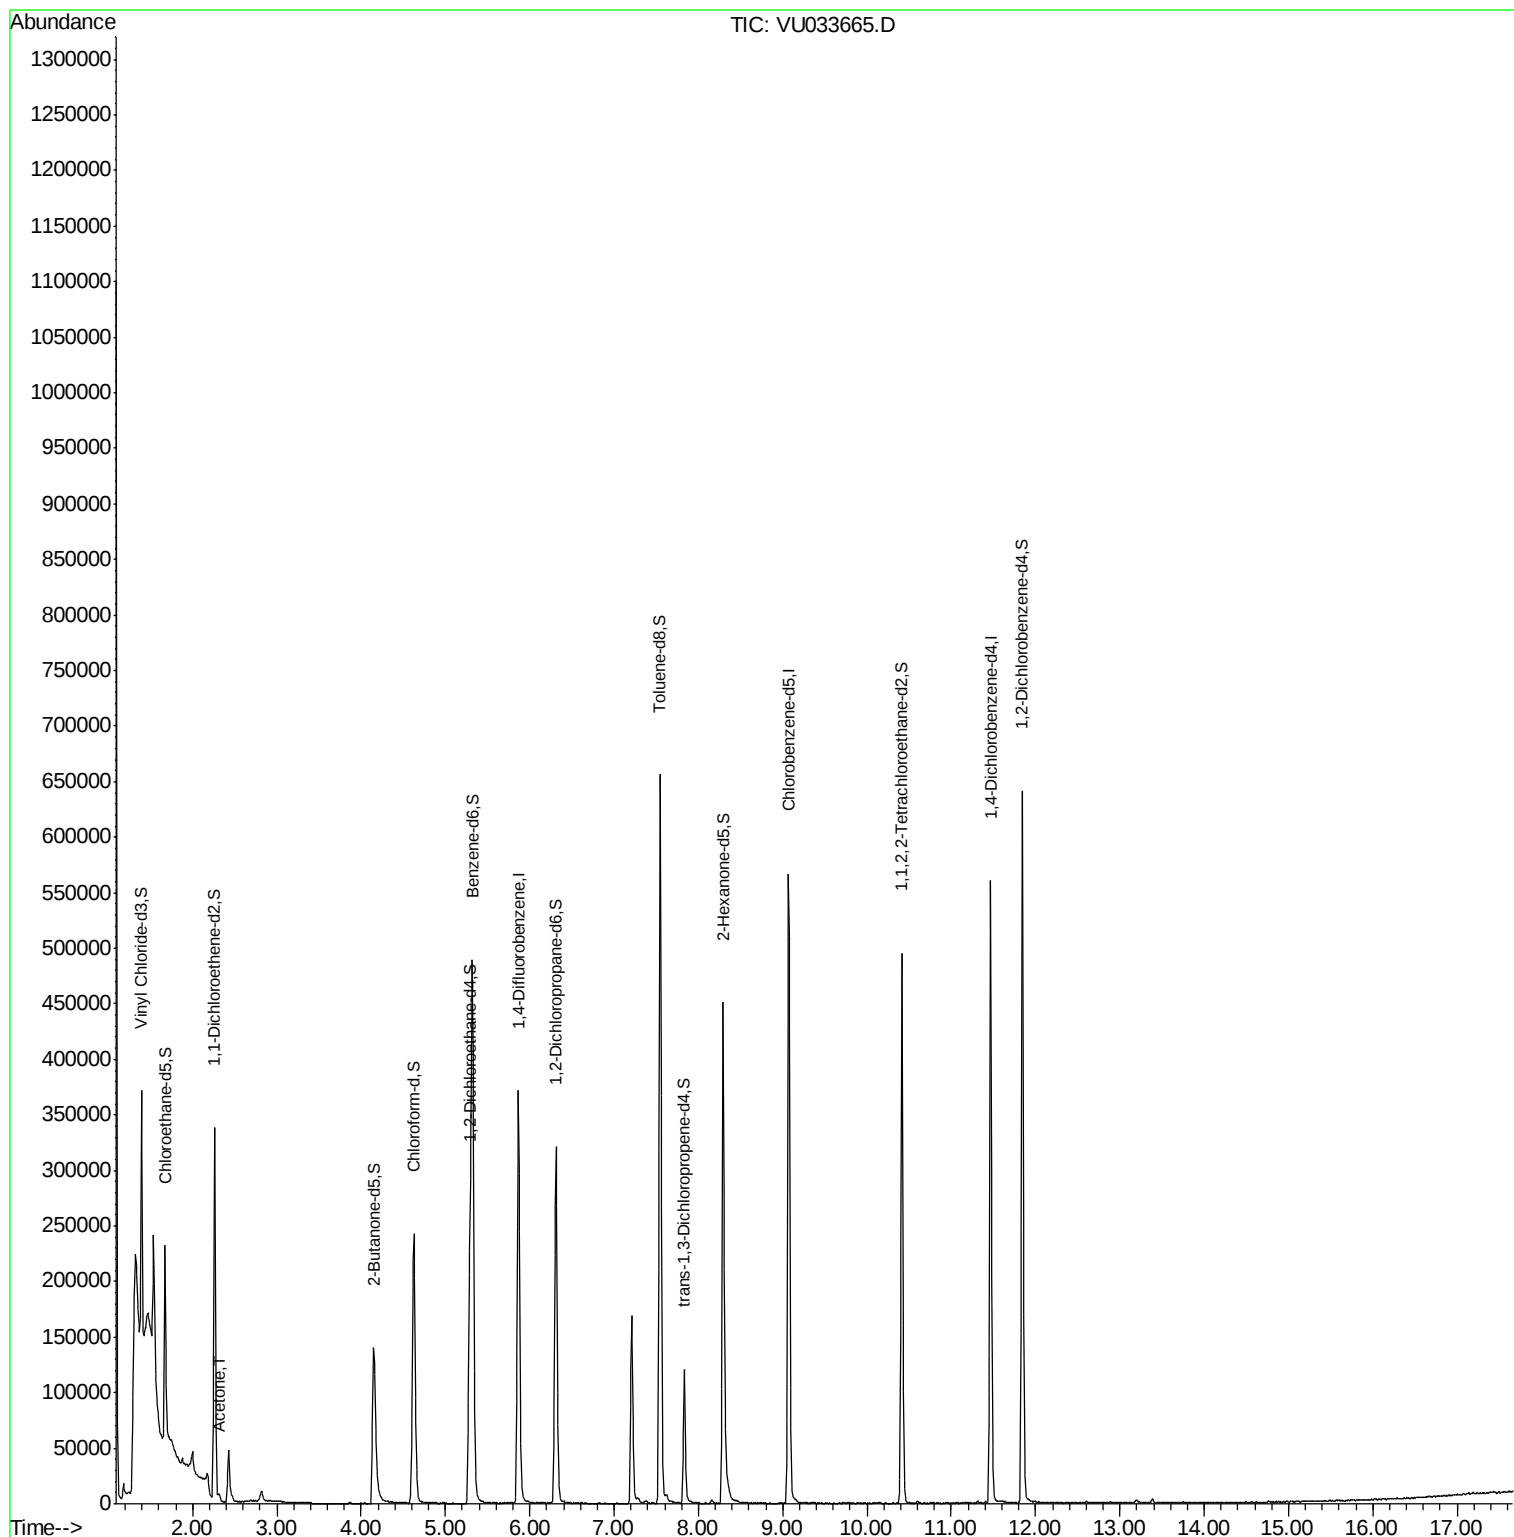

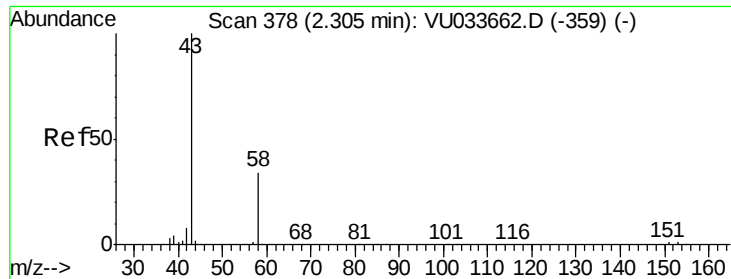

#13

Acetone

Concen: 2.848 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VU033665.D

Acq: 09 Aug 2019 02:37

Instrument :
MSVOA_U
ClientSampleId :
ETOES

Tgt Ion: 43 Resp: 4987

Ion Ratio Lower Upper

43 100

58 32.2 0.0 65.0

