


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081522\
 Data File : VU050331.D
 Acq On : 15 Aug 2022 08:35
 Operator : SY/MD
 Sample : BFB105
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB105

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 16 00:29:27 2022

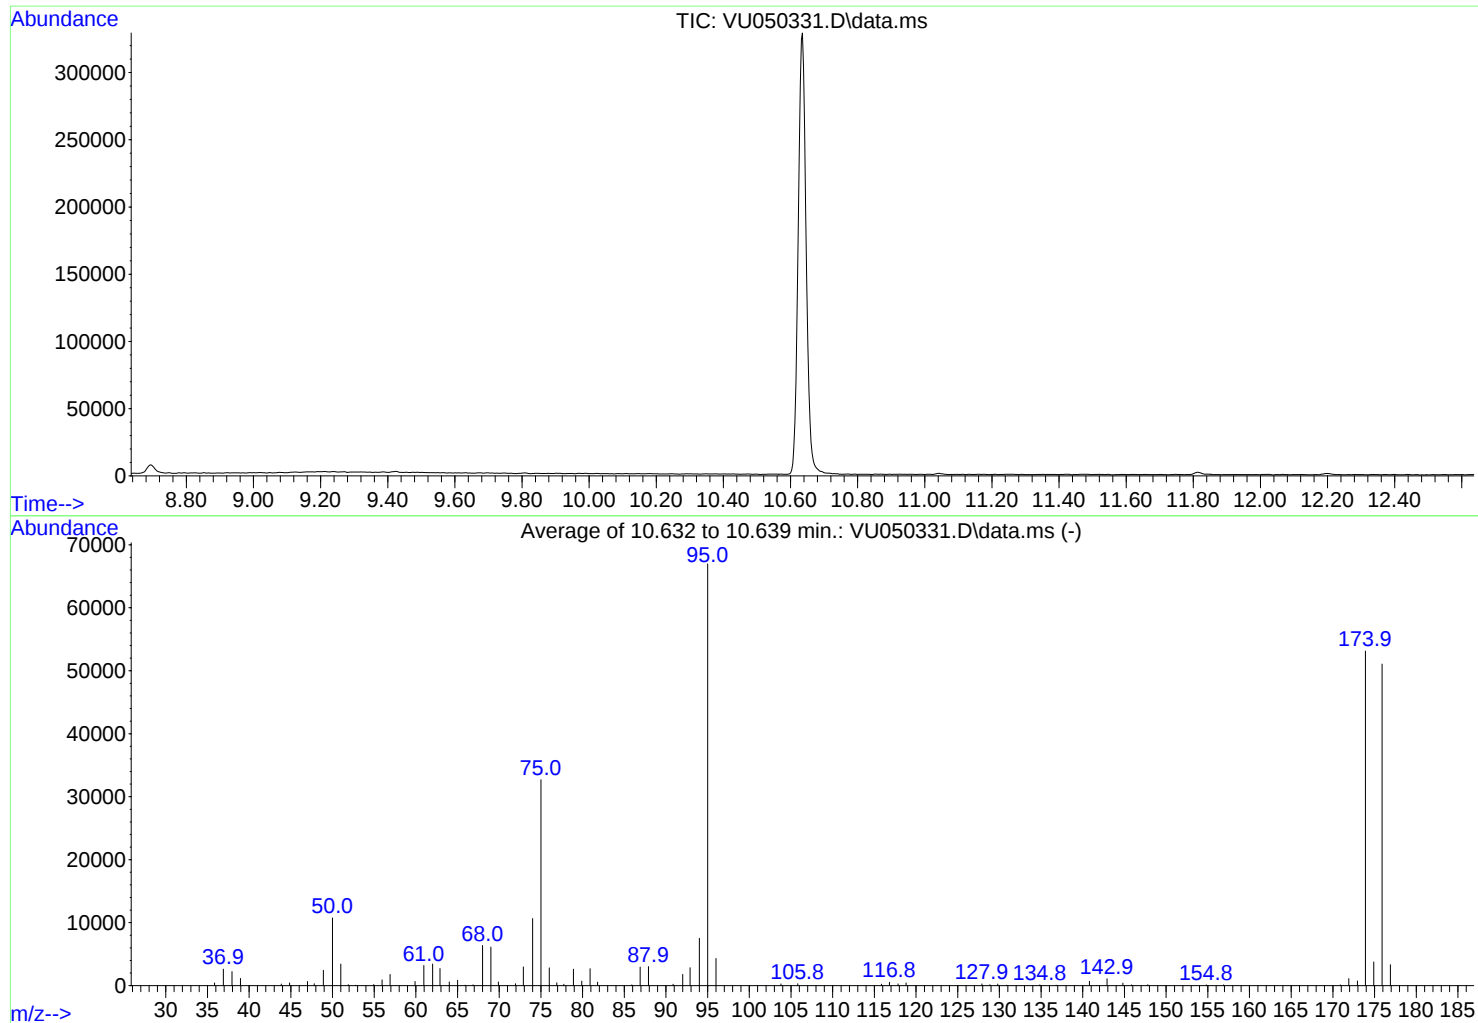

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10752	PASS
75	95	30	80	48.8	32709	PASS
95	95	100	100	100.0	66971	PASS
96	95	5	9	6.5	4334	PASS
173	174	0.00	2	1.4	729	PASS
174	95	50	120	79.3	53128	PASS
175	174	5	9	7.1	3752	PASS
176	174	95	101	96.1	51059	PASS
177	176	5	9	6.5	3331	PASS

m/z	Abundance
35.80	667.0
37.80	218.0
39.80	165.0
43.80	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	1177.0
36.90	2746.0
38.00	2580.0
38.90	1229.0
39.80	195.0
43.90	434.0
44.80	444.0
47.00	742.0
47.80	322.0
48.90	2572.0
50.00	11325.0
51.00	3573.0
51.90	192.0
55.00	175.0
56.00	951.0
56.90	1832.0
59.90	671.0
60.90	3356.0
62.00	3463.0
62.90	2749.0
64.00	583.0
65.00	889.0
66.90	137.0
68.00	6518.0
69.00	6241.0
69.90	603.0
71.90	316.0
72.90	2972.0
74.00	10839.0
75.00	33448.0
76.00	2980.0
76.90	461.0
77.80	220.0
78.90	2699.0
79.90	689.0
80.90	2887.0
81.80	565.0
85.80	143.0
86.90	3033.0
87.90	2977.0
90.80	239.0
92.00	1899.0
92.90	2904.0
94.00	7742.0
95.00	68232.0
96.00	4429.0
103.80	308.0
105.80	313.0
115.80	266.0
116.80	570.0
117.90	288.0
118.80	452.0
127.90	265.0
128.80	154.0
129.80	243.0
130.90	126.0
134.90	150.0
136.80	124.0
140.80	702.0
142.90	1164.0
144.80	440.0
145.80	124.0
147.80	152.0
154.80	146.0
156.90	112.0
170.90	144.0
171.90	1100.0
172.90	657.0
173.90	53064.0
174.90	3843.0
175.90	50944.0
176.90	3468.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	1105.0
36.90	2724.0
38.00	2487.0
38.90	1178.0
39.80	172.0
43.90	451.0
44.90	446.0
47.00	663.0
47.80	303.0
48.90	2547.0
50.00	11050.0
51.00	3501.0
51.90	162.0
52.80	100.0
54.90	182.0
55.90	948.0
56.90	1825.0
59.90	672.0
60.90	3327.0
62.00	3558.0
62.90	2815.0
64.00	612.0
65.00	866.0
65.90	101.0
66.80	144.0
68.00	6581.0
69.00	6274.0
69.90	615.0
72.00	308.0
72.90	3062.0
74.00	11017.0
75.00	33640.0
76.00	2911.0
76.90	500.0
77.70	247.0
78.90	2677.0
79.90	725.0
80.90	2800.0
81.80	583.0
85.90	135.0
86.90	3012.0
87.90	3147.0
90.90	246.0
92.00	1833.0
92.90	2941.0
94.00	7735.0
95.00	69080.0
96.00	4483.0
103.80	296.0
105.80	305.0
115.80	236.0
116.80	553.0
117.80	288.0
118.80	426.0
127.90	289.0
128.90	167.0
129.80	261.0
130.80	122.0
134.90	127.0
136.80	103.0
140.80	710.0
142.90	1153.0
144.80	422.0
145.90	133.0
147.80	143.0
154.70	141.0
156.90	128.0
170.90	147.0
171.90	1164.0
173.00	739.0
173.90	54816.0
174.90	3846.0
175.90	52776.0
176.90	3386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	985.0
36.90	2387.0
38.00	2270.0
39.00	1050.0
40.00	156.0
43.90	439.0
44.90	428.0
47.00	605.0
47.80	304.0
48.90	2206.0
50.00	9881.0
51.00	3232.0
51.90	128.0
52.80	108.0
54.90	177.0
55.90	821.0
56.90	1679.0
59.90	616.0
61.00	2943.0
62.00	3258.0
62.90	2620.0
64.00	563.0
65.00	815.0
65.90	117.0
66.80	134.0
68.00	6029.0
69.00	5853.0
69.90	530.0
71.90	287.0
72.90	2866.0
74.00	10083.0
75.00	31040.0
76.00	2558.0
76.90	426.0
77.80	243.0
78.90	2467.0
79.90	703.0
80.90	2420.0
81.80	535.0
86.00	104.0
86.90	2774.0
87.90	2963.0
90.90	228.0
92.00	1635.0
92.90	2714.0
94.00	7109.0
95.00	63600.0
96.00	4091.0
103.80	255.0
105.80	293.0
115.90	222.0
116.80	484.0
117.80	263.0
118.80	404.0
127.90	263.0
128.90	169.0
129.80	246.0
134.80	105.0
140.80	615.0
141.70	113.0
142.90	988.0
144.80	343.0
145.80	130.0
147.80	142.0
154.90	124.0
156.90	109.0
170.90	131.0
171.90	1111.0
173.00	791.0
173.90	51504.0
174.90	3566.0
175.90	49456.0
176.90	3139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105